

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034697.D
 Acq On : 18 Mar 2024 15:55
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	251310	263636	16.70%	2.302%
2	1.529	145	152	166	rVB	199573	235462	14.91%	2.056%
3	2.059	306	317	335	rBV	407219	605120	38.33%	5.283%
4	2.243	365	374	400	rVB2	13050	34831	2.21%	0.304%
5	2.365	410	412	413	rBV	510	233	0.01%	0.002%
6	2.616	487	490	494	rBV2	180	160	0.01%	0.001%
7	2.728	523	525	528	rBV2	202	140	0.01%	0.001%
8	2.821	549	554	558	rBV2	263	317	0.02%	0.003%
9	2.876	569	571	576	rVB2	222	85	0.01%	0.001%
10	2.899	576	578	580	rBV	272	108	0.01%	0.001%
11	2.940	588	591	593	rBV2	215	146	0.01%	0.001%
12	2.960	593	597	600	rVV	320	253	0.02%	0.002%
13	3.047	621	624	625	rBV	198	102	0.01%	0.001%
14	3.095	638	639	640	rVV	312	118	0.01%	0.001%
15	3.117	643	646	657	rVB3	955	1245	0.08%	0.011%
16	3.188	661	668	671	rBV2	265	307	0.02%	0.003%
17	3.278	695	696	701	rVB	420	170	0.01%	0.001%
18	3.313	701	707	713	rBV	212	218	0.01%	0.002%
19	3.439	739	746	749	rBV2	145	179	0.01%	0.002%
20	3.458	749	752	757	rVV2	222	197	0.01%	0.002%
21	3.715	828	832	836	rBV	203	197	0.01%	0.002%
22	3.786	845	854	902	rBV	121175	366878	23.24%	3.203%
23	4.246	982	997	1028	rBV	245946	630475	39.93%	5.504%
24	4.632	1115	1117	1118	rBV	206	105	0.01%	0.001%
25	4.641	1118	1120	1123	rVV	402	257	0.02%	0.002%
26	4.686	1132	1134	1137	rVB2	234	98	0.01%	0.001%
27	4.702	1137	1139	1142	rVB	206	121	0.01%	0.001%
28	4.722	1142	1145	1150	rBV2	315	343	0.02%	0.003%
29	4.799	1168	1169	1171	rVB	363	125	0.01%	0.001%
30	4.815	1171	1174	1175	rBV2	161	93	0.01%	0.001%
31	4.895	1196	1199	1201	rBV	251	188	0.01%	0.002%
32	4.953	1201	1217	1249	rBV2	598443	1578840	100.00%	13.783%
33	5.349	1337	1340	1343	rVB2	549	281	0.02%	0.002%
34	5.403	1353	1357	1359	rBV2	333	284	0.02%	0.002%
35	5.439	1365	1368	1370	rBV3	293	162	0.01%	0.001%
36	5.490	1382	1384	1386	rVB	224	81	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034697.D
 Acq On : 18 Mar 2024 15:55
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1429	rBV	398860	824621	52.23%	7.199%
38	5.834	1480	1491	1515	rVB7	14398	38310	2.43%	0.334%
39	5.931	1515	1521	1524	rBV2	456	479	0.03%	0.004%
40	5.985	1525	1538	1570	rBV	338751	699444	44.30%	6.106%
41	6.243	1616	1618	1619	rBV	383	155	0.01%	0.001%
42	6.272	1625	1627	1630	rVB2	354	162	0.01%	0.001%
43	6.291	1630	1633	1634	rBV2	264	143	0.01%	0.001%
44	6.304	1634	1637	1641	rVB2	360	261	0.02%	0.002%
45	6.329	1641	1645	1646	rBV2	291	205	0.01%	0.002%
46	6.403	1665	1668	1670	rBV2	340	198	0.01%	0.002%
47	6.436	1676	1678	1682	rBV2	224	126	0.01%	0.001%
48	6.455	1682	1684	1686	rBV	224	98	0.01%	0.001%
49	6.548	1708	1713	1715	rBV2	252	148	0.01%	0.001%
50	6.648	1742	1744	1750	rVB2	116	98	0.01%	0.001%
51	6.699	1754	1760	1763	rBV2	375	315	0.02%	0.003%
52	6.718	1763	1766	1769	rBV	203	147	0.01%	0.001%
53	6.828	1797	1800	1804	rBV2	161	162	0.01%	0.001%
54	6.911	1816	1826	1859	rBV	183509	353143	22.37%	3.083%
55	7.175	1906	1908	1910	rBV2	385	232	0.01%	0.002%
56	7.243	1918	1929	1960	rBV	692995	1223324	77.48%	10.680%
57	7.551	2016	2025	2058	rBV	126118	231575	14.67%	2.022%
58	7.821	2106	2109	2112	rVV3	336	219	0.01%	0.002%
59	7.953	2146	2150	2151	rBV	224	141	0.01%	0.001%
60	8.024	2163	2172	2213	rBV	381683	706183	44.73%	6.165%
61	8.464	2307	2309	2312	rVB3	243	116	0.01%	0.001%
62	8.660	2368	2370	2372	rVB2	232	101	0.01%	0.001%
63	8.673	2372	2374	2375	rBV	287	122	0.01%	0.001%
64	8.709	2381	2385	2389	rBV3	233	187	0.01%	0.002%
65	8.747	2395	2397	2398	rBV	300	143	0.01%	0.001%
66	8.783	2398	2408	2430	rBV	587659	981388	62.16%	8.568%
67	9.024	2481	2483	2484	rBV	251	87	0.01%	0.001%
68	9.120	2511	2513	2518	rBV3	247	218	0.01%	0.002%
69	9.162	2523	2526	2528	rVB	326	180	0.01%	0.002%
70	9.355	2583	2586	2588	rBV	144	96	0.01%	0.001%
71	9.484	2621	2626	2630	rBV2	324	382	0.02%	0.003%
72	9.548	2642	2646	2648	rBV2	223	160	0.01%	0.001%
73	9.577	2652	2655	2660	rVB2	273	248	0.02%	0.002%
74	9.747	2704	2708	2712	rBV2	241	248	0.02%	0.002%
75	9.805	2724	2726	2729	rVB2	245	122	0.01%	0.001%
76	9.828	2729	2733	2734	rBV2	195	138	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034697.D
 Acq On : 18 Mar 2024 15:55
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.963	2773	2775	2779	rVB2	283	125	0.01%	0.001%
78	9.988	2779	2783	2787	rVB	169	110	0.01%	0.001%
79	10.017	2787	2792	2794	rBV2	275	211	0.01%	0.002%
80	10.056	2801	2804	2808	rBV2	212	182	0.01%	0.002%
81	10.152	2822	2834	2856	rBV	444040	705734	44.70%	6.161%
82	10.329	2881	2889	2896	rVB5	1664	2761	0.17%	0.024%
83	10.377	2900	2904	2905	rBV2	267	132	0.01%	0.001%
84	10.416	2913	2916	2917	rBV	195	120	0.01%	0.001%
85	10.458	2926	2929	2931	rBV2	230	159	0.01%	0.001%
86	10.516	2944	2947	2948	rBV	186	93	0.01%	0.001%
87	10.586	2967	2969	2973	rVB2	282	124	0.01%	0.001%
88	10.705	3004	3006	3008	rBV2	170	104	0.01%	0.001%
89	10.783	3024	3030	3032	rBV2	267	209	0.01%	0.002%
90	10.950	3078	3082	3087	rBV2	413	348	0.02%	0.003%
91	10.979	3087	3091	3092	rBV2	193	148	0.01%	0.001%
92	11.123	3134	3136	3139	rBV	218	124	0.01%	0.001%
93	11.185	3144	3155	3180	rBV	574206	902221	57.14%	7.876%
94	11.451	3236	3238	3242	rVB	439	203	0.01%	0.002%
95	11.561	3259	3272	3293	rBV	661051	1054999	66.82%	9.210%
96	11.837	3354	3358	3360	rBV	418	322	0.02%	0.003%
97	12.570	3583	3586	3589	rBV2	244	187	0.01%	0.002%
98	12.786	3651	3653	3657	rBV2	335	254	0.02%	0.002%
99	12.992	3714	3717	3720	rBV2	452	225	0.01%	0.002%
100	13.204	3782	3783	3784	rBV	620	193	0.01%	0.002%




Sum of corrected areas: 11454668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034697.D
Acq On : 18 Mar 2024 15:55
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

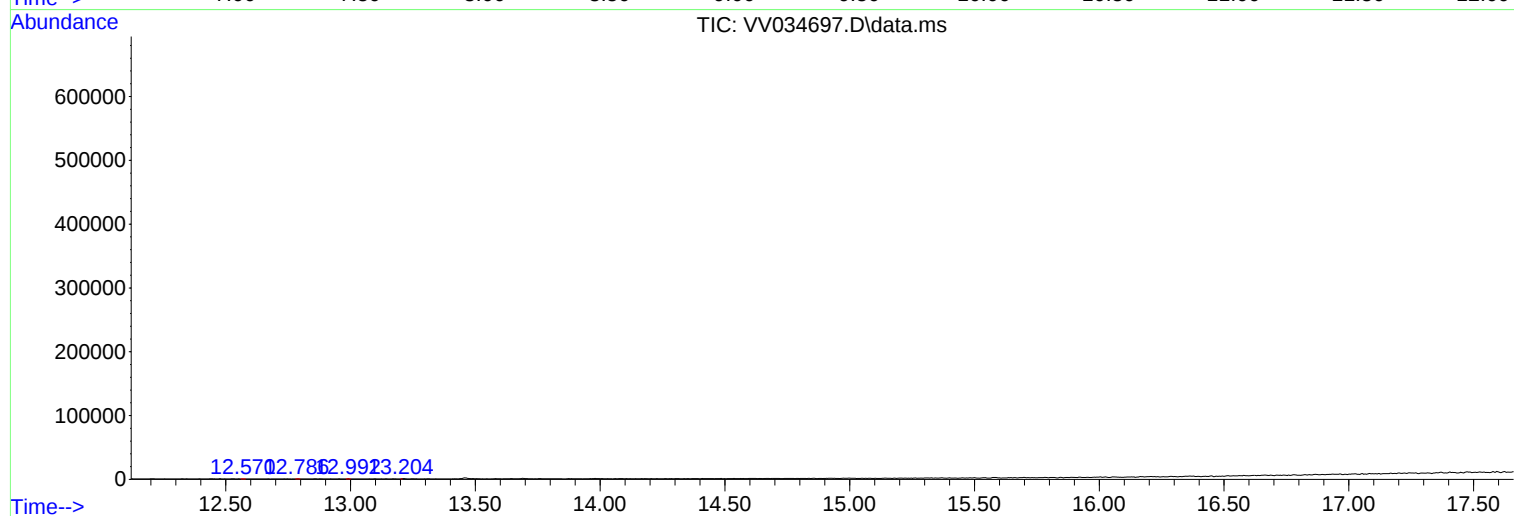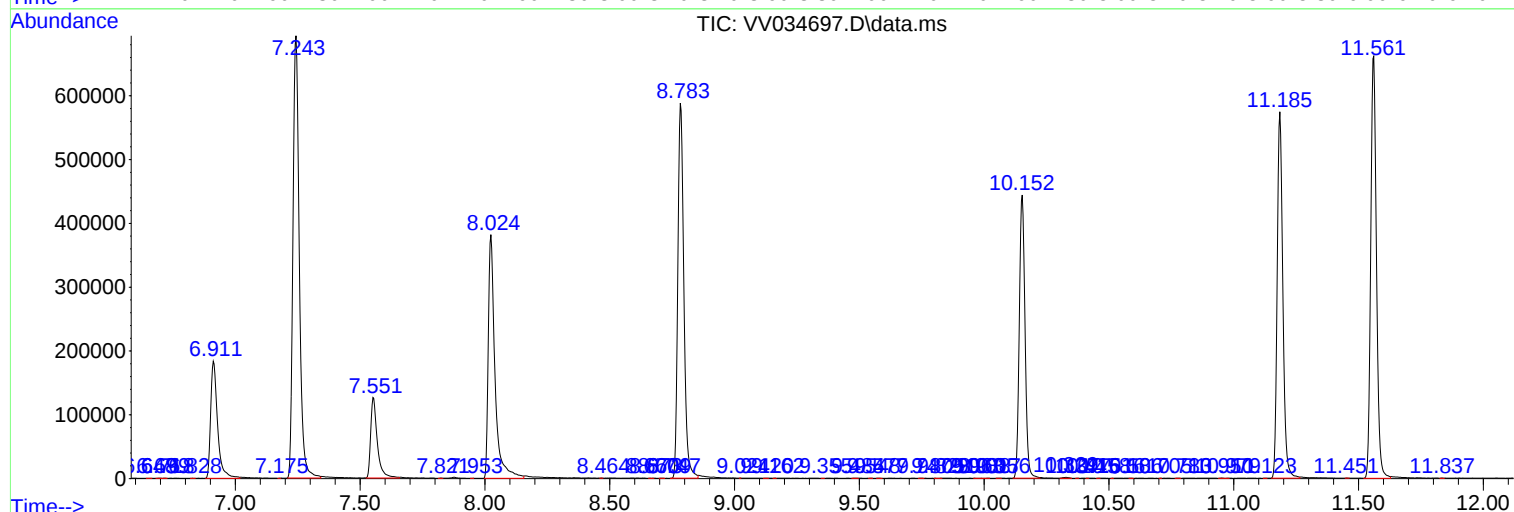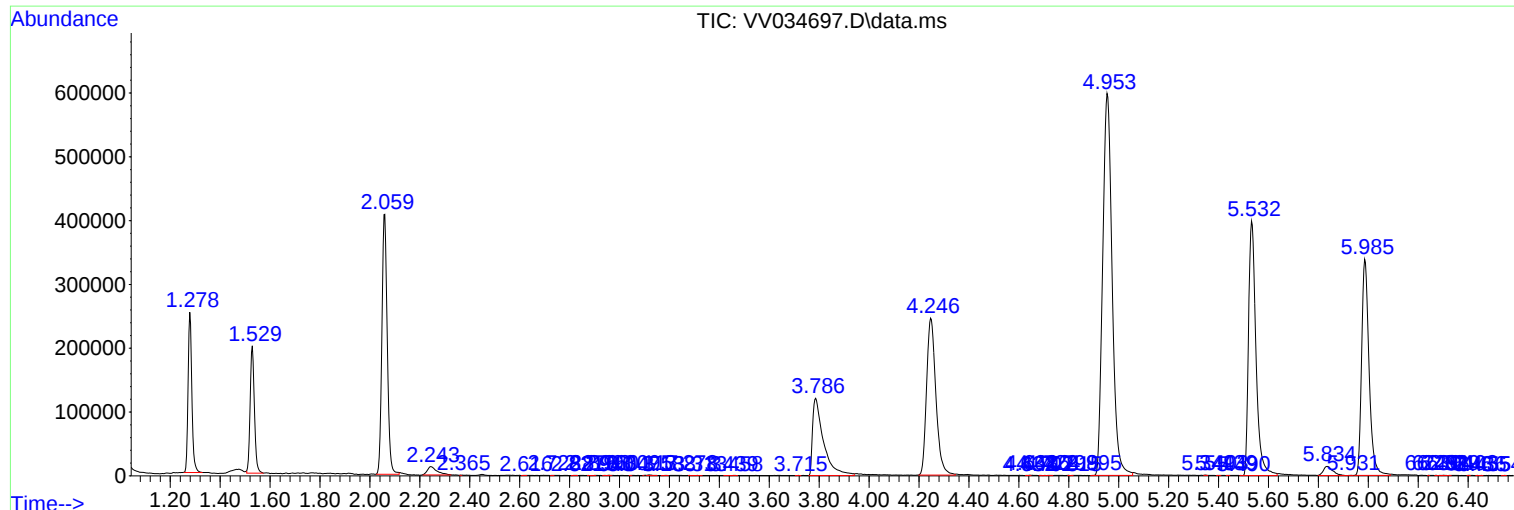

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034697.D
Acq On : 18 Mar 2024 15:55
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034697.D
Acq On : 18 Mar 2024 15:55
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc