

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034698.D
 Acq On : 18 Mar 2024 16:19
 Operator : SY/MD
 Sample : P1739-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	236650	244411	16.14%	2.248%
2	1.529	145	152	171	rVB	187490	222648	14.70%	2.048%
3	2.059	306	317	333	rBV	373251	547586	36.16%	5.036%
4	2.349	404	407	411	rBV3	409	330	0.02%	0.003%
5	2.387	417	419	421	rBV	261	128	0.01%	0.001%
6	2.449	431	438	447	rVB4	2616	3709	0.24%	0.034%
7	2.506	454	456	458	rBV	187	90	0.01%	0.001%
8	2.548	465	469	472	rBV	735	616	0.04%	0.006%
9	2.709	516	519	521	rBV2	248	157	0.01%	0.001%
10	2.867	558	568	572	rBV2	237	439	0.03%	0.004%
11	2.947	590	593	595	rVB2	201	87	0.01%	0.001%
12	3.031	617	619	621	rBV2	141	73	0.00%	0.001%
13	3.108	641	643	647	rVB2	132	61	0.00%	0.001%
14	3.188	663	668	673	rBV2	266	286	0.02%	0.003%
15	3.236	680	683	687	rBV2	170	130	0.01%	0.001%
16	3.259	687	690	691	rBV	189	111	0.01%	0.001%
17	3.320	707	709	710	rBV	191	46	0.00%	0.000%
18	3.336	710	714	716	rBV	185	158	0.01%	0.001%
19	3.416	735	739	740	rBV	243	154	0.01%	0.001%
20	3.442	744	747	752	rVV2	216	197	0.01%	0.002%
21	3.481	755	759	764	rBV	215	258	0.02%	0.002%
22	3.577	786	789	795	rVB	237	151	0.01%	0.001%
23	3.609	795	799	801	rBV	251	204	0.01%	0.002%
24	3.648	808	811	814	rBV	218	163	0.01%	0.001%
25	3.670	815	818	821	rVV2	156	121	0.01%	0.001%
26	3.715	829	832	837	rBV2	230	222	0.01%	0.002%
27	3.786	846	854	895	rBV	118748	332272	21.94%	3.056%
28	4.249	983	998	1030	rBV	236837	598264	39.51%	5.502%
29	4.757	1154	1156	1158	rBV	226	115	0.01%	0.001%
30	4.786	1161	1165	1169	rBV2	249	251	0.02%	0.002%
31	4.844	1181	1183	1188	rBV2	383	289	0.02%	0.003%
32	4.953	1199	1217	1257	rBV2	568449	1514174	100.00%	13.925%
33	5.403	1355	1357	1360	rVB2	272	109	0.01%	0.001%
34	5.419	1360	1362	1363	rBV2	296	136	0.01%	0.001%
35	5.532	1387	1397	1447	rBV	374456	774204	51.13%	7.120%
36	5.837	1480	1492	1511	rVB3	10787	24733	1.63%	0.227%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034698.D
 Acq On : 18 Mar 2024 16:19
 Operator : SY/MD
 Sample : P1739-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.985	1526	1538	1569	rBV	324878	679395	44.87%	6.248%
38	6.284	1628	1631	1633	rBV2	432	262	0.02%	0.002%
39	6.300	1633	1636	1639	rVV3	249	217	0.01%	0.002%
40	6.352	1650	1652	1656	rBV	256	183	0.01%	0.002%
41	6.439	1671	1679	1681	rBV2	214	209	0.01%	0.002%
42	6.458	1683	1685	1689	rVB	222	104	0.01%	0.001%
43	6.481	1689	1692	1695	rBV2	190	163	0.01%	0.001%
44	6.567	1716	1719	1725	rVB2	360	313	0.02%	0.003%
45	6.599	1725	1729	1732	rVB	270	156	0.01%	0.001%
46	6.625	1732	1737	1740	rBV2	228	233	0.02%	0.002%
47	6.645	1740	1743	1745	rBV	196	144	0.01%	0.001%
48	6.821	1796	1798	1800	rBV	213	103	0.01%	0.001%
49	6.911	1816	1826	1848	rBV	175712	332214	21.94%	3.055%
50	7.243	1918	1929	1961	rBV	662267	1164275	76.89%	10.707%
51	7.554	2016	2026	2054	rBV	120922	223358	14.75%	2.054%
52	7.773	2092	2094	2099	rBV2	417	432	0.03%	0.004%
53	7.844	2113	2116	2120	rBV	169	122	0.01%	0.001%
54	7.882	2120	2128	2129	rBV3	634	639	0.04%	0.006%
55	7.927	2140	2142	2144	rBV	187	119	0.01%	0.001%
56	7.963	2151	2153	2158	rVB	311	165	0.01%	0.002%
57	8.024	2163	2172	2214	rBV	370916	709491	46.86%	6.525%
58	8.458	2304	2307	2309	rBV2	365	244	0.02%	0.002%
59	8.509	2319	2323	2325	rBV3	400	280	0.02%	0.003%
60	8.545	2333	2334	2337	rBV	239	130	0.01%	0.001%
61	8.561	2337	2339	2341	rBV2	291	147	0.01%	0.001%
62	8.625	2353	2359	2362	rBV2	376	370	0.02%	0.003%
63	8.699	2381	2382	2384	rBV	203	105	0.01%	0.001%
64	8.744	2394	2396	2398	rBV	216	84	0.01%	0.001%
65	8.783	2398	2408	2436	rBV	571724	934746	61.73%	8.596%
66	9.149	2520	2522	2526	rVB2	226	158	0.01%	0.001%
67	9.175	2527	2530	2532	rBV2	215	137	0.01%	0.001%
68	9.223	2543	2545	2548	rVB2	348	167	0.01%	0.002%
69	9.252	2551	2554	2556	rBV	197	114	0.01%	0.001%
70	9.300	2564	2569	2571	rBV	190	181	0.01%	0.002%
71	9.316	2571	2574	2576	rVV2	305	212	0.01%	0.002%
72	9.345	2579	2583	2585	rBV2	239	196	0.01%	0.002%
73	9.419	2604	2606	2610	rBV	175	93	0.01%	0.001%
74	9.477	2622	2624	2629	rVB	585	292	0.02%	0.003%
75	9.744	2705	2707	2710	rBV	233	104	0.01%	0.001%
76	9.956	2772	2773	2774	rBV	108	27	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034698.D
 Acq On : 18 Mar 2024 16:19
 Operator : SY/MD
 Sample : P1739-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.969	2774	2777	2782	rVB2	188	158	0.01%	0.001%
78	9.995	2782	2785	2786	rBV2	122	78	0.01%	0.001%
79	10.152	2822	2834	2857	rBV	438721	684641	45.22%	6.296%
80	10.265	2867	2869	2872	rBV	356	211	0.01%	0.002%
81	10.384	2904	2906	2910	rBV3	250	185	0.01%	0.002%
82	10.676	2994	2997	2999	rBV2	320	164	0.01%	0.002%
83	10.754	3018	3021	3022	rBV	224	127	0.01%	0.001%
84	10.792	3031	3033	3036	rVB2	393	205	0.01%	0.002%
85	10.812	3036	3039	3041	rBV2	149	81	0.01%	0.001%
86	10.911	3067	3070	3073	rBV2	205	144	0.01%	0.001%
87	11.130	3136	3138	3142	rVB	310	148	0.01%	0.001%
88	11.185	3144	3155	3183	rBV	545108	856442	56.56%	7.876%
89	11.419	3225	3228	3230	rBV2	417	221	0.01%	0.002%
90	11.464	3240	3242	3245	rBV2	204	95	0.01%	0.001%
91	11.561	3260	3272	3296	rBV	639931	1011545	66.81%	9.302%
92	12.111	3439	3443	3449	rVB3	381	331	0.02%	0.003%
93	12.873	3678	3680	3683	rVB	463	237	0.02%	0.002%
94	12.889	3683	3685	3691	rBV2	292	266	0.02%	0.002%
95	13.197	3777	3781	3783	rBV3	465	340	0.02%	0.003%
96	13.265	3796	3802	3804	rBV2	499	487	0.03%	0.004%
97	13.815	3969	3973	3978	rBV	563	655	0.04%	0.006%




Sum of corrected areas: 10873928

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034698.D
Acq On : 18 Mar 2024 16:19
Operator : SY/MD
Sample : P1739-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

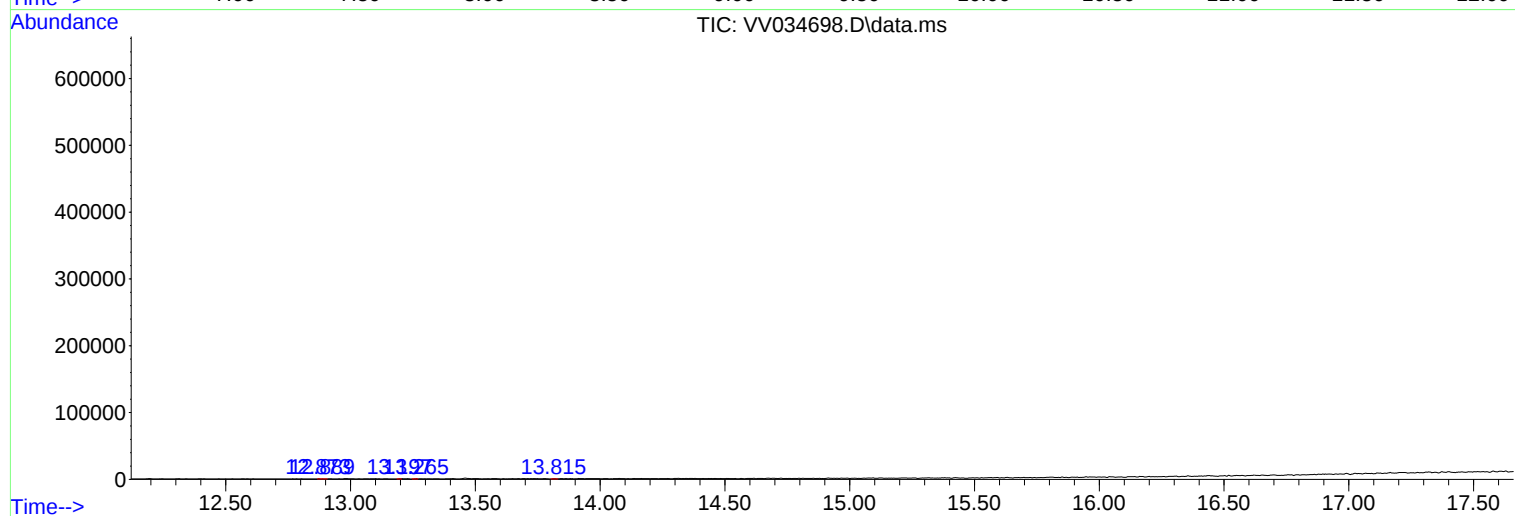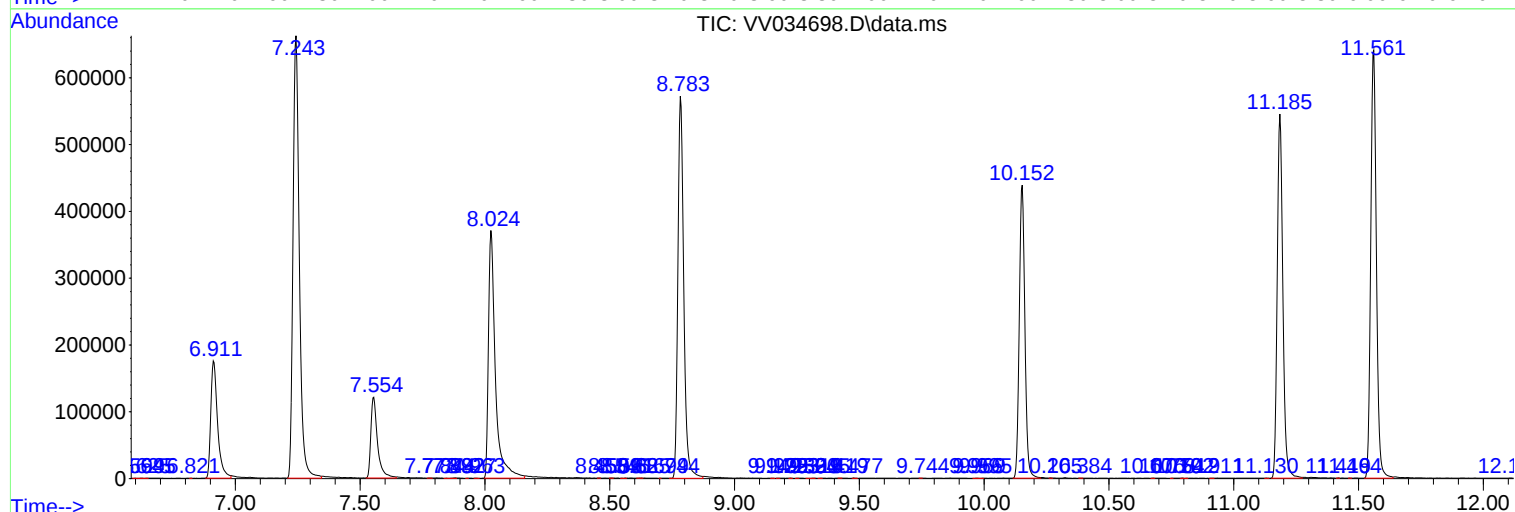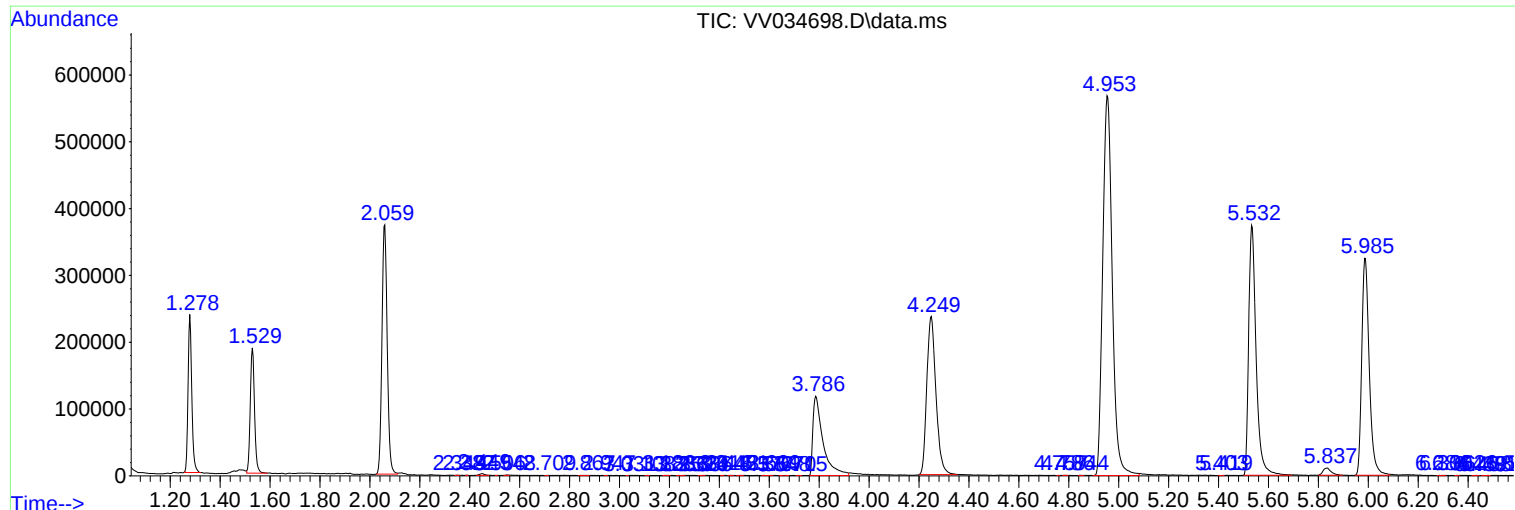

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034698.D
Acq On : 18 Mar 2024 16:19
Operator : SY/MD
Sample : P1739-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034698.D
Acq On : 18 Mar 2024 16:19
Operator : SY/MD
Sample : P1739-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc