

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034708.D
 Acq On : 18 Mar 2024 20:19
 Operator : SY/MD
 Sample : P1766-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	241481	256799	17.16%	2.340%
2	1.529	145	152	171	rVB	194399	231545	15.47%	2.110%
3	2.060	306	317	330	rBV	386625	566424	37.84%	5.161%
4	2.249	367	376	394	rBV2	10925	30342	2.03%	0.276%
5	2.446	433	437	446	rVB6	801	1058	0.07%	0.010%
6	2.966	596	599	601	rBV	159	106	0.01%	0.001%
7	3.040	619	622	626	rBV2	340	217	0.01%	0.002%
8	3.130	647	650	654	rBV	233	152	0.01%	0.001%
9	3.172	659	663	666	rVB	288	221	0.01%	0.002%
10	3.195	666	670	673	rBV2	229	217	0.01%	0.002%
11	3.253	686	688	690	rVB	263	108	0.01%	0.001%
12	3.288	696	699	701	rBV	154	96	0.01%	0.001%
13	3.368	720	724	729	rVB2	281	244	0.02%	0.002%
14	3.471	750	756	760	rBV3	475	460	0.03%	0.004%
15	3.523	769	772	775	rVB2	184	96	0.01%	0.001%
16	3.539	775	777	779	rBV	153	97	0.01%	0.001%
17	3.597	793	795	798	rBV	187	107	0.01%	0.001%
18	3.619	798	802	804	rVV2	197	142	0.01%	0.001%
19	3.748	839	842	844	rBV2	131	103	0.01%	0.001%
20	3.786	845	854	899	rBV2	122957	384311	25.68%	3.502%
21	4.185	976	978	981	rBV3	449	325	0.02%	0.003%
22	4.249	982	998	1025	rVV	234110	606350	40.51%	5.525%
23	4.561	1090	1095	1098	rVB3	278	286	0.02%	0.003%
24	4.619	1108	1113	1116	rBV3	343	370	0.02%	0.003%
25	4.683	1128	1133	1139	rVB3	246	306	0.02%	0.003%
26	4.738	1141	1150	1153	rBV3	397	642	0.04%	0.006%
27	4.957	1201	1218	1249	rBV2	564949	1496777	100.00%	13.639%
28	5.297	1320	1324	1327	rBV	491	384	0.03%	0.003%
29	5.388	1349	1352	1353	rBV	340	189	0.01%	0.002%
30	5.426	1362	1364	1366	rBV2	269	132	0.01%	0.001%
31	5.532	1386	1397	1434	rBV	384691	791644	52.89%	7.214%
32	5.834	1484	1491	1511	rVB6	8500	19716	1.32%	0.180%
33	5.905	1511	1513	1516	rVB3	431	230	0.02%	0.002%
34	5.986	1525	1538	1560	rBV	316717	660308	44.12%	6.017%
35	6.243	1614	1618	1619	rBV2	211	144	0.01%	0.001%
36	6.297	1632	1635	1638	rVB2	149	98	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034708.D
 Acq On : 18 Mar 2024 20:19
 Operator : SY/MD
 Sample : P1766-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.317	1638	1641	1645	rVB	358	222	0.01%	0.002%
38	6.580	1720	1723	1727	rVB2	195	142	0.01%	0.001%
39	6.751	1774	1776	1780	rVB3	266	160	0.01%	0.001%
40	6.809	1789	1794	1797	rBV	258	251	0.02%	0.002%
41	6.912	1816	1826	1857	rBV	169773	326325	21.80%	2.974%
42	7.243	1917	1929	1957	rBV	658773	1174770	78.49%	10.705%
43	7.551	2016	2025	2053	rBV	116755	215147	14.37%	1.960%
44	7.805	2100	2104	2105	rBV	283	201	0.01%	0.002%
45	7.834	2112	2113	2115	rVB	387	120	0.01%	0.001%
46	7.857	2115	2120	2121	rBV2	501	366	0.02%	0.003%
47	7.915	2137	2138	2141	rBV	192	105	0.01%	0.001%
48	7.966	2151	2154	2158	rBV2	190	191	0.01%	0.002%
49	8.024	2163	2172	2214	rBV	351554	680854	45.49%	6.204%
50	8.548	2332	2335	2336	rBV2	374	188	0.01%	0.002%
51	8.558	2336	2338	2340	rVV2	315	146	0.01%	0.001%
52	8.603	2350	2352	2354	rVB	218	91	0.01%	0.001%
53	8.619	2356	2357	2362	rVB3	464	314	0.02%	0.003%
54	8.645	2362	2365	2366	rBV	247	126	0.01%	0.001%
55	8.654	2366	2368	2372	rVB	403	236	0.02%	0.002%
56	8.677	2372	2375	2377	rBV2	158	99	0.01%	0.001%
57	8.783	2397	2408	2440	rBV	571073	955432	63.83%	8.706%
58	9.027	2481	2484	2488	rBV4	332	300	0.02%	0.003%
59	9.085	2497	2502	2505	rVV	443	378	0.03%	0.003%
60	9.201	2535	2538	2541	rBV2	363	229	0.02%	0.002%
61	9.297	2561	2568	2574	rBV2	366	366	0.02%	0.003%
62	9.426	2605	2608	2610	rBV	268	137	0.01%	0.001%
63	9.465	2617	2620	2621	rBV	228	115	0.01%	0.001%
64	9.474	2621	2623	2627	rVB	193	89	0.01%	0.001%
65	9.593	2658	2660	2664	rVB2	261	129	0.01%	0.001%
66	9.619	2664	2668	2673	rVB2	373	327	0.02%	0.003%
67	9.648	2673	2677	2680	rBV2	144	110	0.01%	0.001%
68	9.773	2712	2716	2717	rBV	199	115	0.01%	0.001%
69	9.905	2754	2757	2759	rBV	245	139	0.01%	0.001%
70	9.979	2778	2780	2782	rBV	191	99	0.01%	0.001%
71	10.153	2822	2834	2857	rBV	430097	680610	45.47%	6.202%
72	10.288	2873	2876	2880	rVB3	450	259	0.02%	0.002%
73	10.416	2915	2916	2918	rVB	394	127	0.01%	0.001%
74	10.432	2918	2921	2924	rBV	166	110	0.01%	0.001%
75	10.632	2980	2983	2986	rBV2	138	117	0.01%	0.001%
76	10.747	3011	3019	3022	rBV2	286	343	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034708.D
 Acq On : 18 Mar 2024 20:19
 Operator : SY/MD
 Sample : P1766-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.767	3023	3025	3027	rVV2	331	151	0.01%	0.001%
78	10.789	3030	3032	3036	rVB2	241	129	0.01%	0.001%
79	10.821	3039	3042	3044	rBV	193	134	0.01%	0.001%
80	10.934	3074	3077	3079	rBV2	166	107	0.01%	0.001%
81	11.091	3123	3126	3128	rBV2	195	123	0.01%	0.001%
82	11.136	3137	3140	3143	rBV2	214	146	0.01%	0.001%
83	11.185	3143	3155	3184	rBV	556948	867476	57.96%	7.905%
84	11.490	3248	3250	3251	rBV	271	125	0.01%	0.001%
85	11.561	3259	3272	3298	rBV	639490	1012512	67.65%	9.226%
86	11.812	3347	3350	3352	rBV	214	100	0.01%	0.001%
87	11.831	3353	3356	3363	rVB3	365	429	0.03%	0.004%
88	11.902	3375	3378	3380	rBV2	181	132	0.01%	0.001%
89	11.963	3395	3397	3398	rBV2	290	121	0.01%	0.001%
90	12.156	3455	3457	3462	rBV2	212	141	0.01%	0.001%
91	12.284	3495	3497	3500	rBV2	272	131	0.01%	0.001%
92	12.448	3546	3548	3550	rVB	318	89	0.01%	0.001%
93	12.480	3556	3558	3560	rVB2	430	123	0.01%	0.001%
94	12.500	3561	3564	3566	rBV	285	211	0.01%	0.002%
95	12.628	3601	3604	3609	rVB3	406	284	0.02%	0.003%
96	12.661	3610	3614	3616	rBV	473	358	0.02%	0.003%
97	12.728	3631	3635	3637	rBV2	297	255	0.02%	0.002%
98	13.146	3761	3765	3767	rBV	348	278	0.02%	0.003%
99	13.223	3787	3789	3796	rVB2	317	349	0.02%	0.003%
100	13.509	3875	3878	3879	rBV	330	169	0.01%	0.002%




Sum of corrected areas: 10974404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034708.D
Acq On : 18 Mar 2024 20:19
Operator : SY/MD
Sample : P1766-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COGM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

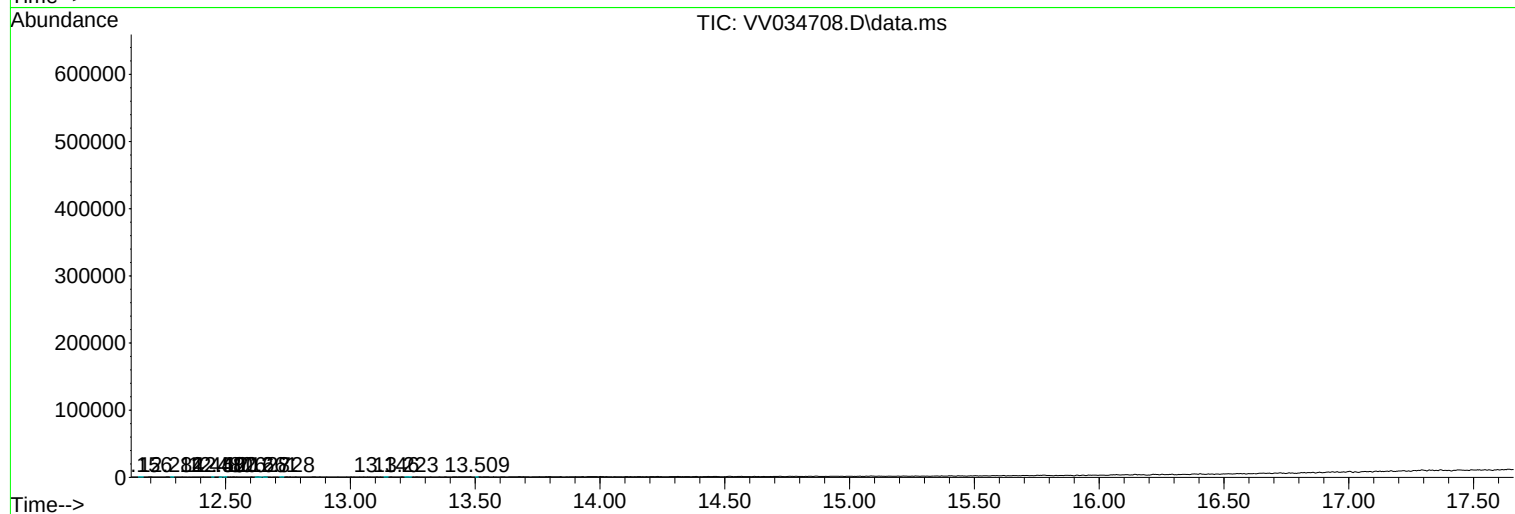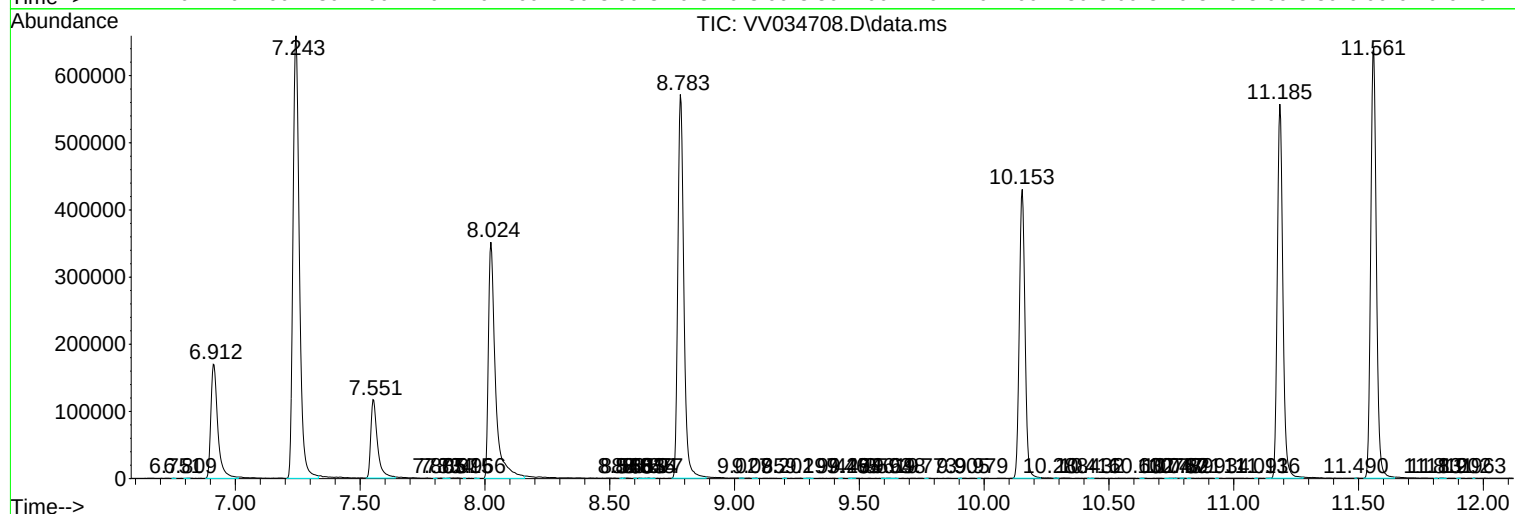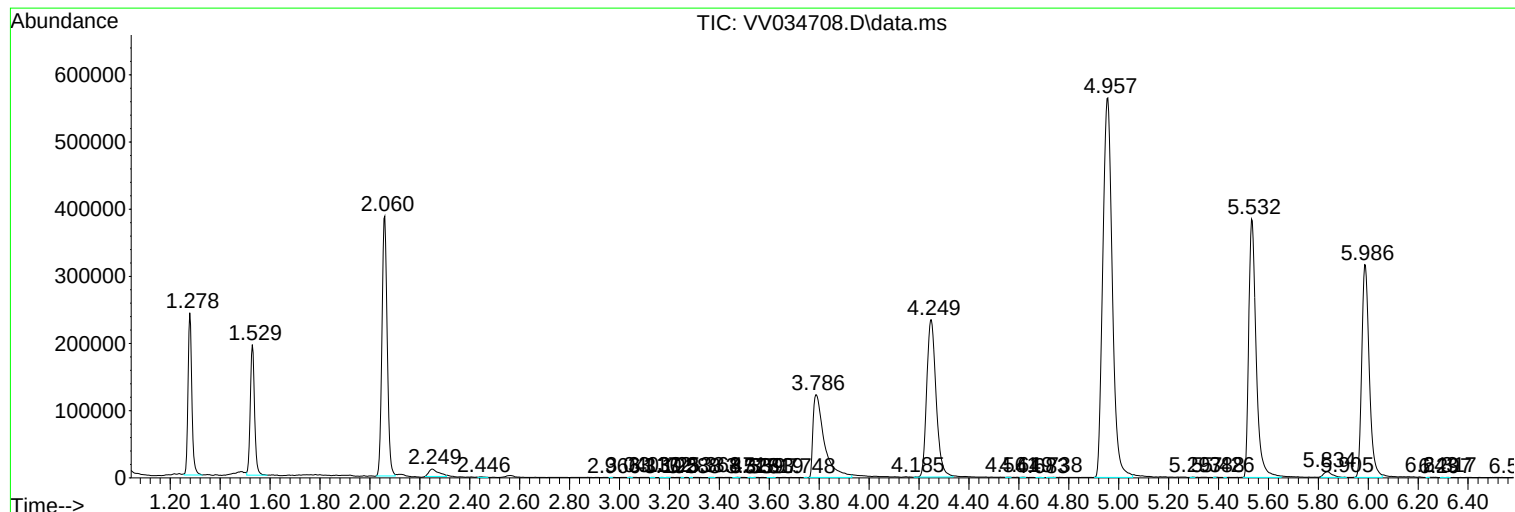

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034708.D
Acq On : 18 Mar 2024 20:19
Operator : SY/MD
Sample : P1766-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034708.D
Acq On : 18 Mar 2024 20:19
Operator : SY/MD
Sample : P1766-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc