

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034714.D
 Acq On : 18 Mar 2024 22:43
 Operator : SY/MD
 Sample : P1766-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	238907	253071	16.17%	2.219%
2	1.532	146	153	169	rVB	196906	235493	15.05%	2.065%
3	2.060	306	317	337	rBV	394261	582416	37.22%	5.107%
4	2.484	447	449	452	rBV2	334	234	0.01%	0.002%
5	2.693	510	514	517	rBV2	165	125	0.01%	0.001%
6	2.715	517	521	525	rVB2	326	239	0.02%	0.002%
7	2.786	537	543	545	rBV2	205	228	0.01%	0.002%
8	2.799	545	547	553	rVB	246	144	0.01%	0.001%
9	2.902	576	579	582	rBV	226	143	0.01%	0.001%
10	3.027	612	618	621	rBV3	280	296	0.02%	0.003%
11	3.088	634	637	641	rVB2	121	105	0.01%	0.001%
12	3.108	641	643	646	rBV2	204	142	0.01%	0.001%
13	3.201	666	672	677	rBV2	170	235	0.02%	0.002%
14	3.384	727	729	733	rVB	213	131	0.01%	0.001%
15	3.487	756	761	763	rBV	205	157	0.01%	0.001%
16	3.503	764	766	770	rVB	232	114	0.01%	0.001%
17	3.564	782	785	789	rBV2	107	105	0.01%	0.001%
18	3.789	846	855	892	rBV	120612	376143	24.04%	3.298%
19	4.246	982	997	1037	rBV	241364	623939	39.88%	5.471%
20	4.516	1071	1081	1095	rVB6	2014	4988	0.32%	0.044%
21	4.667	1123	1128	1135	rVB2	288	374	0.02%	0.003%
22	4.696	1135	1137	1139	rBV2	346	199	0.01%	0.002%
23	4.838	1175	1181	1188	rBV3	306	462	0.03%	0.004%
24	4.879	1192	1194	1197	rBV2	278	172	0.01%	0.002%
25	4.953	1202	1217	1265	rBV2	584074	1564648	100.00%	13.721%
26	5.346	1337	1339	1341	rBV2	258	129	0.01%	0.001%
27	5.461	1372	1375	1378	rBV2	252	145	0.01%	0.001%
28	5.532	1386	1397	1431	rBV	386236	816094	52.16%	7.157%
29	5.838	1479	1492	1526	rBV4	98227	221338	14.15%	1.941%
30	5.985	1526	1538	1579	rVV	331059	692048	44.23%	6.069%
31	6.397	1663	1666	1669	rVB	240	140	0.01%	0.001%
32	6.439	1677	1679	1682	rVV	332	170	0.01%	0.001%
33	6.519	1702	1704	1707	rVB2	262	135	0.01%	0.001%
34	6.551	1707	1714	1715	rBV	173	168	0.01%	0.001%
35	6.603	1728	1730	1732	rVB	280	119	0.01%	0.001%
36	6.674	1747	1752	1754	rBV2	202	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034714.D
 Acq On : 18 Mar 2024 22:43
 Operator : SY/MD
 Sample : P1766-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.699	1758	1760	1763	rVB	288	153	0.01%	0.001%
38	6.870	1809	1813	1816	rBV2	196	198	0.01%	0.002%
39	6.911	1816	1826	1855	rBV	177134	337817	21.59%	2.962%
40	7.130	1892	1894	1896	rBV	437	184	0.01%	0.002%
41	7.178	1906	1909	1915	rVB3	418	274	0.02%	0.002%
42	7.243	1917	1929	1956	rBV	695205	1219355	77.93%	10.693%
43	7.554	2016	2026	2054	rBV	120030	222670	14.23%	1.953%
44	7.799	2100	2102	2104	rBV	267	153	0.01%	0.001%
45	7.812	2104	2106	2108	rVV2	288	137	0.01%	0.001%
46	7.963	2151	2153	2155	rVB	251	113	0.01%	0.001%
47	7.985	2155	2160	2163	rBV	177	151	0.01%	0.001%
48	8.024	2163	2172	2219	rBV	357268	718517	45.92%	6.301%
49	8.455	2302	2306	2308	rBV2	434	303	0.02%	0.003%
50	8.509	2320	2323	2325	rBV2	411	228	0.01%	0.002%
51	8.580	2342	2345	2348	rBV3	241	149	0.01%	0.001%
52	8.648	2362	2366	2367	rBV	214	141	0.01%	0.001%
53	8.696	2378	2381	2386	rBV3	442	392	0.03%	0.003%
54	8.722	2386	2389	2392	rVV	254	165	0.01%	0.001%
55	8.783	2397	2408	2437	rBV	576425	957812	61.22%	8.399%
56	9.114	2508	2511	2516	rVB3	369	297	0.02%	0.003%
57	9.149	2519	2522	2527	rVB3	331	236	0.02%	0.002%
58	9.217	2540	2543	2546	rBV2	292	218	0.01%	0.002%
59	9.320	2573	2575	2585	rVB2	322	289	0.02%	0.003%
60	9.477	2622	2624	2628	rVB2	306	168	0.01%	0.001%
61	9.516	2633	2636	2639	rVB	194	114	0.01%	0.001%
62	9.686	2686	2689	2695	rVB3	351	303	0.02%	0.003%
63	9.718	2695	2699	2702	rBV2	256	219	0.01%	0.002%
64	9.812	2724	2728	2731	rBV	199	142	0.01%	0.001%
65	9.831	2731	2734	2738	rVV2	169	130	0.01%	0.001%
66	9.995	2782	2785	2788	rVB2	307	201	0.01%	0.002%
67	10.011	2788	2790	2795	rVB2	248	141	0.01%	0.001%
68	10.033	2795	2797	2800	rBV	157	109	0.01%	0.001%
69	10.066	2804	2807	2810	rBV2	169	126	0.01%	0.001%
70	10.152	2822	2834	2850	rBV	423133	673649	43.05%	5.907%
71	10.323	2883	2887	2888	rBV2	408	275	0.02%	0.002%
72	10.583	2965	2968	2970	rBV2	262	158	0.01%	0.001%
73	10.606	2971	2975	2978	rVV2	214	179	0.01%	0.002%
74	10.654	2986	2990	2992	rBV2	195	119	0.01%	0.001%
75	10.963	3084	3086	3096	rVB2	260	279	0.02%	0.002%
76	11.005	3096	3099	3101	rBV	279	147	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034714.D
 Acq On : 18 Mar 2024 22:43
 Operator : SY/MD
 Sample : P1766-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.053	3109	3114	3119	rBV2	309	306	0.02%	0.003%
78	11.185	3144	3155	3180	rBV	557891	863594	55.19%	7.573%
79	11.451	3236	3238	3242	rVB2	392	219	0.01%	0.002%
80	11.474	3242	3245	3250	rBV3	309	294	0.02%	0.003%
81	11.558	3259	3271	3295	rBV	634362	1024169	65.46%	8.981%
82	11.750	3327	3331	3332	rBV	483	317	0.02%	0.003%
83	11.837	3355	3358	3361	rVB2	392	218	0.01%	0.002%
84	11.905	3375	3379	3381	rBV2	277	144	0.01%	0.001%
85	12.088	3434	3436	3441	rVB2	197	132	0.01%	0.001%
86	12.156	3455	3457	3458	rBV	361	137	0.01%	0.001%
87	12.297	3498	3501	3503	rBV2	169	118	0.01%	0.001%
88	12.361	3518	3521	3523	rBV2	204	118	0.01%	0.001%
89	12.593	3587	3593	3597	rBV2	292	321	0.02%	0.003%
90	12.615	3598	3600	3603	rVV2	303	174	0.01%	0.002%
91	12.635	3603	3606	3609	rVB2	298	147	0.01%	0.001%
92	12.873	3676	3680	3684	rBV2	399	328	0.02%	0.003%
93	12.992	3714	3717	3719	rBV	369	185	0.01%	0.002%
94	13.448	3857	3859	3861	rBV2	222	130	0.01%	0.001%
95	13.487	3869	3871	3872	rBV	279	152	0.01%	0.001%
96	13.541	3886	3888	3890	rBV2	412	195	0.01%	0.002%
97	13.590	3899	3903	3904	rBV	388	285	0.02%	0.002%
98	13.683	3930	3932	3934	rBV	242	126	0.01%	0.001%
99	13.802	3966	3969	3970	rBV2	356	208	0.01%	0.002%
100	13.940	4009	4012	4013	rBV2	296	146	0.01%	0.001%




Sum of corrected areas: 11403522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034714.D
Acq On : 18 Mar 2024 22:43
Operator : SY/MD
Sample : P1766-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COGN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

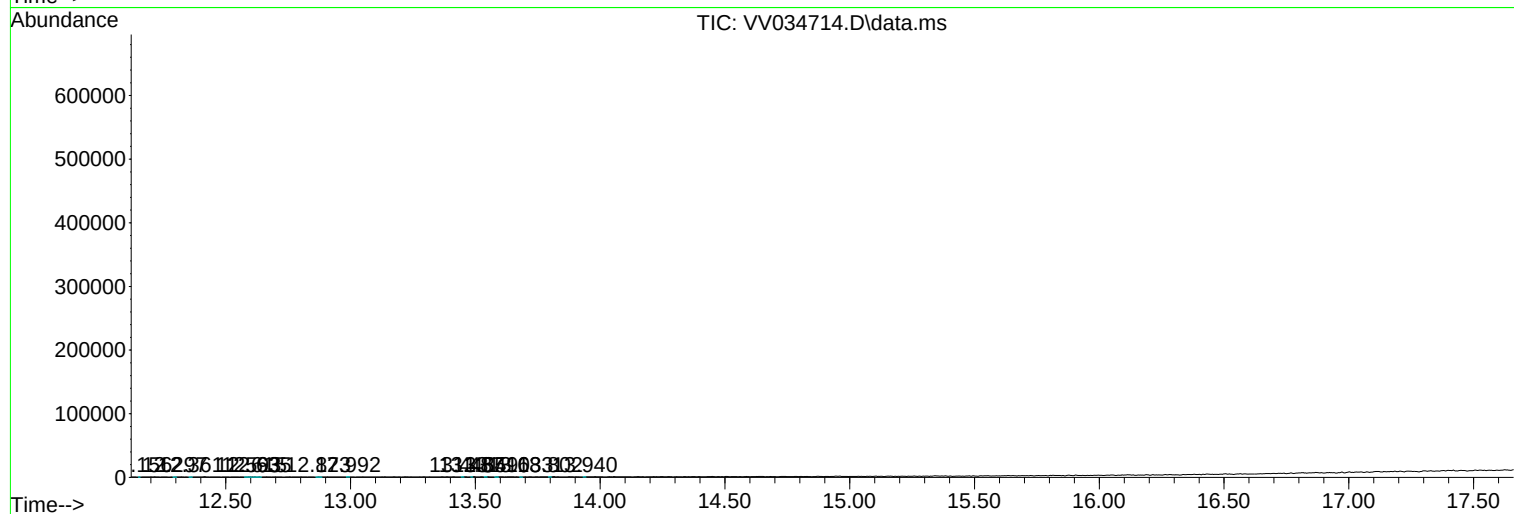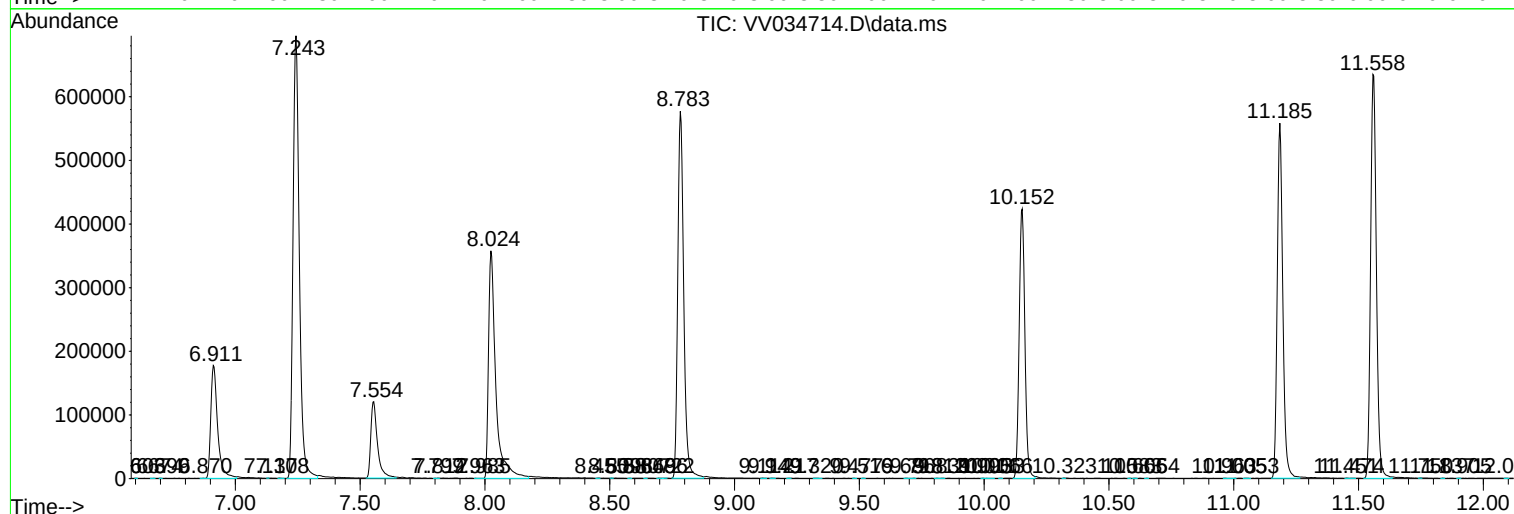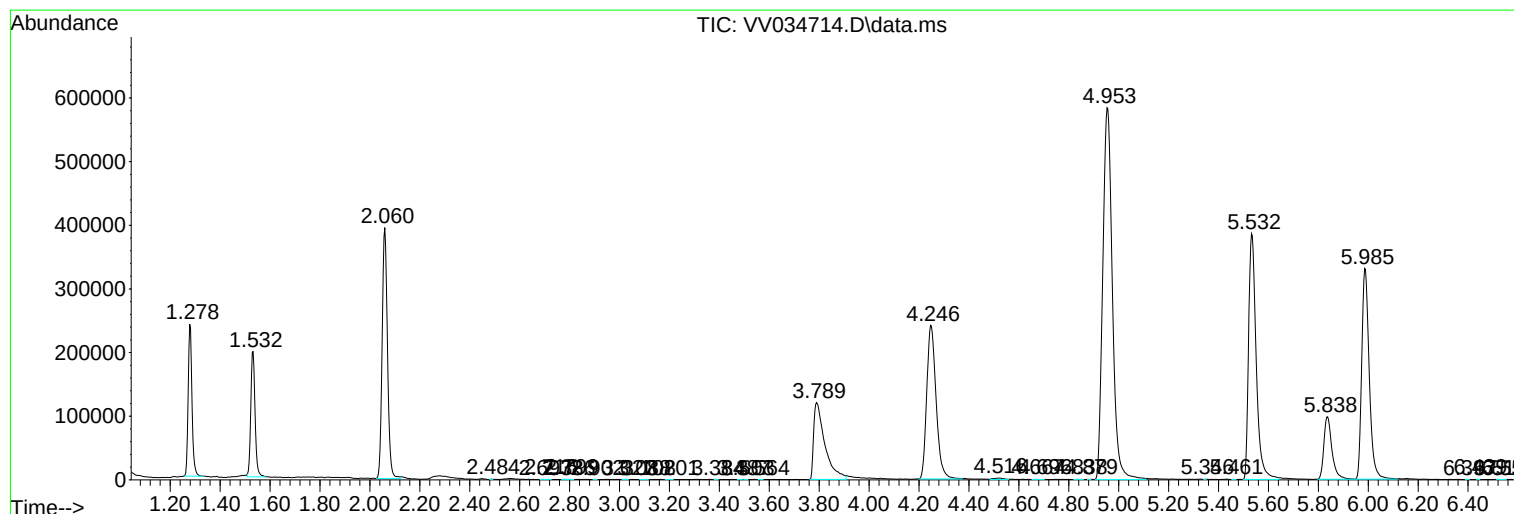

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034714.D
Acq On : 18 Mar 2024 22:43
Operator : SY/MD
Sample : P1766-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034714.D
Acq On : 18 Mar 2024 22:43
Operator : SY/MD
Sample : P1766-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------