

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034715.D
 Acq On : 18 Mar 2024 23:06
 Operator : SY/MD
 Sample : P1766-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	239980	249659	16.70%	2.315%
2	1.529	146	152	166	rVB	193834	224959	15.05%	2.086%
3	2.059	307	317	331	rBV	386163	562122	37.60%	5.213%
4	2.272	371	383	384	rBV2	4145	6971	0.47%	0.065%
5	2.555	467	471	474	rBV4	442	402	0.03%	0.004%
6	2.892	573	576	579	rBV2	185	130	0.01%	0.001%
7	2.908	579	581	582	rBV	178	59	0.00%	0.001%
8	2.995	600	608	610	rBV2	259	256	0.02%	0.002%
9	3.059	625	628	633	rVB2	187	146	0.01%	0.001%
10	3.101	638	641	643	rBV	466	271	0.02%	0.003%
11	3.233	674	682	684	rBV2	209	265	0.02%	0.002%
12	3.301	702	703	704	rBV2	134	42	0.00%	0.000%
13	3.339	713	715	717	rVB	107	42	0.00%	0.000%
14	3.355	717	720	724	rBV2	266	230	0.02%	0.002%
15	3.432	742	744	747	rVB	113	56	0.00%	0.001%
16	3.452	747	750	753	rBV	187	136	0.01%	0.001%
17	3.545	778	779	780	rVB	143	28	0.00%	0.000%
18	3.561	780	784	787	rBV2	263	198	0.01%	0.002%
19	3.577	787	789	791	rBV	132	70	0.00%	0.001%
20	3.789	846	855	887	rBV2	105267	308083	20.61%	2.857%
21	4.246	981	997	1034	rBV	232851	603352	40.36%	5.595%
22	4.641	1119	1120	1121	rBV	282	70	0.00%	0.001%
23	4.767	1156	1159	1160	rBV	328	167	0.01%	0.002%
24	4.838	1178	1181	1185	rBV3	176	149	0.01%	0.001%
25	4.879	1191	1194	1197	rVB2	344	195	0.01%	0.002%
26	4.899	1197	1200	1202	rBV	230	146	0.01%	0.001%
27	4.953	1202	1217	1249	rBV2	562931	1494855	100.00%	13.862%
28	5.252	1306	1310	1312	rBV	320	250	0.02%	0.002%
29	5.397	1352	1355	1358	rVB2	495	279	0.02%	0.003%
30	5.423	1358	1363	1365	rBV2	315	259	0.02%	0.002%
31	5.432	1365	1366	1368	rVB2	228	78	0.01%	0.001%
32	5.532	1387	1397	1432	rBV	372415	780772	52.23%	7.240%
33	5.837	1481	1492	1505	rBV4	8856	19934	1.33%	0.185%
34	5.985	1526	1538	1564	rBV	315700	659194	44.10%	6.113%
35	6.220	1608	1611	1612	rBV	258	125	0.01%	0.001%
36	6.333	1642	1646	1653	rBV3	400	512	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034715.D
 Acq On : 18 Mar 2024 23:06
 Operator : SY/MD
 Sample : P1766-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.394	1662	1665	1670	rBV3	286	326	0.02%	0.003%
38	6.683	1748	1755	1758	rBV2	246	325	0.02%	0.003%
39	6.741	1771	1773	1778	rVB2	193	134	0.01%	0.001%
40	6.764	1778	1780	1782	rBV	207	96	0.01%	0.001%
41	6.911	1816	1826	1855	rBV	170318	323580	21.65%	3.001%
42	7.130	1892	1894	1896	rBV2	380	147	0.01%	0.001%
43	7.243	1917	1929	1954	rBV	664718	1170417	78.30%	10.853%
44	7.551	2017	2025	2049	rBV	115384	211408	14.14%	1.960%
45	7.850	2117	2118	2119	rBV	245	48	0.00%	0.000%
46	7.895	2130	2132	2135	rVB3	361	177	0.01%	0.002%
47	7.966	2151	2154	2158	rBV	401	222	0.01%	0.002%
48	7.982	2158	2159	2161	rBV	134	56	0.00%	0.001%
49	8.024	2163	2172	2217	rBV	335473	675646	45.20%	6.265%
50	8.571	2341	2342	2346	rVB	266	112	0.01%	0.001%
51	8.590	2346	2348	2353	rBV2	271	239	0.02%	0.002%
52	8.635	2360	2362	2364	rBV2	186	107	0.01%	0.001%
53	8.725	2387	2390	2391	rBV2	289	127	0.01%	0.001%
54	8.783	2396	2408	2436	rBV	567636	941569	62.99%	8.731%
55	9.162	2523	2526	2528	rBV2	301	174	0.01%	0.002%
56	9.175	2528	2530	2532	rVB	254	120	0.01%	0.001%
57	9.220	2542	2544	2546	rBV	146	40	0.00%	0.000%
58	9.294	2564	2567	2568	rBV2	170	100	0.01%	0.001%
59	9.387	2593	2596	2599	rBV	113	80	0.01%	0.001%
60	9.448	2610	2615	2617	rBV2	325	283	0.02%	0.003%
61	9.628	2668	2671	2673	rVB2	213	121	0.01%	0.001%
62	9.654	2673	2679	2683	rBV	204	265	0.02%	0.002%
63	9.702	2692	2694	2697	rBV2	180	90	0.01%	0.001%
64	9.985	2779	2782	2783	rBV	126	79	0.01%	0.001%
65	10.069	2807	2808	2812	rVB2	281	124	0.01%	0.001%
66	10.091	2812	2815	2817	rBV	152	103	0.01%	0.001%
67	10.152	2822	2834	2859	rBV	423583	672311	44.97%	6.234%
68	10.332	2888	2890	2894	rVB2	461	319	0.02%	0.003%
69	10.455	2926	2928	2929	rBV2	138	45	0.00%	0.000%
70	10.493	2939	2940	2946	rVB2	247	123	0.01%	0.001%
71	10.763	3022	3024	3027	rVB	185	79	0.01%	0.001%
72	10.847	3047	3050	3051	rBV	144	92	0.01%	0.001%
73	10.879	3057	3060	3064	rBV2	315	229	0.02%	0.002%
74	11.127	3135	3137	3139	rVB	266	99	0.01%	0.001%
75	11.185	3144	3155	3187	rBV	532979	854084	57.13%	7.920%
76	11.561	3259	3272	3296	rBV	625358	1014490	67.87%	9.407%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034715.D
Acq On : 18 Mar 2024 23:06
Operator : SY/MD
Sample : P1766-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

77	11.776	3337	3339	3341	rBV2	270	148	0.01%	0.001%
78	11.930	3385	3387	3392	rBV2	249	202	0.01%	0.002%
79	11.953	3392	3394	3399	rVV2	162	96	0.01%	0.001%
80	12.117	3444	3445	3446	rBV2	197	64	0.00%	0.001%
81	12.185	3463	3466	3470	rBV3	398	292	0.02%	0.003%
82	12.387	3528	3529	3531	rBV	142	46	0.00%	0.000%
83	12.422	3537	3540	3542	rBV2	261	169	0.01%	0.002%
84	12.750	3640	3642	3644	rBV2	196	78	0.01%	0.001%
85	12.837	3666	3669	3673	rBV	340	235	0.02%	0.002%




Sum of corrected areas: 10783978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034715.D
Acq On : 18 Mar 2024 23:06
Operator : SY/MD
Sample : P1766-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

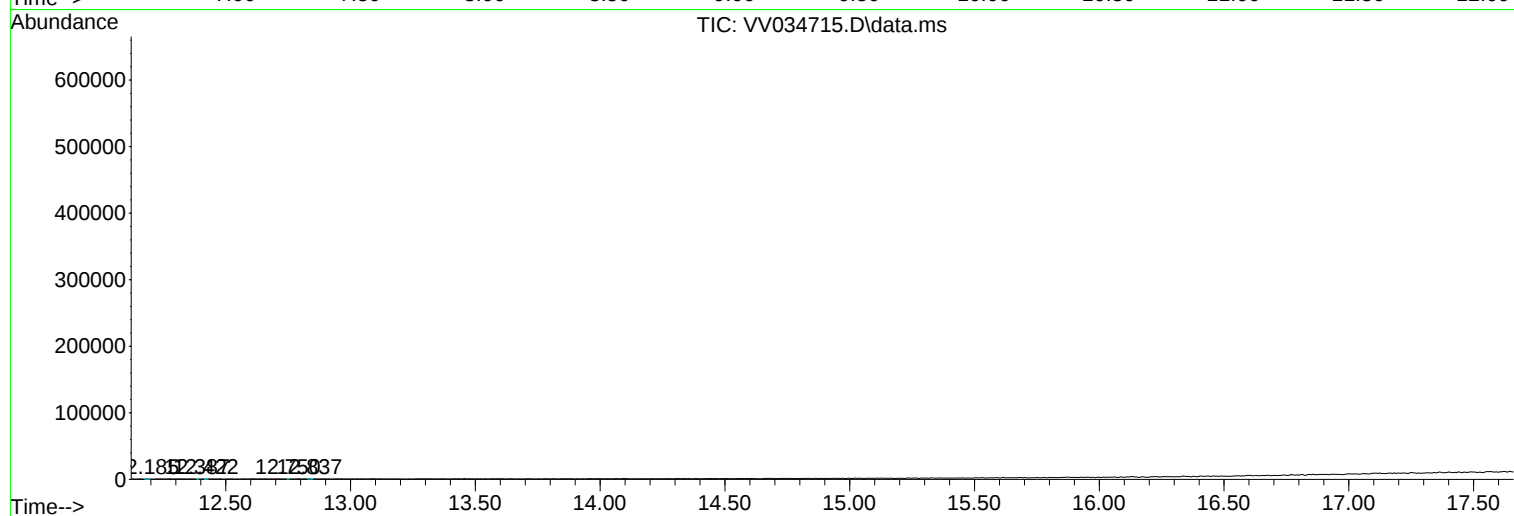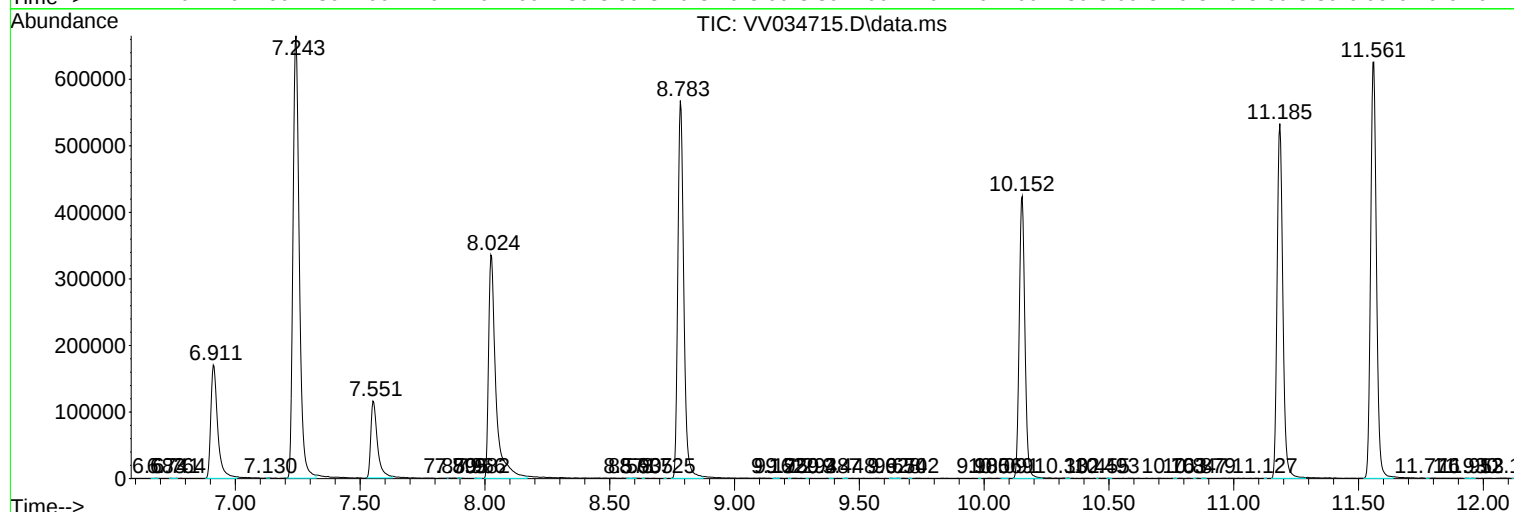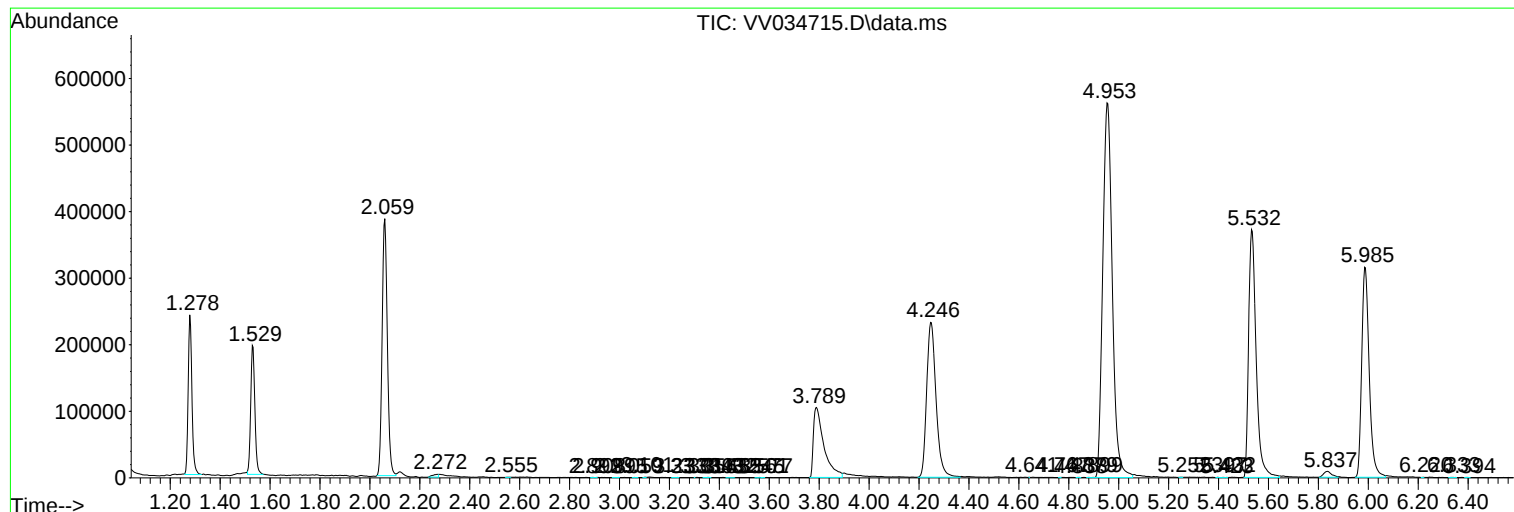

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034715.D
Acq On : 18 Mar 2024 23:06
Operator : SY/MD
Sample : P1766-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034715.D
Acq On : 18 Mar 2024 23:06
Operator : SY/MD
Sample : P1766-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
