

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034716.D
 Acq On : 18 Mar 2024 23:30
 Operator : SY/MD
 Sample : P1766-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	241723	251588	16.08%	2.026%
2	1.529	146	152	167	rVB	197155	230330	14.72%	1.855%
3	2.060	306	317	331	rBV2	417787	634938	40.58%	5.112%
4	2.516	457	459	461	rVB	425	127	0.01%	0.001%
5	2.558	464	472	479	rVV3	2221	3698	0.24%	0.030%
6	2.796	545	546	550	rBV	153	122	0.01%	0.001%
7	3.085	635	636	638	rBV	242	111	0.01%	0.001%
8	3.159	657	659	663	rBV	199	123	0.01%	0.001%
9	3.204	669	673	674	rBV	228	155	0.01%	0.001%
10	3.237	680	683	686	rBV	292	191	0.01%	0.002%
11	3.365	721	723	727	rVB2	245	103	0.01%	0.001%
12	3.413	733	738	740	rBV2	315	257	0.02%	0.002%
13	3.712	827	831	836	rBV2	238	207	0.01%	0.002%
14	3.741	836	840	843	rBV	209	143	0.01%	0.001%
15	3.793	846	856	904	rBV	125209	434661	27.78%	3.500%
16	4.246	982	997	1030	rBV	246935	625914	40.00%	5.040%
17	4.516	1068	1081	1098	rVB4	7562	19794	1.26%	0.159%
18	4.616	1108	1112	1113	rBV	320	223	0.01%	0.002%
19	4.642	1118	1120	1122	rVV2	326	135	0.01%	0.001%
20	4.728	1144	1147	1151	rBV2	239	255	0.02%	0.002%
21	4.954	1201	1217	1261	rBV2	586179	1564767	100.00%	12.599%
22	5.400	1353	1356	1358	rBV2	274	198	0.01%	0.002%
23	5.413	1358	1360	1364	rVV3	379	295	0.02%	0.002%
24	5.490	1381	1384	1386	rBV	302	197	0.01%	0.002%
25	5.532	1386	1397	1432	rBV	393502	820375	52.43%	6.606%
26	5.831	1477	1490	1524	rBV	574783	1174225	75.04%	9.455%
27	5.986	1527	1538	1575	rVB	336090	697597	44.58%	5.617%
28	6.269	1623	1626	1630	rBV2	418	294	0.02%	0.002%
29	6.384	1660	1662	1665	rBV	167	126	0.01%	0.001%
30	6.404	1665	1668	1671	rVB2	296	169	0.01%	0.001%
31	6.426	1671	1675	1677	rBV2	279	164	0.01%	0.001%
32	6.449	1681	1682	1684	rVB	265	101	0.01%	0.001%
33	6.500	1694	1698	1701	rBV2	240	214	0.01%	0.002%
34	6.548	1710	1713	1717	rBV	306	265	0.02%	0.002%
35	6.616	1728	1734	1737	rBV2	178	179	0.01%	0.001%
36	6.693	1754	1758	1761	rBV	180	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034716.D
 Acq On : 18 Mar 2024 23:30
 Operator : SY/MD
 Sample : P1766-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.757	1773	1778	1780	rBV	164	144	0.01%	0.001%
38	6.806	1789	1793	1796	rBV	285	231	0.01%	0.002%
39	6.854	1801	1808	1811	rBV2	182	241	0.02%	0.002%
40	6.912	1816	1826	1868	rBV	176980	341570	21.83%	2.750%
41	7.153	1896	1901	1902	rBV2	333	240	0.02%	0.002%
42	7.243	1915	1929	1952	rBV	675812	1182335	75.56%	9.520%
43	7.551	2016	2025	2055	rBV	117961	216926	13.86%	1.747%
44	7.786	2096	2098	2103	rVB3	482	338	0.02%	0.003%
45	7.847	2112	2117	2118	rBV	322	281	0.02%	0.002%
46	7.937	2142	2145	2149	rBV2	171	117	0.01%	0.001%
47	7.963	2150	2153	2157	rVB2	210	140	0.01%	0.001%
48	7.989	2157	2161	2163	rBV2	208	150	0.01%	0.001%
49	8.024	2163	2172	2214	rBV	340175	683248	43.66%	5.501%
50	8.449	2302	2304	2306	rBV2	263	142	0.01%	0.001%
51	8.548	2332	2335	2338	rBV2	383	316	0.02%	0.003%
52	8.590	2344	2348	2351	rBV	177	158	0.01%	0.001%
53	8.645	2360	2365	2367	rBV2	478	234	0.01%	0.002%
54	8.667	2369	2372	2373	rBV	325	130	0.01%	0.001%
55	8.725	2385	2390	2394	rBV	311	321	0.02%	0.003%
56	8.783	2397	2408	2438	rBV	574484	950511	60.74%	7.653%
57	9.082	2499	2501	2503	rVB	366	132	0.01%	0.001%
58	9.101	2503	2507	2511	rBV	358	291	0.02%	0.002%
59	9.149	2517	2522	2523	rBV2	265	222	0.01%	0.002%
60	9.175	2527	2530	2535	rBV2	138	123	0.01%	0.001%
61	9.201	2535	2538	2543	rVB2	297	255	0.02%	0.002%
62	9.233	2543	2548	2550	rBV2	325	254	0.02%	0.002%
63	9.268	2557	2559	2562	rVB	284	121	0.01%	0.001%
64	9.291	2562	2566	2567	rBV	228	136	0.01%	0.001%
65	9.330	2574	2578	2582	rVB2	216	181	0.01%	0.001%
66	9.359	2583	2587	2591	rBV2	353	278	0.02%	0.002%
67	9.384	2591	2595	2597	rBV	289	249	0.02%	0.002%
68	9.497	2624	2630	2633	rBV2	254	274	0.02%	0.002%
69	9.526	2636	2639	2642	rVB2	148	100	0.01%	0.001%
70	9.616	2663	2667	2671	rBV2	294	325	0.02%	0.003%
71	9.680	2686	2687	2689	rVB	271	103	0.01%	0.001%
72	9.841	2734	2737	2739	rBV	177	103	0.01%	0.001%
73	9.902	2753	2756	2758	rVV2	171	109	0.01%	0.001%
74	9.953	2768	2772	2776	rBV2	156	160	0.01%	0.001%
75	10.043	2798	2800	2804	rVV	181	136	0.01%	0.001%
76	10.153	2821	2834	2859	rBV	427061	675804	43.19%	5.441%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034716.D
 Acq On : 18 Mar 2024 23:30
 Operator : SY/MD
 Sample : P1766-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.320	2882	2886	2887	rBV2	656	515	0.03%	0.004%
78	10.513	2943	2946	2949	rBV2	255	170	0.01%	0.001%
79	10.645	2984	2987	2990	rVB	249	150	0.01%	0.001%
80	10.847	3046	3050	3052	rBV2	173	137	0.01%	0.001%
81	11.018	3100	3103	3107	rVB2	218	175	0.01%	0.001%
82	11.108	3129	3131	3135	rVB	196	103	0.01%	0.001%
83	11.185	3144	3155	3186	rBV	552617	873456	55.82%	7.033%
84	11.442	3233	3235	3239	rVB	348	172	0.01%	0.001%
85	11.465	3239	3242	3243	rBV	210	138	0.01%	0.001%
86	11.561	3259	3272	3300	rBV	632649	1022416	65.34%	8.232%
87	11.825	3351	3354	3355	rBV	264	148	0.01%	0.001%
88	12.021	3413	3415	3419	rVB2	225	108	0.01%	0.001%
89	12.519	3568	3570	3571	rBV	254	113	0.01%	0.001%
90	12.580	3586	3589	3593	rVB	294	200	0.01%	0.002%
91	12.664	3612	3615	3619	rBV3	313	268	0.02%	0.002%
92	12.699	3623	3626	3630	rVB2	430	286	0.02%	0.002%
93	12.760	3642	3645	3649	rBV	232	130	0.01%	0.001%
94	12.870	3676	3679	3682	rBV	464	297	0.02%	0.002%
95	12.982	3711	3714	3719	rBV2	387	317	0.02%	0.003%
96	13.210	3783	3785	3789	rBV3	220	113	0.01%	0.001%
97	13.227	3789	3790	3794	rVB	286	137	0.01%	0.001%
98	13.336	3821	3824	3825	rBV2	277	152	0.01%	0.001%
99	13.371	3833	3835	3837	rBV2	235	103	0.01%	0.001%
100	13.387	3837	3840	3844	rBV	275	208	0.01%	0.002%




Sum of corrected areas: 12419558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034716.D
Acq On : 18 Mar 2024 23:30
Operator : SY/MD
Sample : P1766-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

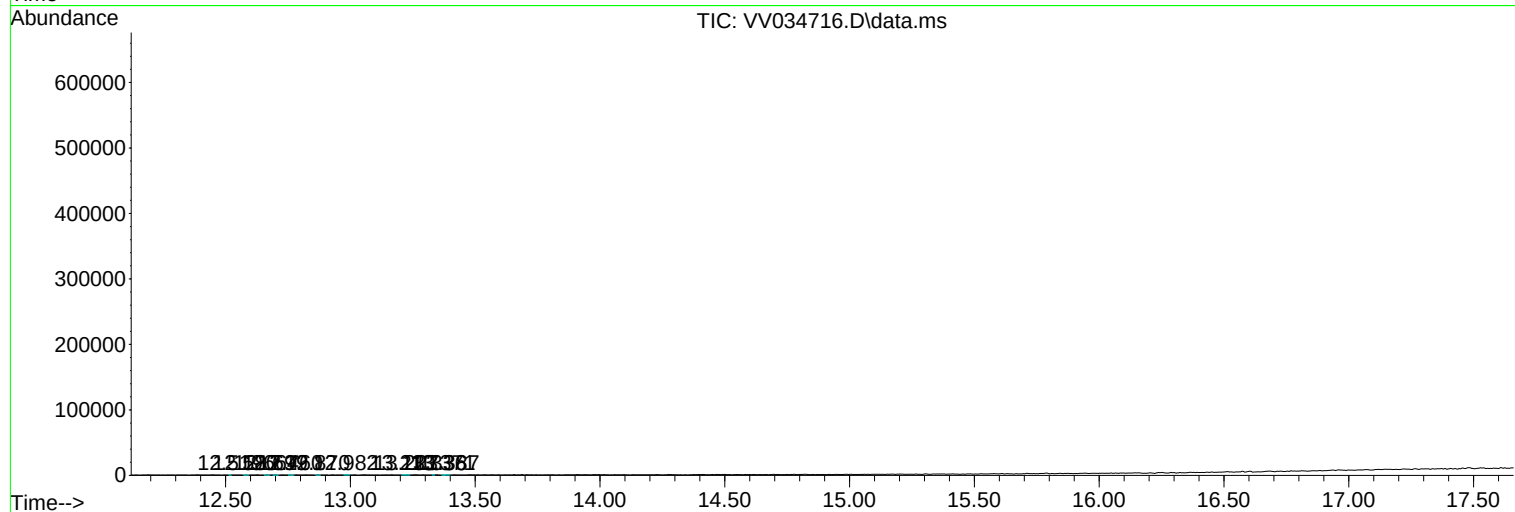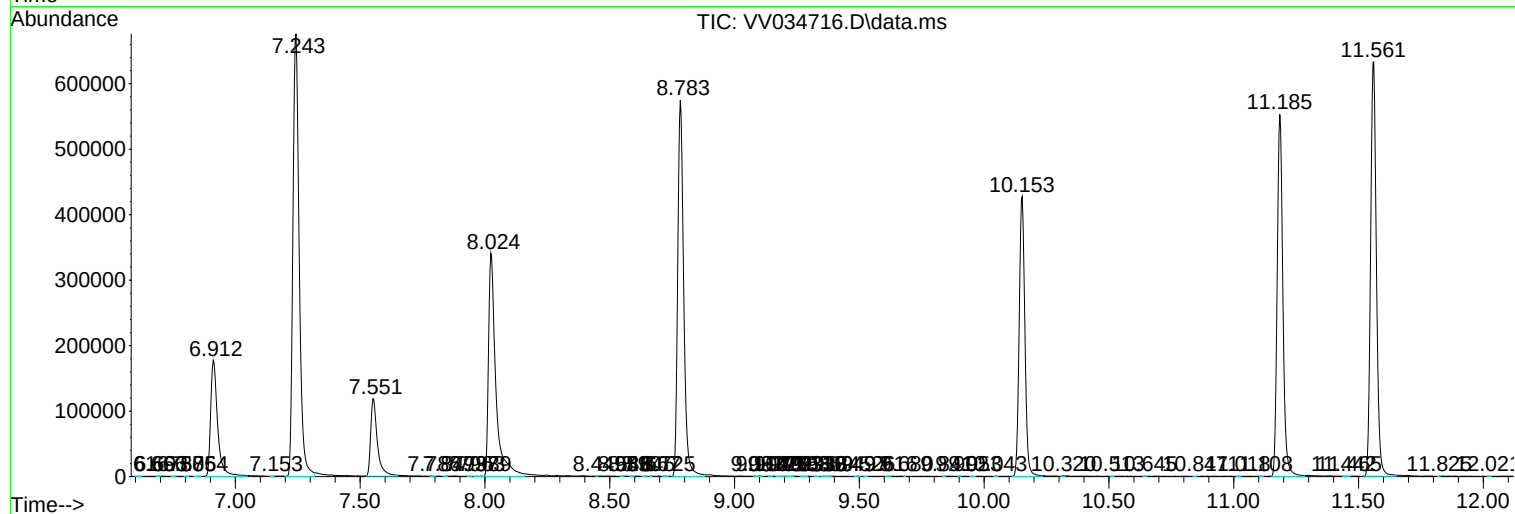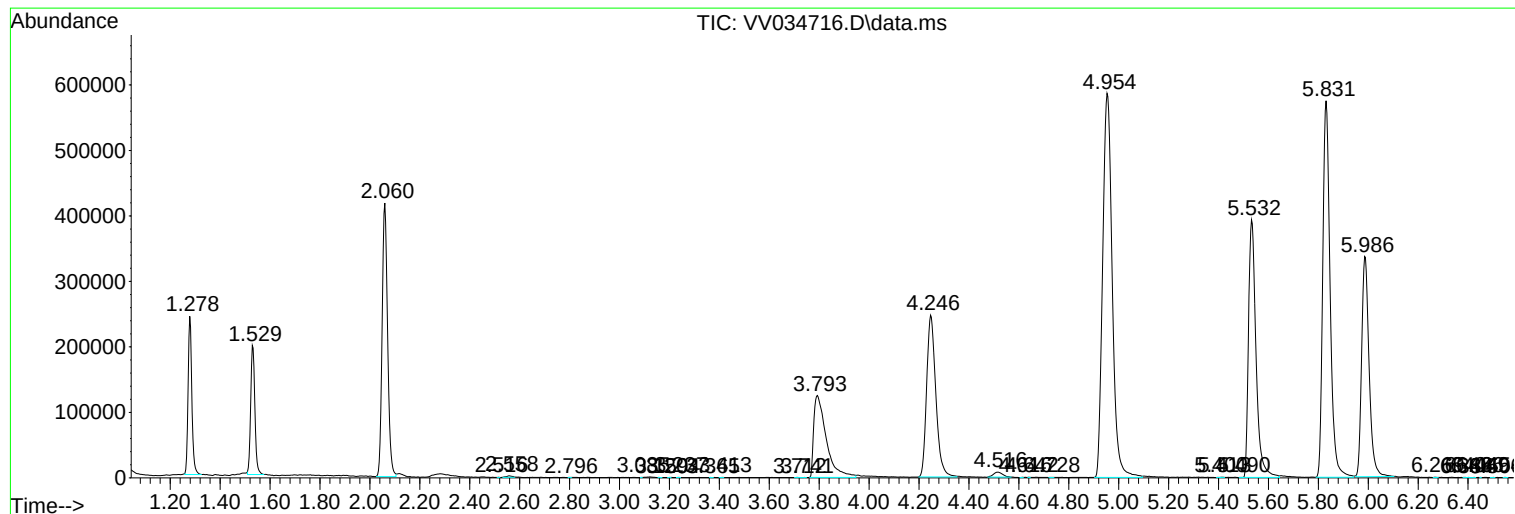

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034716.D
Acq On : 18 Mar 2024 23:30
Operator : SY/MD
Sample : P1766-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034716.D
Acq On : 18 Mar 2024 23:30
Operator : SY/MD
Sample : P1766-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
