

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034722.D
 Acq On : 19 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0319WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	252910	269213	16.13%	2.250%
2	1.536	147	154	173	rVB	213336	248365	14.88%	2.075%
3	2.063	307	318	333	rBV	416658	619705	37.14%	5.178%
4	2.237	368	372	373	rBV	717	504	0.03%	0.004%
5	2.446	432	437	445	rBV4	1413	2442	0.15%	0.020%
6	2.529	461	463	467	rBV2	233	84	0.01%	0.001%
7	2.571	474	476	479	rBV	235	133	0.01%	0.001%
8	2.648	498	500	502	rVB2	200	85	0.01%	0.001%
9	2.703	514	517	521	rBV3	294	207	0.01%	0.002%
10	2.857	563	565	568	rVB2	149	63	0.00%	0.001%
11	3.021	612	616	618	rBV2	211	150	0.01%	0.001%
12	3.066	627	630	632	rBV	205	109	0.01%	0.001%
13	3.124	647	648	654	rBV2	163	97	0.01%	0.001%
14	3.288	697	699	704	rBV2	170	92	0.01%	0.001%
15	3.378	721	727	731	rBV	259	280	0.02%	0.002%
16	3.593	791	794	797	rBV2	253	223	0.01%	0.002%
17	3.687	822	823	824	rBV	173	50	0.00%	0.000%
18	3.735	833	838	841	rBV2	199	155	0.01%	0.001%
19	3.757	841	845	848	rBV2	168	141	0.01%	0.001%
20	3.793	848	856	900	rBV	107031	326684	19.58%	2.730%
21	4.249	983	998	1035	rBV	256129	659569	39.52%	5.511%
22	4.654	1116	1124	1126	rBV3	433	597	0.04%	0.005%
23	4.761	1155	1157	1161	rVV2	251	122	0.01%	0.001%
24	4.780	1161	1163	1166	rVB	284	106	0.01%	0.001%
25	4.841	1178	1182	1184	rBV2	185	163	0.01%	0.001%
26	4.957	1202	1218	1259	rBV2	630771	1668755	100.00%	13.944%
27	5.346	1336	1339	1343	rBV2	637	408	0.02%	0.003%
28	5.452	1369	1372	1375	rBV3	434	352	0.02%	0.003%
29	5.532	1386	1397	1427	rBV	416458	855623	51.27%	7.150%
30	5.831	1480	1490	1512	rVB3	11361	26795	1.61%	0.224%
31	5.986	1525	1538	1571	rBV	349506	735261	44.06%	6.144%
32	6.207	1606	1607	1614	rVB4	626	355	0.02%	0.003%
33	6.320	1639	1642	1645	rVB3	394	254	0.02%	0.002%
34	6.343	1645	1649	1650	rBV2	251	126	0.01%	0.001%
35	6.355	1650	1653	1655	rBV2	276	151	0.01%	0.001%
36	6.433	1673	1677	1680	rVB2	249	150	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034722.D
 Acq On : 19 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0319WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.455	1680	1684	1685	rBV	242	121	0.01%	0.001%
38	6.500	1695	1698	1702	rVB2	189	111	0.01%	0.001%
39	6.542	1709	1711	1715	rBV2	121	121	0.01%	0.001%
40	6.709	1761	1763	1767	rBV2	157	103	0.01%	0.001%
41	6.860	1804	1810	1811	rBV2	186	174	0.01%	0.001%
42	6.912	1815	1826	1863	rBV2	190846	367949	22.05%	3.075%
43	7.243	1917	1929	1959	rBV	735200	1315068	78.81%	10.989%
44	7.551	2016	2025	2055	rBV2	132586	242587	14.54%	2.027%
45	7.847	2115	2117	2118	rBV2	114	44	0.00%	0.000%
46	7.857	2118	2120	2121	rBV2	140	41	0.00%	0.000%
47	7.876	2124	2126	2127	rBV	260	83	0.00%	0.001%
48	7.905	2133	2135	2137	rVB	205	81	0.00%	0.001%
49	7.918	2137	2139	2144	rBV	369	251	0.02%	0.002%
50	7.960	2148	2152	2154	rBV3	237	180	0.01%	0.002%
51	8.024	2163	2172	2216	rBV	353369	718806	43.07%	6.006%
52	8.613	2352	2355	2357	rBV	216	163	0.01%	0.001%
53	8.699	2379	2382	2385	rBV2	247	201	0.01%	0.002%
54	8.738	2391	2394	2397	rBV	358	286	0.02%	0.002%
55	8.783	2397	2408	2440	rBV	628222	1038537	62.23%	8.678%
56	9.162	2523	2526	2529	rVB	363	187	0.01%	0.002%
57	9.236	2547	2549	2550	rBV	152	44	0.00%	0.000%
58	9.246	2550	2552	2555	rVV	192	87	0.01%	0.001%
59	9.310	2569	2572	2574	rBV2	195	145	0.01%	0.001%
60	9.336	2577	2580	2581	rBV	123	63	0.00%	0.001%
61	9.474	2620	2623	2627	rVV3	204	148	0.01%	0.001%
62	9.542	2641	2644	2646	rVB2	368	164	0.01%	0.001%
63	9.561	2646	2650	2655	rBV3	324	350	0.02%	0.003%
64	9.603	2661	2663	2664	rBV	125	38	0.00%	0.000%
65	9.638	2671	2674	2677	rBV2	155	145	0.01%	0.001%
66	9.674	2682	2685	2689	rBV	275	197	0.01%	0.002%
67	9.879	2742	2749	2753	rVB3	385	532	0.03%	0.004%
68	9.902	2753	2756	2759	rBV2	330	233	0.01%	0.002%
69	10.030	2794	2796	2797	rBV	252	102	0.01%	0.001%
70	10.149	2821	2833	2859	rBV	458987	725145	43.45%	6.059%
71	10.326	2886	2888	2893	rBV4	401	365	0.02%	0.003%
72	10.384	2903	2906	2913	rVB2	399	373	0.02%	0.003%
73	10.429	2918	2920	2921	rBV	243	63	0.00%	0.001%
74	10.490	2936	2939	2941	rVB	435	204	0.01%	0.002%
75	10.529	2948	2951	2953	rBV	197	113	0.01%	0.001%
76	10.600	2970	2973	2974	rBV	229	106	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034722.D
 Acq On : 19 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0319WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.735	3014	3015	3017	rVB2	173	63	0.00%	0.001%
78	10.870	3051	3057	3062	rBV2	664	795	0.05%	0.007%
79	10.944	3079	3080	3081	rVB	263	51	0.00%	0.000%
80	11.127	3133	3137	3140	rBV2	704	667	0.04%	0.006%
81	11.185	3144	3155	3189	rBV	615436	973741	58.35%	8.137%
82	11.468	3241	3243	3245	rBV	240	113	0.01%	0.001%
83	11.558	3259	3271	3296	rBV	704066	1123448	67.32%	9.388%
84	11.908	3378	3380	3381	rBV2	214	84	0.01%	0.001%
85	12.008	3408	3411	3413	rVB	179	103	0.01%	0.001%
86	12.063	3427	3428	3429	rBV	176	64	0.00%	0.001%
87	12.085	3433	3435	3440	rBV2	181	168	0.01%	0.001%
88	12.403	3532	3534	3540	rBV2	344	246	0.01%	0.002%
89	12.580	3586	3589	3590	rBV2	474	264	0.02%	0.002%
90	12.590	3590	3592	3601	rVB4	1229	1462	0.09%	0.012%
91	12.622	3601	3602	3604	rBV	307	69	0.00%	0.001%
92	12.882	3679	3683	3684	rBV	277	170	0.01%	0.001%
93	12.989	3709	3716	3719	rBV2	298	373	0.02%	0.003%
94	13.210	3777	3785	3797	rVB4	2722	4776	0.29%	0.040%
95	13.333	3820	3823	3828	rBV2	335	360	0.02%	0.003%
96	13.445	3850	3858	3872	rBV3	13916	22956	1.38%	0.192%
97	13.644	3917	3920	3922	rBV3	349	204	0.01%	0.002%
98	13.689	3926	3934	3941	rVV5	3379	5271	0.32%	0.044%
99	14.181	4084	4087	4091	rBV	316	311	0.02%	0.003%
100	14.239	4104	4105	4106	rBV	547	133	0.01%	0.001%




Sum of corrected areas: 11967172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034722.D
Acq On : 19 Mar 2024 10:02
Operator : SY/MD
Sample : VV0319WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

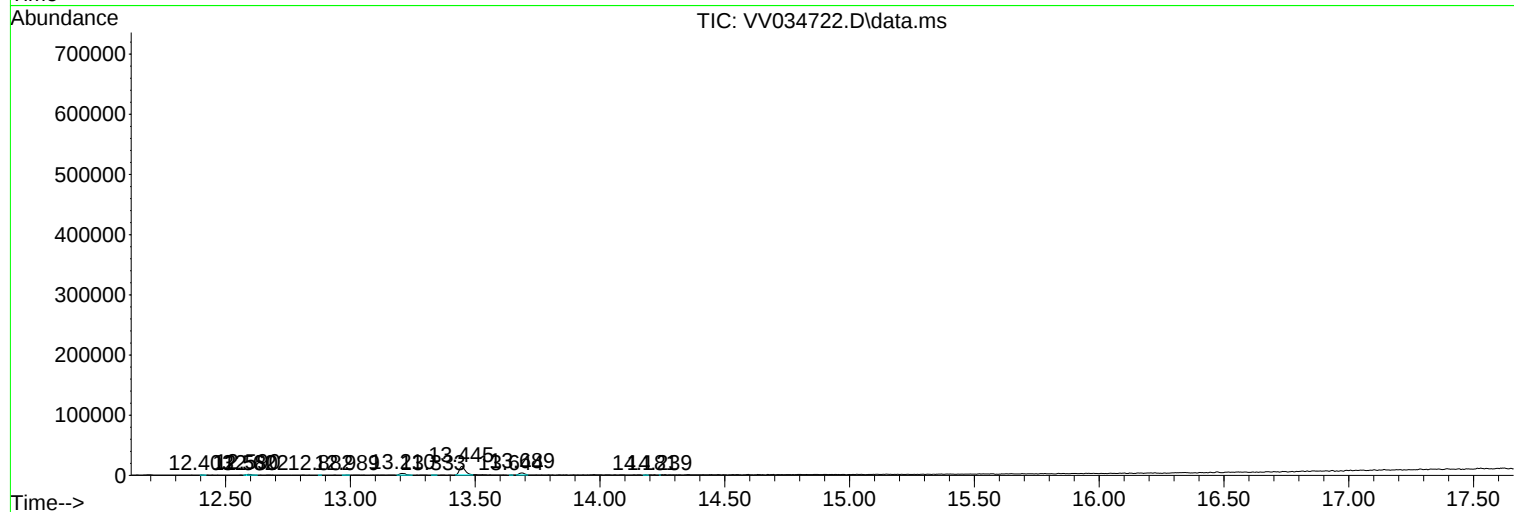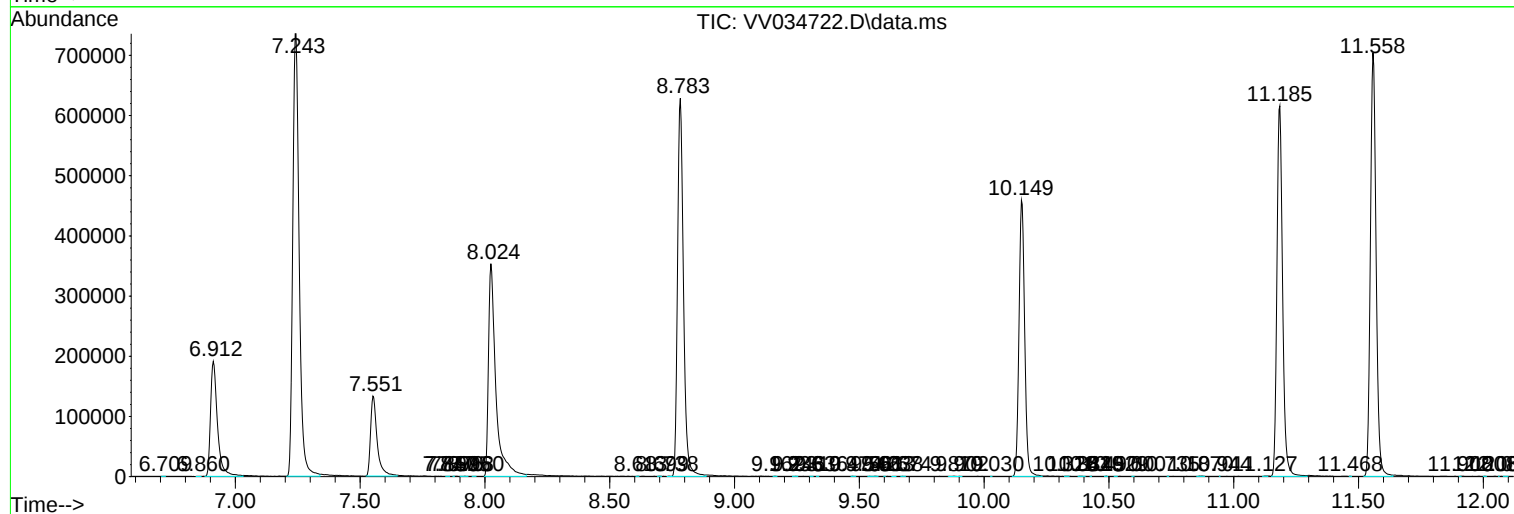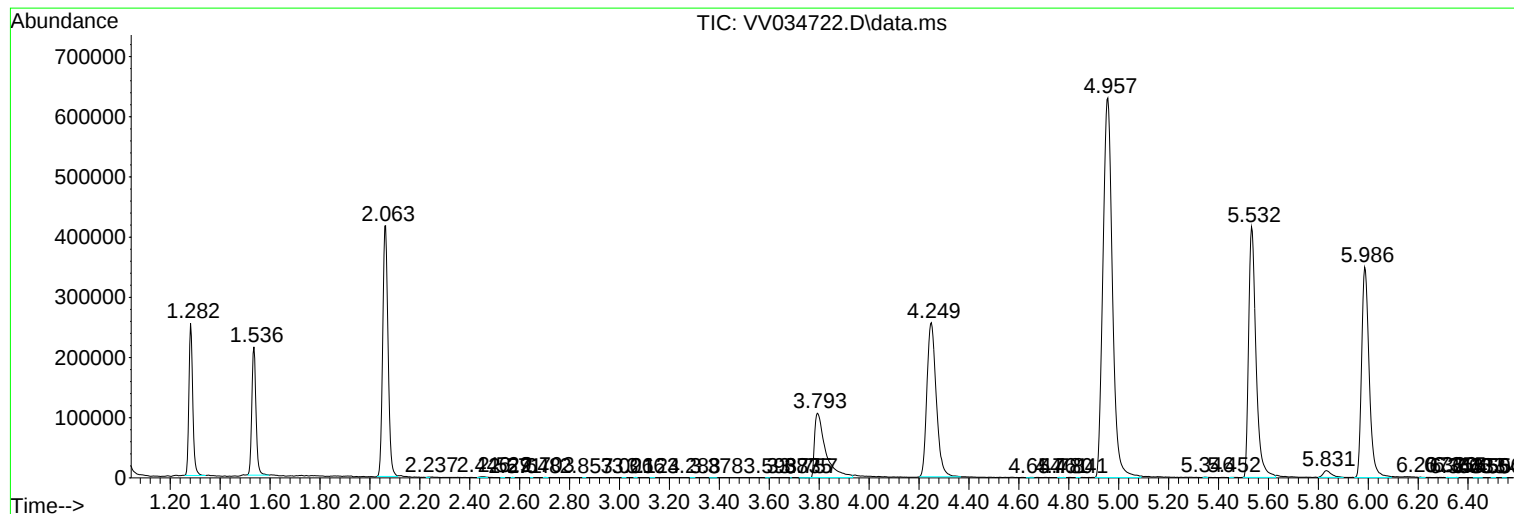

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034722.D
Acq On : 19 Mar 2024 10:02
Operator : SY/MD
Sample : VV0319WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034722.D
Acq On : 19 Mar 2024 10:02
Operator : SY/MD
Sample : VV0319WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------