

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034723.D
 Acq On : 19 Mar 2024 10:25
 Operator : SY/MD
 Sample : P1766-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	227572	247134	16.57%	2.258%
2	1.532	145	153	173	rVB	196767	234838	15.75%	2.146%
3	2.060	306	317	333	rBV	384850	563247	37.77%	5.146%
4	2.278	365	385	388	rBV2	8085	18589	1.25%	0.170%
5	2.555	462	471	479	rBV4	3567	7240	0.49%	0.066%
6	2.873	567	570	578	rVB3	312	360	0.02%	0.003%
7	2.928	581	587	594	rBV2	207	287	0.02%	0.003%
8	3.008	609	612	617	rBV2	237	259	0.02%	0.002%
9	3.394	727	732	737	rVB2	213	183	0.01%	0.002%
10	3.606	794	798	799	rBV	224	165	0.01%	0.002%
11	3.793	846	856	897	rBV2	108148	345453	23.16%	3.156%
12	4.246	981	997	1024	rBV	234465	598778	40.15%	5.471%
13	4.449	1058	1060	1064	rVB2	479	274	0.02%	0.003%
14	4.478	1064	1069	1071	rBV3	430	404	0.03%	0.004%
15	4.523	1080	1083	1086	rBV3	244	167	0.01%	0.002%
16	4.863	1187	1189	1192	rVB	403	228	0.02%	0.002%
17	4.899	1196	1200	1201	rBV	486	290	0.02%	0.003%
18	4.953	1201	1217	1253	rBV2	561219	1491324	100.00%	13.625%
19	5.188	1288	1290	1292	rVB2	429	183	0.01%	0.002%
20	5.256	1309	1311	1315	rVB2	593	363	0.02%	0.003%
21	5.281	1315	1319	1322	rBV3	475	370	0.02%	0.003%
22	5.359	1340	1343	1348	rVB2	422	244	0.02%	0.002%
23	5.462	1373	1375	1381	rBV2	278	241	0.02%	0.002%
24	5.532	1386	1397	1431	rBV	400242	830695	55.70%	7.589%
25	5.834	1479	1491	1505	rBV4	9558	21814	1.46%	0.199%
26	5.986	1525	1538	1569	rBV	317706	662146	44.40%	6.049%
27	6.243	1615	1618	1621	rBV2	369	222	0.01%	0.002%
28	6.285	1629	1631	1635	rVV2	315	214	0.01%	0.002%
29	6.365	1652	1656	1658	rBV	344	269	0.02%	0.002%
30	6.442	1678	1680	1686	rVB2	267	211	0.01%	0.002%
31	6.912	1815	1826	1855	rBV	165314	320107	21.46%	2.925%
32	7.140	1894	1897	1898	rBV	336	218	0.01%	0.002%
33	7.240	1917	1928	1970	rVV	660374	1168326	78.34%	10.674%
34	7.551	2016	2025	2048	rBV	113705	205578	13.78%	1.878%
35	7.728	2077	2080	2084	rBV2	454	405	0.03%	0.004%
36	7.850	2115	2118	2120	rBV3	333	242	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034723.D
 Acq On : 19 Mar 2024 10:25
 Operator : SY/MD
 Sample : P1766-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.873	2120	2125	2134	rVB2	1054	1450	0.10%	0.013%
38	7.921	2134	2140	2142	rBV2	281	255	0.02%	0.002%
39	8.024	2163	2172	2220	rBV	311556	644726	43.23%	5.890%
40	8.362	2275	2277	2279	rBV2	349	200	0.01%	0.002%
41	8.494	2316	2318	2323	rVB2	445	274	0.02%	0.003%
42	8.783	2396	2408	2436	rBV	601580	987181	66.19%	9.019%
43	9.075	2495	2499	2501	rBV2	381	235	0.02%	0.002%
44	9.095	2501	2505	2507	rBV2	329	213	0.01%	0.002%
45	9.256	2552	2555	2559	rVB	314	222	0.01%	0.002%
46	9.375	2590	2592	2597	rVB2	297	193	0.01%	0.002%
47	9.657	2677	2680	2686	rVB2	211	198	0.01%	0.002%
48	9.754	2707	2710	2714	rVB2	229	189	0.01%	0.002%
49	9.815	2725	2729	2734	rBV2	339	352	0.02%	0.003%
50	9.883	2744	2750	2752	rBV2	282	262	0.02%	0.002%
51	10.149	2821	2833	2858	rBV	415426	656979	44.05%	6.002%
52	10.281	2870	2874	2875	rVB2	472	267	0.02%	0.002%
53	10.304	2879	2881	2883	rVV2	306	215	0.01%	0.002%
54	10.323	2883	2887	2896	rVB4	1132	1343	0.09%	0.012%
55	10.426	2915	2919	2922	rBV2	325	221	0.01%	0.002%
56	10.487	2934	2938	2944	rBV3	508	623	0.04%	0.006%
57	10.542	2951	2955	2957	rVB2	480	206	0.01%	0.002%
58	10.561	2957	2961	2964	rBV	279	256	0.02%	0.002%
59	10.622	2974	2980	2983	rBV2	185	212	0.01%	0.002%
60	10.641	2983	2986	2993	rVB2	290	305	0.02%	0.003%
61	10.821	3040	3042	3047	rVB	351	219	0.01%	0.002%
62	11.037	3103	3109	3116	rBV2	298	487	0.03%	0.004%
63	11.185	3144	3155	3179	rBV	570036	898207	60.23%	8.206%
64	11.323	3194	3198	3205	rVB5	1267	1533	0.10%	0.014%
65	11.481	3243	3247	3252	rVB2	356	391	0.03%	0.004%
66	11.558	3252	3271	3294	rBV	636820	1002867	67.25%	9.162%
67	11.728	3320	3324	3330	rVB2	457	449	0.03%	0.004%
68	11.796	3343	3345	3348	rBV	298	164	0.01%	0.001%
69	11.976	3397	3401	3403	rBV	212	182	0.01%	0.002%
70	12.236	3480	3482	3486	rBV2	226	166	0.01%	0.002%
71	12.513	3565	3568	3570	rBV	230	164	0.01%	0.001%
72	12.545	3577	3578	3587	rVB	626	422	0.03%	0.004%
73	12.587	3587	3591	3594	rBV	961	708	0.05%	0.006%
74	12.645	3607	3609	3613	rBV2	276	170	0.01%	0.002%
75	12.760	3641	3645	3647	rBV2	301	214	0.01%	0.002%
76	12.792	3652	3655	3658	rVV2	294	231	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034723.D
 Acq On : 19 Mar 2024 10:25
 Operator : SY/MD
 Sample : P1766-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.985	3713	3715	3720	rVB2	375	276	0.02%	0.003%
78	13.149	3763	3766	3769	rBV2	261	181	0.01%	0.002%
79	13.210	3779	3785	3794	rBV5	1916	2617	0.18%	0.024%
80	13.288	3806	3809	3811	rBV	257	163	0.01%	0.001%
81	13.371	3832	3835	3838	rBV2	445	293	0.02%	0.003%
82	13.419	3847	3850	3852	rBV	342	203	0.01%	0.002%
83	13.448	3852	3859	3871	rBV3	5473	9422	0.63%	0.086%
84	13.535	3882	3886	3889	rBV3	282	267	0.02%	0.002%
85	13.564	3892	3895	3897	rVB	373	225	0.02%	0.002%
86	13.625	3911	3914	3920	rVB	387	286	0.02%	0.003%
87	13.689	3922	3934	3942	rBV5	2165	3554	0.24%	0.032%
88	13.802	3966	3969	3973	rBV3	305	222	0.01%	0.002%
89	13.863	3986	3988	3992	rVV2	336	200	0.01%	0.002%
90	13.898	3996	3999	4001	rBV3	302	183	0.01%	0.002%
91	13.943	4010	4013	4016	rVB2	425	210	0.01%	0.002%
92	13.960	4016	4018	4020	rBV	410	268	0.02%	0.002%
93	14.152	4075	4078	4079	rBV2	285	182	0.01%	0.002%
94	14.243	4103	4106	4108	rBV2	398	254	0.02%	0.002%
95	14.429	4162	4164	4168	rBV3	578	322	0.02%	0.003%
96	14.538	4195	4198	4202	rVB4	557	346	0.02%	0.003%
97	14.731	4255	4258	4261	rBV3	402	320	0.02%	0.003%
98	14.918	4313	4316	4321	rBV5	649	598	0.04%	0.005%
99	15.104	4371	4374	4376	rBV2	594	434	0.03%	0.004%
100	15.223	4408	4411	4412	rBV2	519	325	0.02%	0.003%




Sum of corrected areas: 10945570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034723.D
Acq On : 19 Mar 2024 10:25
Operator : SY/MD
Sample : P1766-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

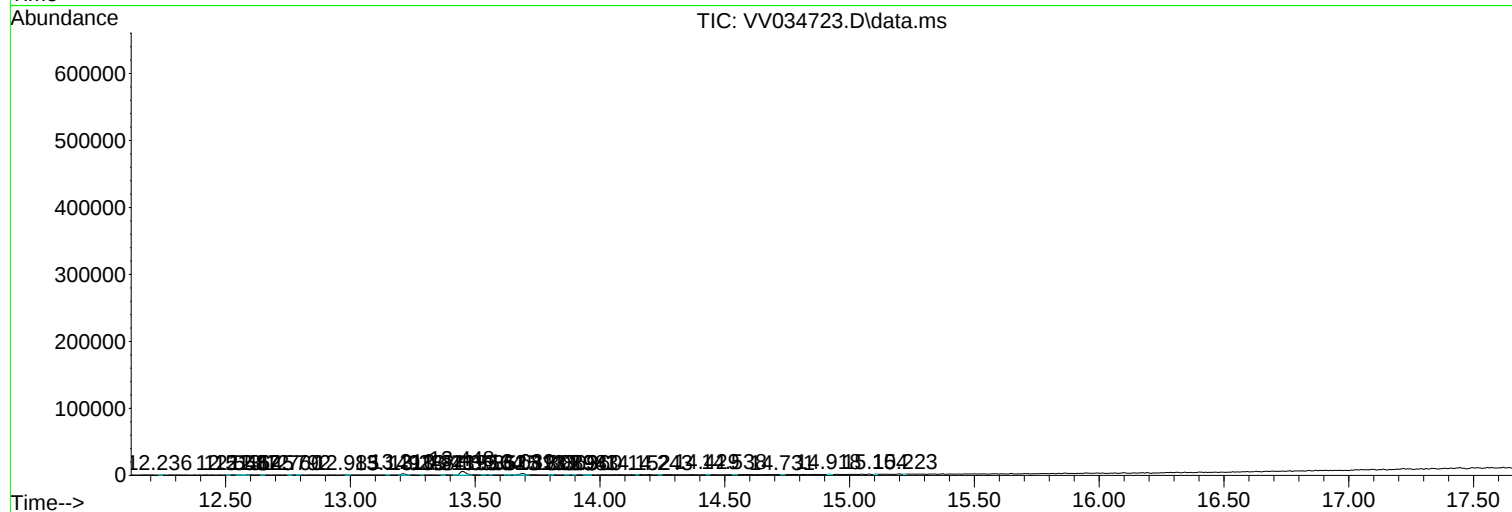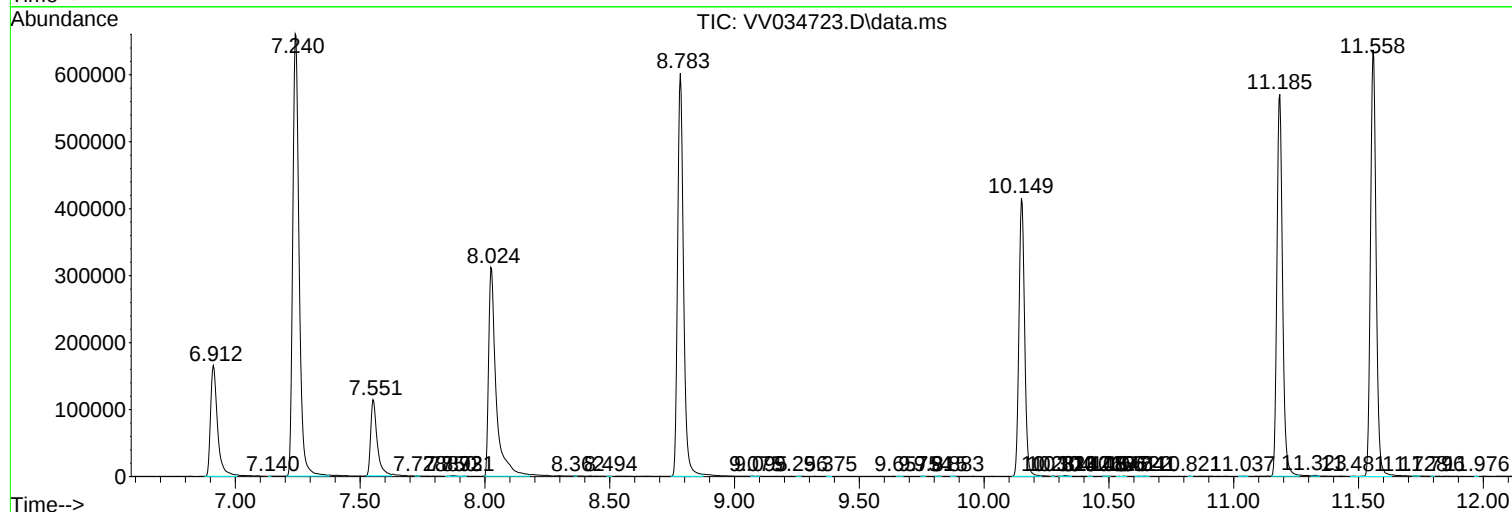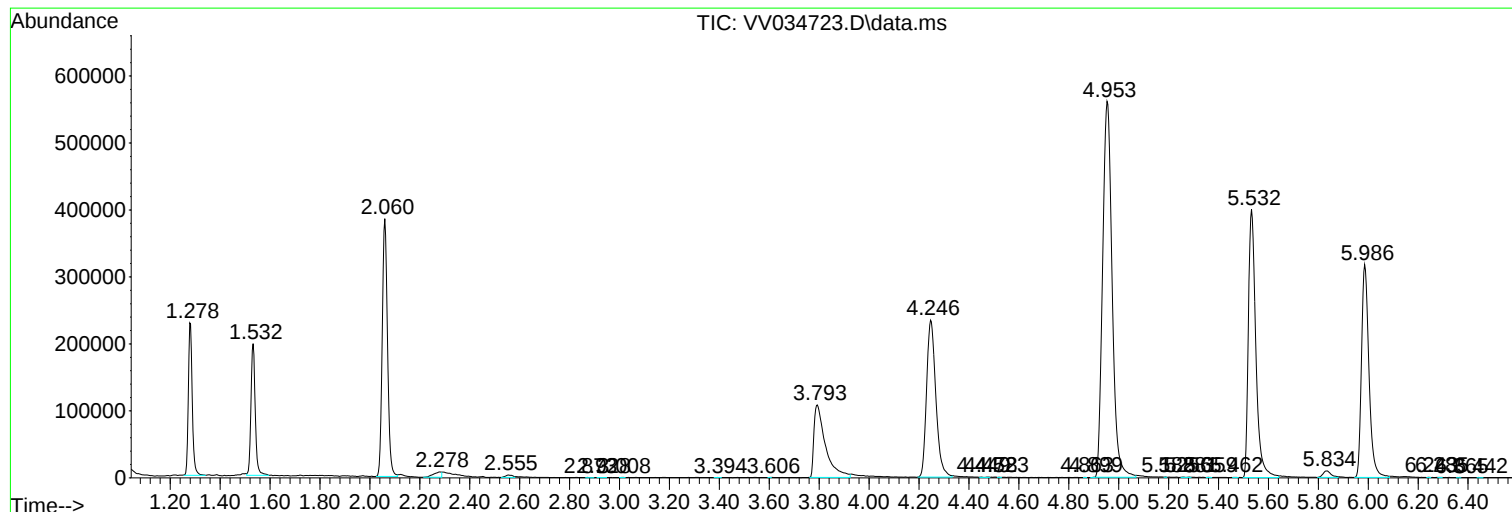

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034723.D
Acq On : 19 Mar 2024 10:25
Operator : SY/MD
Sample : P1766-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034723.D
Acq On : 19 Mar 2024 10:25
Operator : SY/MD
Sample : P1766-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
