

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034724.D
 Acq On : 19 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1766-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	237681	255844	16.61%	2.248%
2	1.532	146	153	169	rVB	204976	233237	15.15%	2.049%
3	2.060	307	317	334	rBV	403435	600006	38.96%	5.272%
4	2.548	463	469	470	rBV2	1317	1101	0.07%	0.010%
5	2.712	518	520	521	rBV2	210	80	0.01%	0.001%
6	2.879	569	572	573	rBV2	115	73	0.00%	0.001%
7	2.953	593	595	596	rBV	149	60	0.00%	0.001%
8	3.047	620	624	626	rBV2	179	157	0.01%	0.001%
9	3.088	634	637	639	rBV	185	121	0.01%	0.001%
10	3.117	641	646	648	rBV3	273	262	0.02%	0.002%
11	3.204	668	673	678	rBV2	174	214	0.01%	0.002%
12	3.233	678	682	686	rVB2	264	210	0.01%	0.002%
13	3.291	697	700	702	rBV2	133	80	0.01%	0.001%
14	3.320	706	709	711	rBV	112	70	0.00%	0.001%
15	3.365	720	723	724	rBV2	302	161	0.01%	0.001%
16	3.397	730	733	735	rBV	249	107	0.01%	0.001%
17	3.461	751	753	754	rBV	142	41	0.00%	0.000%
18	3.513	765	769	771	rBV	150	124	0.01%	0.001%
19	3.529	771	774	775	rBV	153	89	0.01%	0.001%
20	3.561	783	784	785	rBV	202	58	0.00%	0.001%
21	3.593	792	794	795	rBV	101	41	0.00%	0.000%
22	3.648	808	811	812	rBV	75	42	0.00%	0.000%
23	3.699	824	827	829	rBV2	113	78	0.01%	0.001%
24	3.712	829	831	832	rBB	111	23	0.00%	0.000%
25	3.738	836	839	841	rVB2	104	54	0.00%	0.000%
26	3.754	841	844	845	rBV	140	71	0.00%	0.001%
27	3.793	847	856	893	rBV	106696	341156	22.15%	2.997%
28	4.246	982	997	1027	rBV	240067	616454	40.03%	5.416%
29	4.780	1161	1163	1167	rVB2	162	98	0.01%	0.001%
30	4.799	1167	1169	1172	rBV2	151	130	0.01%	0.001%
31	4.838	1178	1181	1183	rBV2	188	118	0.01%	0.001%
32	4.953	1201	1217	1249	rBV2	581403	1539893	100.00%	13.530%
33	5.410	1357	1359	1362	rBV2	253	121	0.01%	0.001%
34	5.432	1365	1366	1369	rVB2	222	87	0.01%	0.001%
35	5.532	1386	1397	1424	rBV	384878	798380	51.85%	7.015%
36	5.834	1479	1491	1520	rBV2	155934	332902	21.62%	2.925%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034724.D
 Acq On : 19 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1766-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.985	1526	1538	1572	rBV	328124	685517	44.52%	6.023%
38	6.278	1626	1629	1631	rBV	233	181	0.01%	0.002%
39	6.313	1635	1640	1641	rBV2	207	152	0.01%	0.001%
40	6.397	1662	1666	1667	rBV	118	78	0.01%	0.001%
41	6.403	1667	1668	1669	rVB	158	30	0.00%	0.000%
42	6.420	1669	1673	1675	rBV	259	205	0.01%	0.002%
43	6.522	1703	1705	1710	rVB	221	120	0.01%	0.001%
44	6.612	1731	1733	1736	rBV	105	63	0.00%	0.001%
45	6.657	1742	1747	1748	rBV2	170	132	0.01%	0.001%
46	6.690	1753	1757	1760	rBV2	220	157	0.01%	0.001%
47	6.809	1792	1794	1796	rBV2	56	25	0.00%	0.000%
48	6.873	1811	1814	1816	rBV	203	122	0.01%	0.001%
49	6.911	1816	1826	1857	rBV	170807	326320	21.19%	2.867%
50	7.239	1917	1928	1956	rBV	682632	1206181	78.33%	10.598%
51	7.551	2016	2025	2052	rBV	115899	215120	13.97%	1.890%
52	7.908	2133	2136	2138	rBV2	243	155	0.01%	0.001%
53	7.976	2155	2157	2159	rBV2	119	51	0.00%	0.000%
54	8.024	2163	2172	2213	rBV	323875	673244	43.72%	5.915%
55	8.381	2281	2283	2284	rBV2	427	214	0.01%	0.002%
56	8.471	2310	2311	2313	rBV	201	56	0.00%	0.000%
57	8.619	2353	2357	2360	rBV2	472	388	0.03%	0.003%
58	8.693	2378	2380	2381	rBV2	184	84	0.01%	0.001%
59	8.715	2385	2387	2388	rBV	200	68	0.00%	0.001%
60	8.783	2396	2408	2436	rBV	585804	962593	62.51%	8.457%
61	9.050	2489	2491	2494	rVB2	184	82	0.01%	0.001%
62	9.072	2494	2498	2502	rBV	445	309	0.02%	0.003%
63	9.130	2513	2516	2517	rBV2	93	47	0.00%	0.000%
64	9.153	2517	2523	2525	rVV3	243	289	0.02%	0.003%
65	9.194	2535	2536	2538	rBV	126	69	0.00%	0.001%
66	9.474	2621	2623	2627	rBV2	184	88	0.01%	0.001%
67	9.564	2648	2651	2653	rBV	146	98	0.01%	0.001%
68	9.648	2675	2677	2679	rBV	146	92	0.01%	0.001%
69	9.715	2694	2698	2703	rBV2	232	243	0.02%	0.002%
70	9.831	2731	2734	2738	rBV2	270	236	0.02%	0.002%
71	9.879	2746	2749	2752	rVB4	435	269	0.02%	0.002%
72	10.027	2793	2795	2800	rVB	260	151	0.01%	0.001%
73	10.149	2822	2833	2856	rBV	431988	678858	44.08%	5.965%
74	10.426	2916	2919	2925	rVB	317	262	0.02%	0.002%
75	10.452	2925	2927	2930	rBV2	117	84	0.01%	0.001%
76	10.506	2941	2944	2945	rBV	143	61	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034724.D
 Acq On : 19 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1766-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.661	2988	2992	2995	rBV2	210	173	0.01%	0.002%
78	10.741	3013	3017	3019	rBV	231	206	0.01%	0.002%
79	10.754	3020	3021	3024	rVB	275	69	0.00%	0.001%
80	10.773	3024	3027	3030	rBV	256	214	0.01%	0.002%
81	11.185	3144	3155	3178	rBV	550127	871444	56.59%	7.657%
82	11.558	3259	3271	3298	rBV	645838	1030159	66.90%	9.051%
83	11.786	3340	3342	3350	rVB3	328	306	0.02%	0.003%
84	11.892	3368	3375	3379	rBV2	338	458	0.03%	0.004%
85	12.085	3432	3435	3437	rBV	218	96	0.01%	0.001%
86	12.133	3448	3450	3455	rVB	349	162	0.01%	0.001%
87	12.529	3571	3573	3574	rBV	181	62	0.00%	0.001%
88	12.812	3659	3661	3663	rBV	263	123	0.01%	0.001%
89	13.117	3750	3756	3757	rBV2	383	361	0.02%	0.003%
90	13.204	3780	3783	3784	rBV2	562	315	0.02%	0.003%
91	13.291	3807	3810	3813	rVB2	480	293	0.02%	0.003%
92	13.310	3813	3816	3817	rBV	288	151	0.01%	0.001%
93	13.451	3853	3860	3862	rBV3	2400	2386	0.15%	0.021%
94	13.815	3971	3973	3975	rBV	329	171	0.01%	0.002%
95	14.455	4170	4172	4174	rBV2	425	188	0.01%	0.002%




Sum of corrected areas: 11381574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034724.D
Acq On : 19 Mar 2024 10:49
Operator : SY/MD
Sample : P1766-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

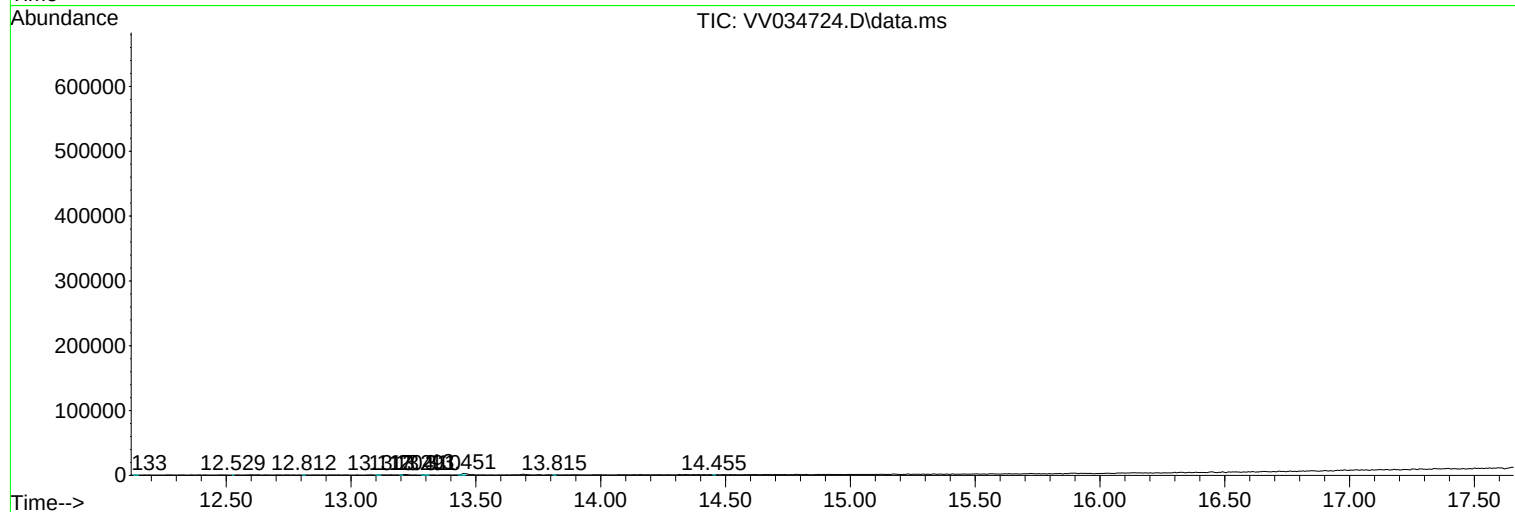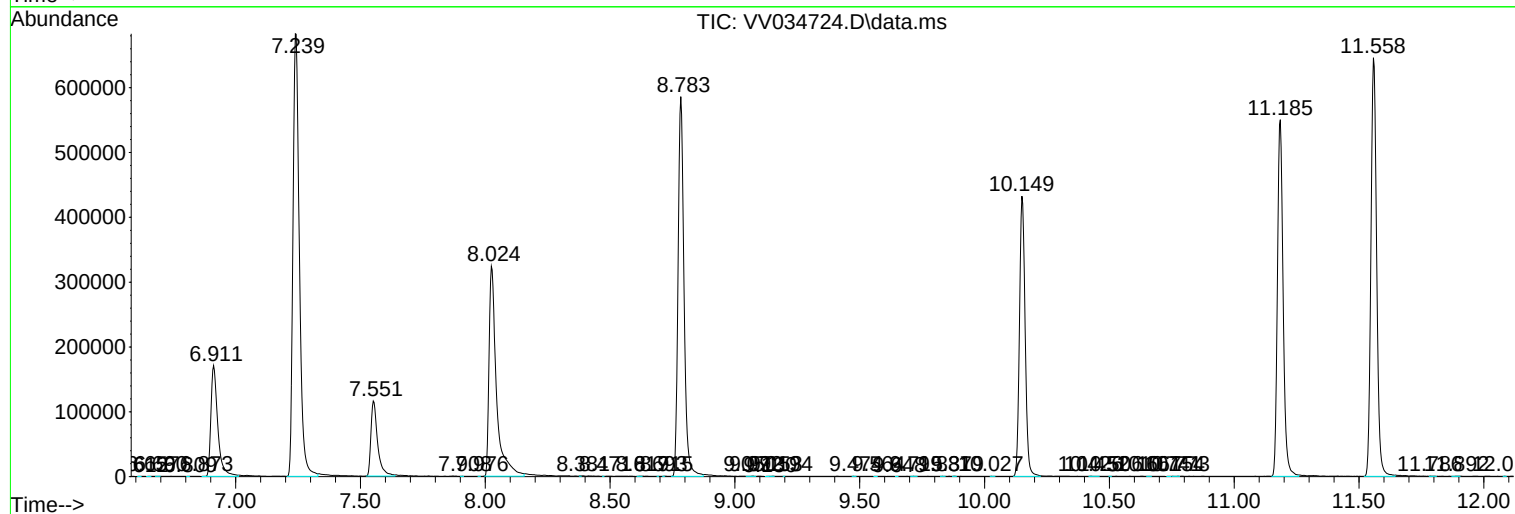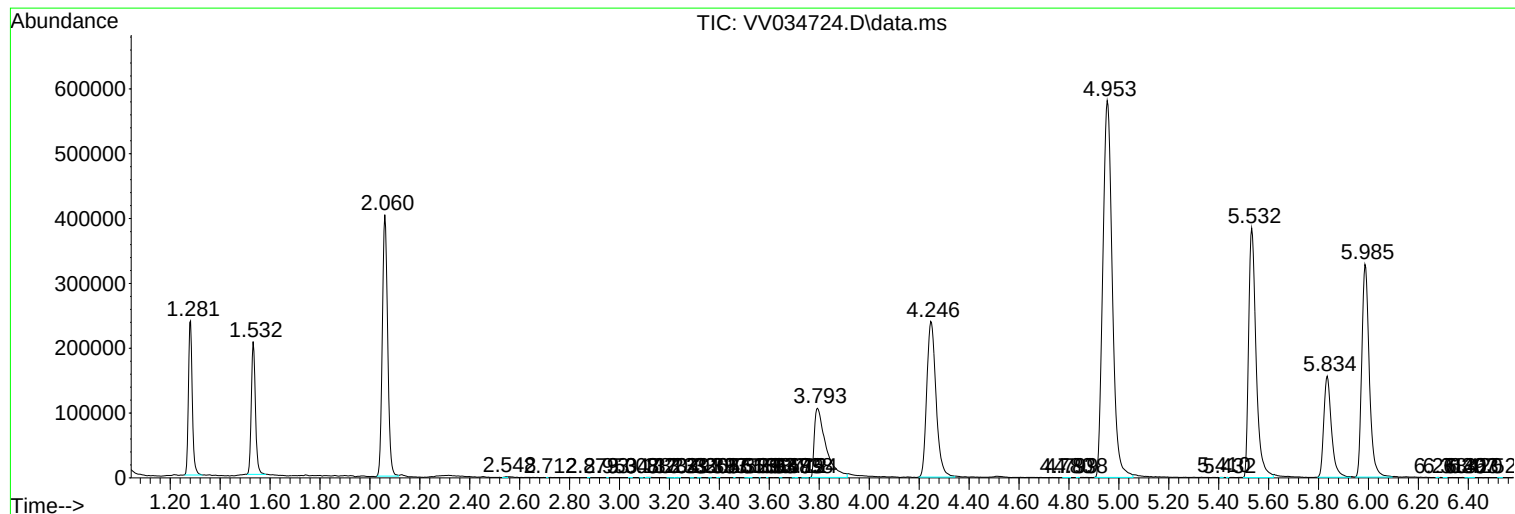

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034724.D
Acq On : 19 Mar 2024 10:49
Operator : SY/MD
Sample : P1766-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034724.D
Acq On : 19 Mar 2024 10:49
Operator : SY/MD
Sample : P1766-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc