

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034725.D
 Acq On : 19 Mar 2024 11:13
 Operator : SY/MD
 Sample : P1766-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	236165	245705	15.86%	2.200%
2	1.532	146	153	172	rVB	199726	229307	14.81%	2.053%
3	1.960	283	286	287	rBV	933	531	0.03%	0.005%
4	2.060	307	317	336	rBV	389468	563429	36.38%	5.044%
5	2.513	455	458	460	rBV	167	109	0.01%	0.001%
6	2.552	466	470	474	rBV4	397	459	0.03%	0.004%
7	2.622	491	492	497	rBV	151	113	0.01%	0.001%
8	2.754	530	533	535	rBV2	167	92	0.01%	0.001%
9	2.790	541	544	545	rBV	148	66	0.00%	0.001%
10	2.835	553	558	560	rBV	195	197	0.01%	0.002%
11	3.095	635	639	640	rBV	142	86	0.01%	0.001%
12	3.130	647	650	652	rBV	114	81	0.01%	0.001%
13	3.172	658	663	664	rBV	75	69	0.00%	0.001%
14	3.230	680	681	684	rBV2	135	54	0.00%	0.000%
15	3.249	684	687	691	rBV2	101	100	0.01%	0.001%
16	3.314	705	707	708	rVB	206	55	0.00%	0.000%
17	3.333	708	713	714	rBV2	187	146	0.01%	0.001%
18	3.359	719	721	723	rVV	233	114	0.01%	0.001%
19	3.384	726	729	733	rBV2	153	111	0.01%	0.001%
20	3.494	761	763	764	rBV2	243	102	0.01%	0.001%
21	3.529	771	774	777	rBV	186	103	0.01%	0.001%
22	3.642	805	809	812	rBV	219	170	0.01%	0.002%
23	3.761	843	846	847	rBV	108	59	0.00%	0.001%
24	3.789	847	855	901	rBV	110850	331052	21.38%	2.964%
25	4.246	981	997	1036	rBV	240062	621923	40.16%	5.568%
26	4.690	1131	1135	1136	rBV	327	217	0.01%	0.002%
27	4.728	1145	1147	1150	rBV2	164	68	0.00%	0.001%
28	4.802	1166	1170	1174	rBV2	317	365	0.02%	0.003%
29	4.873	1187	1192	1195	rBV2	255	268	0.02%	0.002%
30	4.953	1201	1217	1250	rBV2	581959	1548738	100.00%	13.865%
31	5.394	1351	1354	1356	rBV3	405	283	0.02%	0.003%
32	5.436	1365	1367	1372	rVB2	238	135	0.01%	0.001%
33	5.532	1385	1397	1426	rBV	382737	793206	51.22%	7.101%
34	5.831	1480	1490	1512	rBV2	11429	25024	1.62%	0.224%
35	5.986	1525	1538	1571	rBV	337498	695472	44.91%	6.226%
36	6.240	1614	1617	1620	rBB	510	290	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034725.D
 Acq On : 19 Mar 2024 11:13
 Operator : SY/MD
 Sample : P1766-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.420	1669	1673	1675	rBV2	356	203	0.01%	0.002%
38	6.484	1690	1693	1696	rBV2	243	157	0.01%	0.001%
39	6.522	1703	1705	1711	rVB	289	251	0.02%	0.002%
40	6.551	1711	1714	1717	rBV2	125	99	0.01%	0.001%
41	6.574	1718	1721	1726	rVV	180	128	0.01%	0.001%
42	6.600	1726	1729	1734	rVV2	169	133	0.01%	0.001%
43	6.638	1739	1741	1742	rBV	214	74	0.00%	0.001%
44	6.664	1747	1749	1752	rBV	140	76	0.00%	0.001%
45	6.696	1758	1759	1763	rVB	237	123	0.01%	0.001%
46	6.844	1801	1805	1806	rBV	167	100	0.01%	0.001%
47	6.912	1815	1826	1852	rBV	185681	346588	22.38%	3.103%
48	7.239	1917	1928	1961	rBV	674018	1208738	78.05%	10.821%
49	7.551	2016	2025	2048	rBV	125933	228589	14.76%	2.046%
50	7.776	2093	2095	2097	rBV	447	272	0.02%	0.002%
51	7.834	2111	2113	2116	rBV2	191	107	0.01%	0.001%
52	7.944	2144	2147	2150	rBV2	178	160	0.01%	0.001%
53	7.973	2153	2156	2157	rBV2	199	111	0.01%	0.001%
54	8.024	2163	2172	2214	rBV	347820	703739	45.44%	6.300%
55	8.487	2310	2316	2319	rBV3	345	423	0.03%	0.004%
56	8.545	2331	2334	2336	rBV	494	303	0.02%	0.003%
57	8.648	2362	2366	2369	rBV2	268	196	0.01%	0.002%
58	8.696	2379	2381	2383	rBV	208	104	0.01%	0.001%
59	8.731	2388	2392	2395	rBV2	364	307	0.02%	0.003%
60	8.783	2397	2408	2435	rBV	583198	971812	62.75%	8.700%
61	9.394	2596	2598	2600	rBV	119	66	0.00%	0.001%
62	9.474	2620	2623	2625	rBV2	246	135	0.01%	0.001%
63	9.542	2641	2644	2646	rBV	95	58	0.00%	0.001%
64	9.558	2646	2649	2651	rBV	217	139	0.01%	0.001%
65	9.574	2652	2654	2659	rVB2	331	204	0.01%	0.002%
66	9.683	2684	2688	2691	rVB2	196	119	0.01%	0.001%
67	9.770	2711	2715	2717	rBV	182	144	0.01%	0.001%
68	9.895	2751	2754	2756	rBV2	159	124	0.01%	0.001%
69	9.947	2767	2770	2771	rBV2	100	55	0.00%	0.000%
70	9.989	2781	2783	2785	rBV	143	61	0.00%	0.001%
71	10.149	2822	2833	2858	rBV	445323	700552	45.23%	6.272%
72	10.458	2928	2929	2931	rBV	180	76	0.00%	0.001%
73	10.561	2959	2961	2964	rBV2	236	100	0.01%	0.001%
74	10.606	2973	2975	2976	rBV	231	61	0.00%	0.001%
75	10.683	2997	2999	3003	rBB2	214	122	0.01%	0.001%
76	10.706	3003	3006	3009	rBV2	186	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034725.D
 Acq On : 19 Mar 2024 11:13
 Operator : SY/MD
 Sample : P1766-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.870	3054	3057	3060	rBV	156	143	0.01%	0.001%
78	11.066	3115	3118	3120	rBV	221	138	0.01%	0.001%
79	11.101	3126	3129	3131	rBV2	178	98	0.01%	0.001%
80	11.120	3134	3135	3136	rVB	284	55	0.00%	0.000%
81	11.133	3136	3139	3141	rBV	306	142	0.01%	0.001%
82	11.185	3144	3155	3183	rBV	572779	891930	57.59%	7.985%
83	11.461	3237	3241	3244	rBV2	328	216	0.01%	0.002%
84	11.558	3259	3271	3306	rBV	665825	1051356	67.88%	9.412%
85	11.799	3343	3346	3350	rBV	396	300	0.02%	0.003%
86	11.934	3385	3388	3390	rBV	177	136	0.01%	0.001%
87	12.079	3432	3433	3434	rVB	290	56	0.00%	0.001%
88	12.152	3452	3456	3461	rBV2	422	336	0.02%	0.003%
89	12.291	3496	3499	3501	rBV2	321	202	0.01%	0.002%
90	12.445	3545	3547	3549	rVB	200	74	0.00%	0.001%
91	12.596	3592	3594	3597	rVB2	292	147	0.01%	0.001%
92	12.731	3634	3636	3638	rBV2	216	79	0.01%	0.001%
93	12.799	3655	3657	3659	rBV	239	139	0.01%	0.001%
94	12.847	3669	3672	3675	rBV	307	201	0.01%	0.002%
95	12.950	3701	3704	3711	rBV	342	258	0.02%	0.002%
96	13.107	3751	3753	3756	rVB2	316	85	0.01%	0.001%
97	13.268	3801	3803	3805	rBV	188	92	0.01%	0.001%
98	13.316	3815	3818	3820	rBV2	211	153	0.01%	0.001%
99	13.686	3929	3933	3934	rBV2	737	438	0.03%	0.004%
100	14.657	4233	4235	4237	rBV2	454	190	0.01%	0.002%


Sum of corrected areas: 11170192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034725.D
Acq On : 19 Mar 2024 11:13
Operator : SY/MD
Sample : P1766-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

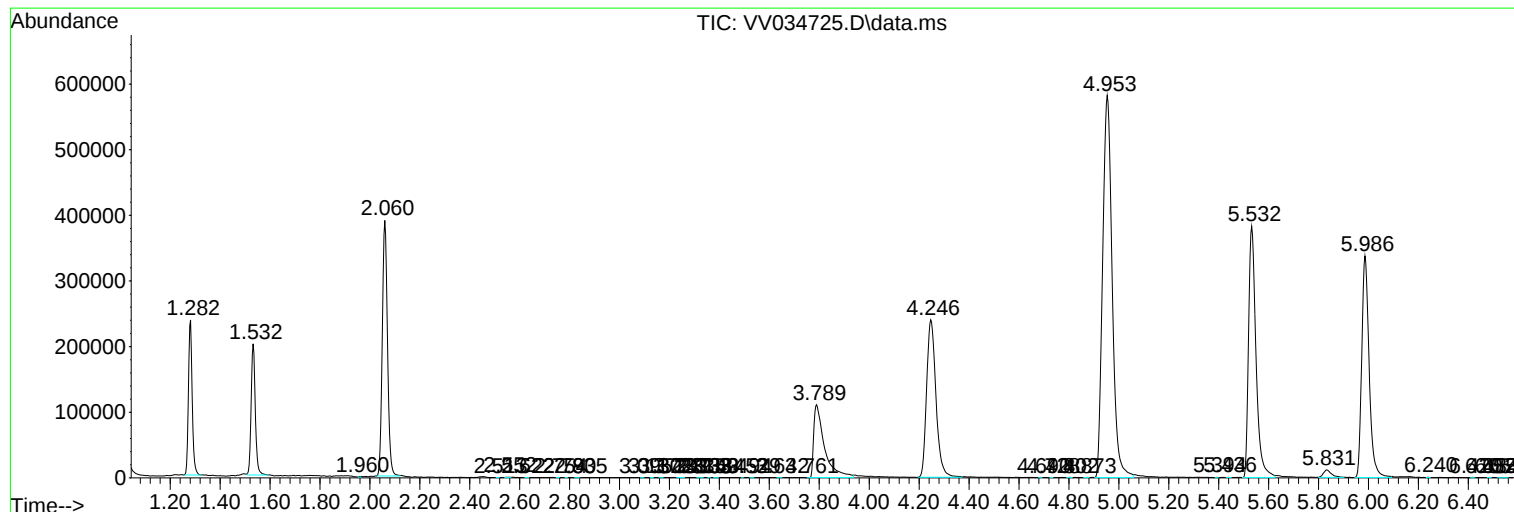

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034725.D
Acq On : 19 Mar 2024 11:13
Operator : SY/MD
Sample : P1766-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034725.D
Acq On : 19 Mar 2024 11:13
Operator : SY/MD
Sample : P1766-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc