

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034744.D
 Acq On : 19 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1755-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	204882	219510	15.57%	1.983%
2	1.529	145	152	163	rVB	172057	201517	14.30%	1.821%
3	2.060	306	317	326	rBV	347820	500783	35.53%	4.525%
4	2.114	327	334	360	rVV	213940	349110	24.77%	3.154%
5	2.240	362	373	405	rVV	123147	357790	25.38%	3.233%
6	2.741	527	529	533	rBV2	339	237	0.02%	0.002%
7	2.764	533	536	537	rBV2	299	129	0.01%	0.001%
8	2.867	566	568	569	rBV	164	73	0.01%	0.001%
9	2.998	606	609	615	rVB	218	196	0.01%	0.002%
10	3.121	639	647	649	rBV2	555	599	0.04%	0.005%
11	3.162	657	660	661	rBV2	202	91	0.01%	0.001%
12	3.217	675	677	678	rBV2	76	34	0.00%	0.000%
13	3.269	690	693	696	rBV2	272	155	0.01%	0.001%
14	3.407	733	736	737	rBV	93	55	0.00%	0.000%
15	3.458	748	752	754	rBV	225	120	0.01%	0.001%
16	3.474	754	757	758	rBV	217	82	0.01%	0.001%
17	3.577	786	789	792	rBV2	160	99	0.01%	0.001%
18	3.597	792	795	797	rBV2	134	93	0.01%	0.001%
19	3.642	807	809	814	rBV2	137	60	0.00%	0.001%
20	3.677	818	820	824	rVB	141	93	0.01%	0.001%
21	3.703	824	828	829	rBV2	300	122	0.01%	0.001%
22	3.751	839	843	846	rBV2	149	133	0.01%	0.001%
23	3.786	846	854	882	rBV	101668	279015	19.80%	2.521%
24	4.246	983	997	1030	rBV	222324	573638	40.70%	5.183%
25	4.722	1143	1145	1148	rBB	188	79	0.01%	0.001%
26	4.818	1174	1175	1177	rVB	397	128	0.01%	0.001%
27	4.834	1177	1180	1183	rBV	210	116	0.01%	0.001%
28	4.953	1200	1217	1249	rBV2	526570	1409494	100.00%	12.735%
29	5.532	1386	1397	1432	rBV	391335	807358	57.28%	7.295%
30	5.834	1481	1491	1510	rBV4	10195	22044	1.56%	0.199%
31	5.985	1526	1538	1571	rBV	303732	628952	44.62%	5.683%
32	6.285	1628	1631	1634	rBV	217	157	0.01%	0.001%
33	6.432	1675	1677	1680	rBV2	271	138	0.01%	0.001%
34	6.612	1729	1733	1737	rVB2	335	263	0.02%	0.002%
35	6.632	1737	1739	1741	rBV	96	60	0.00%	0.001%
36	6.654	1741	1746	1748	rBV	195	171	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034744.D
 Acq On : 19 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1755-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.706	1758	1762	1765	rBV2	142	119	0.01%	0.001%
38	6.754	1776	1777	1778	rBV	208	44	0.00%	0.000%
39	6.770	1779	1782	1786	rBV	143	136	0.01%	0.001%
40	6.821	1795	1798	1801	rBV	306	204	0.01%	0.002%
41	6.866	1811	1812	1813	rVB	97	19	0.00%	0.000%
42	6.912	1815	1826	1860	rBV	160891	311550	22.10%	2.815%
43	7.166	1900	1905	1908	rBV2	425	381	0.03%	0.003%
44	7.243	1917	1929	1961	rBV	615138	1094535	77.65%	9.889%
45	7.551	2016	2025	2052	rBV	111018	208457	14.79%	1.883%
46	7.821	2105	2109	2113	rVB4	442	307	0.02%	0.003%
47	7.847	2114	2117	2119	rBV	332	178	0.01%	0.002%
48	7.918	2136	2139	2142	rBV2	337	211	0.01%	0.002%
49	7.953	2146	2150	2154	rVB2	397	317	0.02%	0.003%
50	7.973	2154	2156	2161	rVB2	285	190	0.01%	0.002%
51	7.992	2161	2162	2163	rBV	186	47	0.00%	0.000%
52	8.024	2163	2172	2207	rBV	315778	620347	44.01%	5.605%
53	8.513	2320	2324	2326	rBV2	300	274	0.02%	0.002%
54	8.555	2334	2337	2338	rBV2	110	54	0.00%	0.000%
55	8.561	2338	2339	2340	rBV	211	57	0.00%	0.001%
56	8.651	2364	2367	2368	rBV	325	170	0.01%	0.002%
57	8.683	2375	2377	2378	rBV	252	76	0.01%	0.001%
58	8.709	2382	2385	2387	rBV	241	188	0.01%	0.002%
59	8.783	2395	2408	2438	rBV	586292	969506	68.78%	8.760%
60	9.091	2501	2504	2506	rBV	338	156	0.01%	0.001%
61	9.117	2510	2512	2518	rVB2	430	329	0.02%	0.003%
62	9.233	2544	2548	2552	rBV2	242	171	0.01%	0.002%
63	9.255	2552	2555	2557	rBV	261	140	0.01%	0.001%
64	9.317	2571	2574	2576	rBV	114	63	0.00%	0.001%
65	9.397	2595	2599	2601	rBV2	241	131	0.01%	0.001%
66	9.413	2601	2604	2606	rBV2	183	127	0.01%	0.001%
67	9.548	2643	2646	2648	rBV	147	99	0.01%	0.001%
68	9.632	2670	2672	2675	rBV2	162	106	0.01%	0.001%
69	9.866	2743	2745	2748	rVB2	311	166	0.01%	0.001%
70	9.889	2749	2752	2753	rBV	239	131	0.01%	0.001%
71	9.956	2766	2773	2784	rBV3	1071	1894	0.13%	0.017%
72	10.040	2796	2799	2801	rBV2	165	108	0.01%	0.001%
73	10.153	2822	2834	2858	rBV	406713	641350	45.50%	5.795%
74	10.452	2921	2927	2929	rBV2	266	261	0.02%	0.002%
75	10.500	2939	2942	2947	rVB	253	180	0.01%	0.002%
76	10.529	2950	2951	2952	rBV	130	34	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034744.D
 Acq On : 19 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1755-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.735	3013	3015	3017	rBV	210	73	0.01%	0.001%
78	10.808	3036	3038	3041	rBV	225	110	0.01%	0.001%
79	10.902	3063	3067	3069	rBV	282	209	0.01%	0.002%
80	10.963	3083	3086	3088	rBV	328	218	0.02%	0.002%
81	11.075	3115	3121	3124	rVB2	317	353	0.03%	0.003%
82	11.104	3124	3130	3132	rBV2	320	377	0.03%	0.003%
83	11.185	3144	3155	3188	rBV	569098	890161	63.15%	8.043%
84	11.480	3244	3247	3248	rBV	270	134	0.01%	0.001%
85	11.516	3253	3258	3259	rBV3	910	558	0.04%	0.005%
86	11.558	3260	3271	3295	rVV	602887	966429	68.57%	8.732%
87	11.754	3329	3332	3339	rVB2	746	630	0.04%	0.006%
88	11.841	3357	3359	3361	rBV	346	120	0.01%	0.001%
89	11.934	3385	3388	3394	rBV2	272	278	0.02%	0.003%
90	12.024	3411	3416	3418	rBV2	328	281	0.02%	0.003%
91	12.127	3444	3448	3453	rBV3	375	405	0.03%	0.004%
92	12.146	3453	3454	3455	rBV	313	66	0.00%	0.001%
93	12.188	3463	3467	3468	rBV	306	206	0.01%	0.002%
94	12.458	3549	3551	3556	rVB4	714	601	0.04%	0.005%
95	12.670	3614	3617	3621	rBV	333	258	0.02%	0.002%
96	12.927	3690	3697	3699	rBV	292	357	0.03%	0.003%
97	13.024	3724	3727	3729	rBV	375	203	0.01%	0.002%
98	13.123	3756	3758	3759	rBV2	214	66	0.00%	0.001%
99	13.927	4004	4008	4011	rBV4	390	301	0.02%	0.003%




Sum of corrected areas: 11067901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034744.D
Acq On : 19 Mar 2024 18:45
Operator : SY/MD
Sample : P1755-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

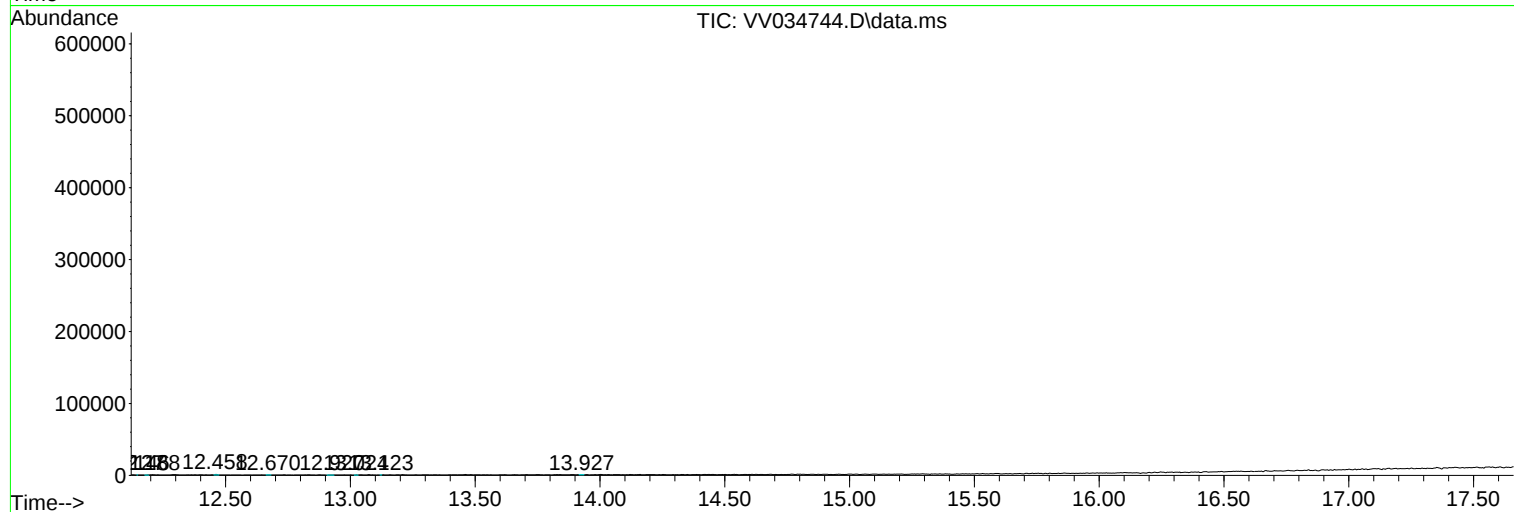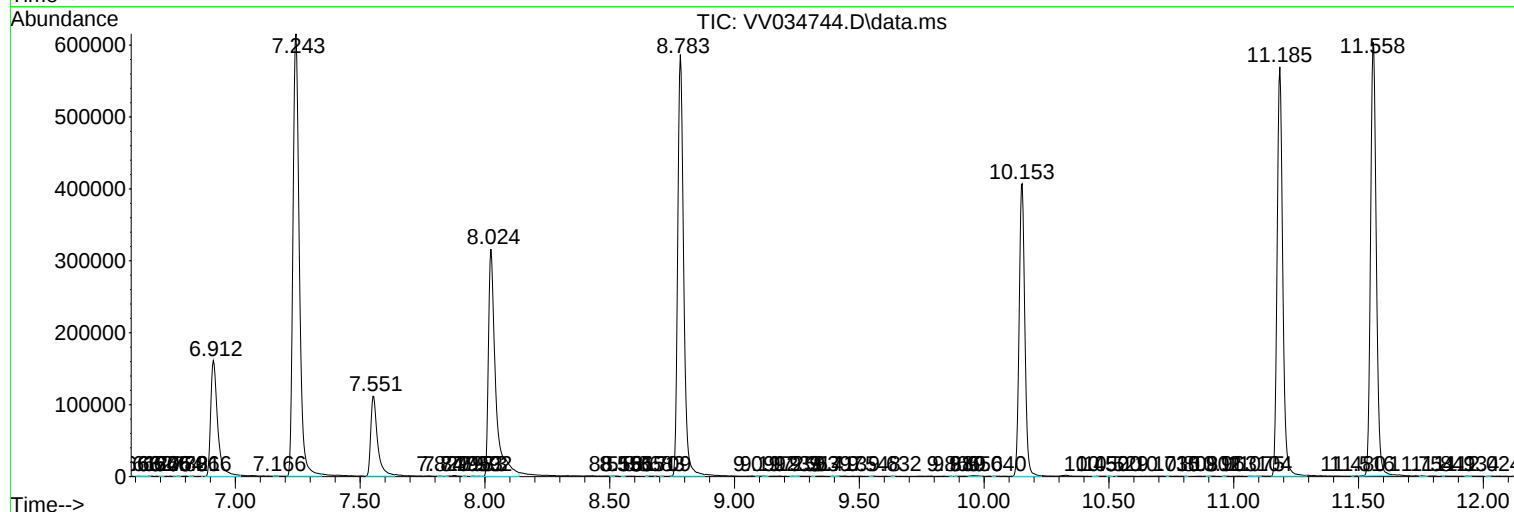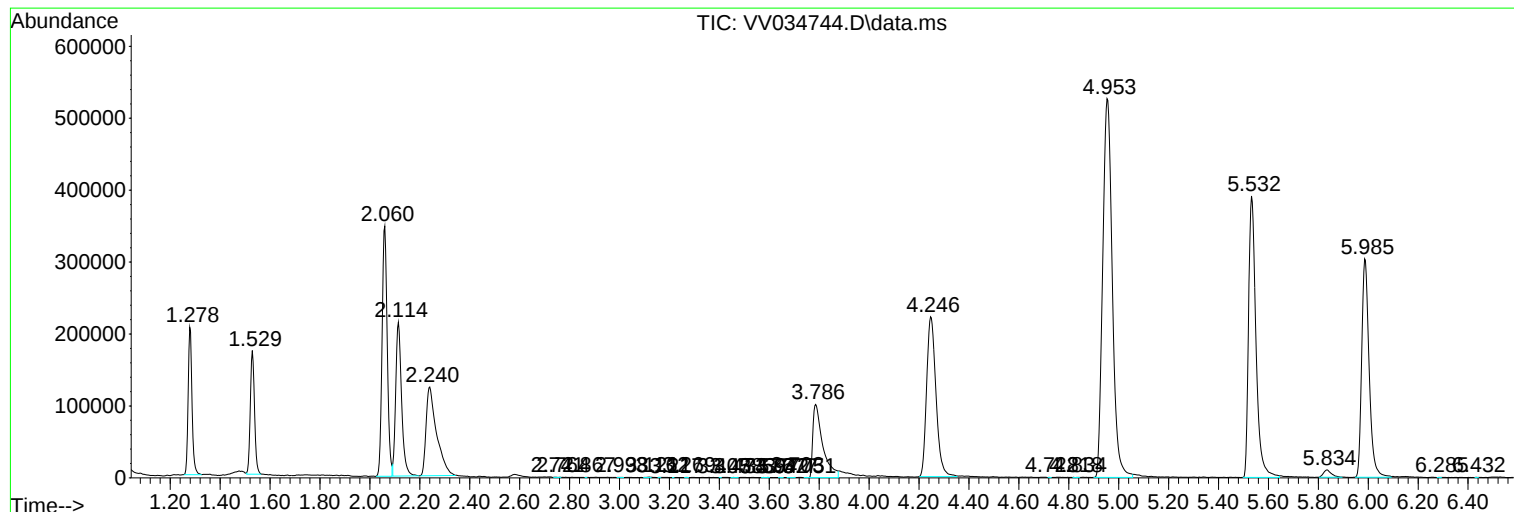

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034744.D
Acq On : 19 Mar 2024 18:45
Operator : SY/MD
Sample : P1755-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKW0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	22.16 ug/L	357790	1,4-Difluorobenzene	5.532

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
4			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	56

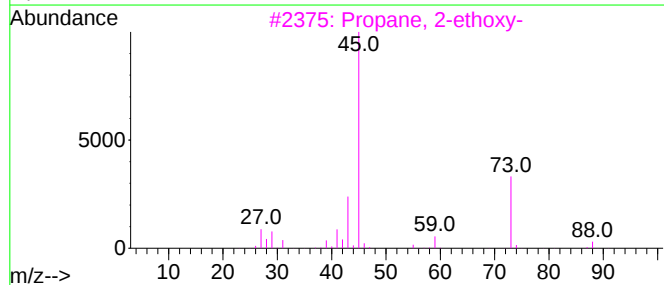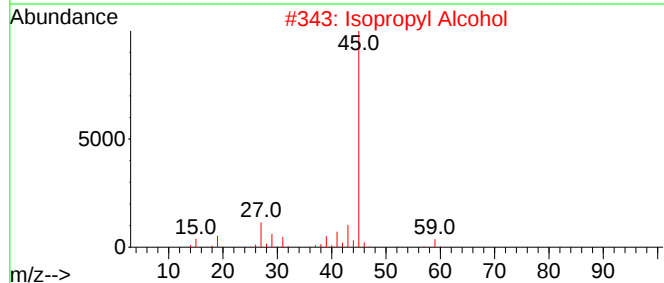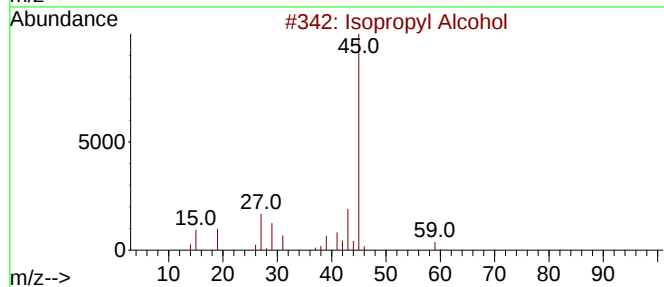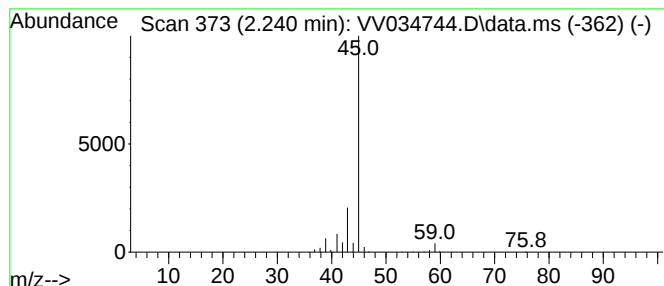

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034744.D
Acq On : 19 Mar 2024 18:45
Operator : SY/MD
Sample : P1755-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.240	22.2	ug/L	357790	1	5.532	807358	50.0