


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034694.D
Acq On : 18 Mar 2024 12:54
Operator : SY/MD
Sample : BFB270
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB270

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Wed Mar 20 01:19:21 2024

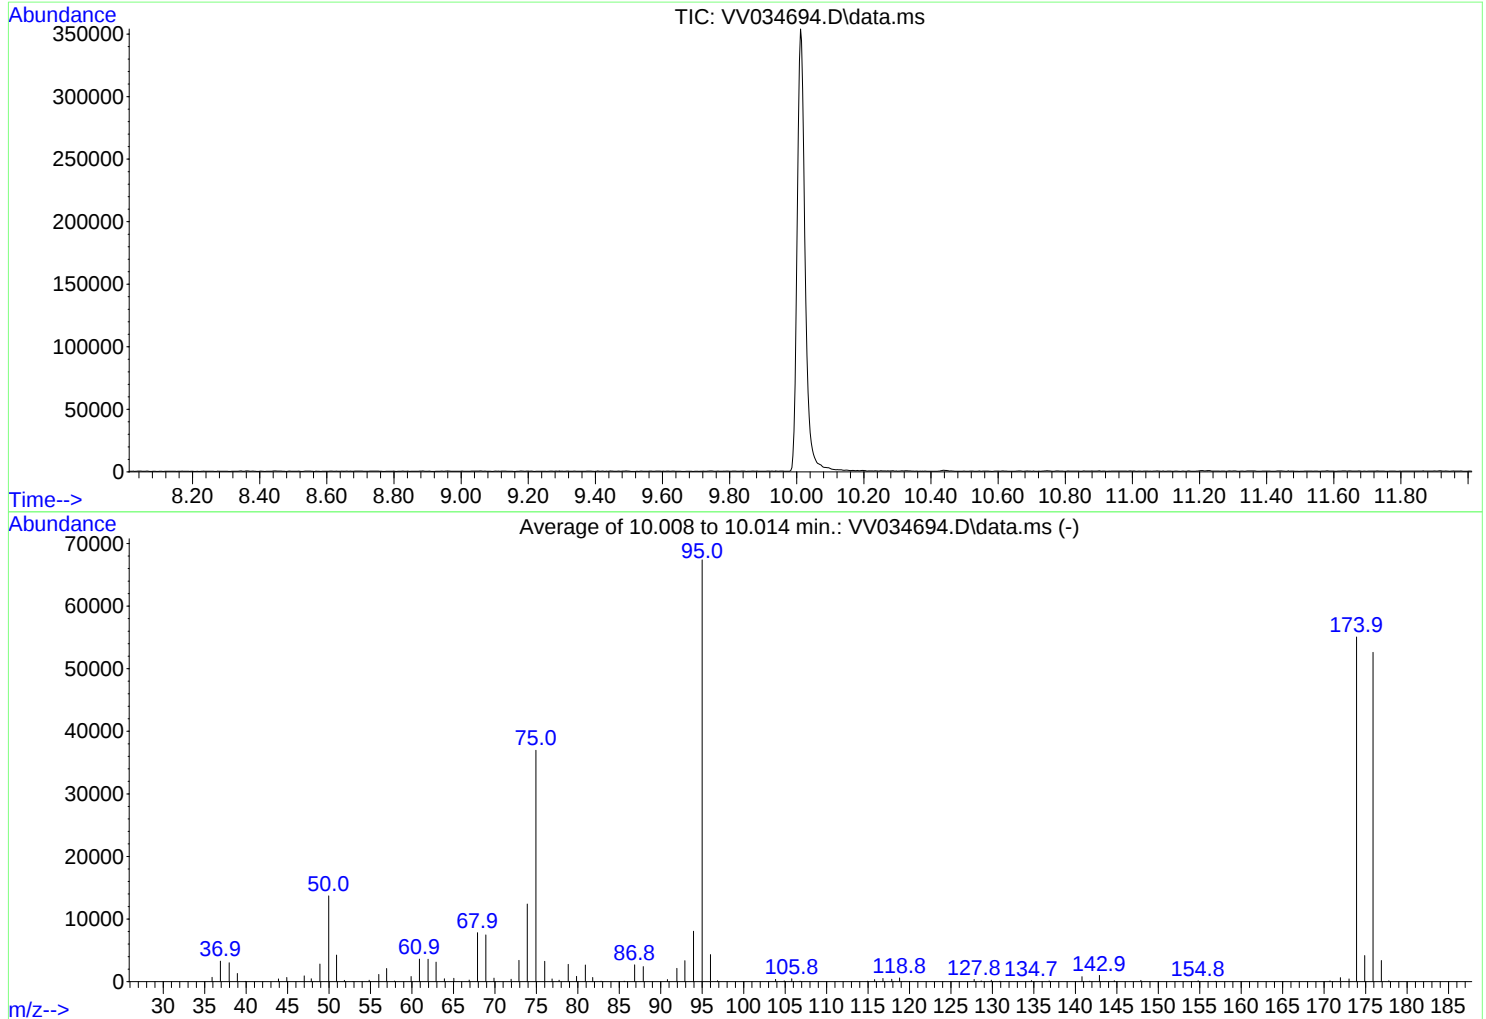

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	13702	PASS
75	95	30	80	54.9	36973	PASS
95	95	100	100	100.0	67397	PASS
96	95	5	9	6.4	4314	PASS
173	174	0.00	2	0.8	442	PASS
174	95	50	120	81.7	55056	PASS
175	174	5	9	7.6	4164	PASS
176	174	95	105	95.6	52611	PASS
177	176	5	10	6.4	3387	PASS

m/z	Abundance
39.80	224.0
43.90	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	631.0
36.90	3329.0
38.00	2913.0
38.90	1346.0
40.00	288.0
43.90	710.0
44.90	606.0
47.00	821.0
47.90	466.0
48.90	2744.0
49.90	13275.0
50.90	4153.0
51.90	161.0
54.80	275.0
56.00	1199.0
56.90	2042.0
59.90	784.0
60.90	3694.0
61.90	3597.0
62.90	3089.0
63.90	484.0
65.00	553.0
66.90	206.0
67.90	7609.0
68.90	7075.0
69.90	573.0
71.90	383.0
72.90	3261.0
73.90	12165.0
75.00	36176.0
76.00	3055.0
76.90	467.0
77.80	211.0
78.90	2683.0
79.80	741.0
80.90	2609.0
81.80	683.0
82.80	105.0
85.60	103.0
86.80	2514.0
87.90	2299.0
90.80	352.0
91.90	1971.0
92.90	3135.0
94.00	7883.0
95.00	64728.0
96.00	4259.0
96.80	134.0
103.90	395.0
104.90	109.0
105.80	483.0
115.80	277.0
116.80	503.0
117.90	365.0
118.80	522.0
127.80	367.0
128.60	119.0
129.90	210.0
134.70	178.0
136.90	127.0
140.80	762.0
142.90	941.0
144.70	124.0
147.90	212.0
154.80	179.0
170.70	119.0
171.90	573.0
173.00	651.0
173.90	51456.0
174.90	3853.0
175.90	49552.0
176.90	3322.0
177.80	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	733.0
36.90	3332.0
38.00	3116.0
38.90	1359.0
40.00	298.0
43.90	765.0
44.90	708.0
47.00	994.0
47.80	475.0
48.90	2901.0
50.00	14083.0
50.90	4371.0
51.80	211.0
52.90	115.0
54.80	241.0
56.00	1190.0
56.90	2152.0
57.90	139.0
59.90	852.0
60.90	3715.0
61.90	3678.0
62.90	3254.0
63.90	499.0
65.00	587.0
66.90	252.0
67.90	8161.0
68.90	7759.0
69.90	560.0
72.00	410.0
72.90	3498.0
73.90	12701.0
74.90	38152.0
76.00	3379.0
76.90	462.0
77.80	243.0
78.80	2834.0
79.90	883.0
80.90	2686.0
81.80	692.0
82.80	106.0
85.60	108.0
86.80	2727.0
87.90	2542.0
90.80	356.0
91.90	2223.0
92.90	3469.0
94.00	8326.0
95.00	69784.0
96.00	4451.0
96.80	161.0
103.90	369.0
104.90	141.0
105.80	493.0
106.80	123.0
114.90	115.0
115.80	341.0
116.80	512.0
117.90	401.0
118.80	604.0
127.80	374.0
128.70	139.0
129.80	223.0
130.90	131.0
134.70	175.0
136.80	111.0
140.80	836.0
141.70	105.0
142.90	1044.0
144.70	188.0
147.90	223.0
154.80	164.0
170.70	135.0
171.90	659.0
173.00	675.0
173.90	56952.0
174.90	4292.0
175.90	54200.0
176.90	3436.0
177.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	694.0
36.90	3145.0
37.90	3032.0
39.00	1231.0
40.00	264.0
43.90	779.0
44.90	687.0
47.00	948.0
47.80	462.0
48.90	2814.0
49.90	13749.0
50.90	4200.0
51.80	228.0
54.90	207.0
56.00	1101.0
57.00	2076.0
57.90	166.0
59.90	804.0
60.90	3407.0
62.00	3435.0
62.90	3035.0
63.90	403.0
65.10	509.0
66.90	273.0
67.90	7721.0
68.90	7600.0
69.90	549.0
71.90	397.0
72.90	3482.0
73.90	12347.0
74.90	36592.0
76.00	3334.0
76.90	382.0
77.70	243.0
78.80	2770.0
79.90	949.0
80.90	2654.0
81.80	629.0
86.90	2831.0
87.90	2401.0
90.80	305.0
92.00	2146.0
92.90	3419.0
93.90	7962.0
95.00	67680.0
96.00	4233.0
96.90	146.0
103.80	345.0
104.90	145.0
105.80	445.0
106.80	111.0
115.00	118.0
115.80	362.0
116.80	490.0
117.80	395.0
118.80	641.0
127.80	321.0
128.70	129.0
129.80	240.0
130.90	111.0
134.70	156.0
136.80	120.0
140.80	779.0
141.80	130.0
142.90	991.0
144.70	182.0
147.90	199.0
154.80	151.0
156.90	150.0
170.70	111.0
172.00	680.0
173.90	56760.0
174.90	4347.0
175.90	54080.0
176.90	3402.0
177.80	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270