
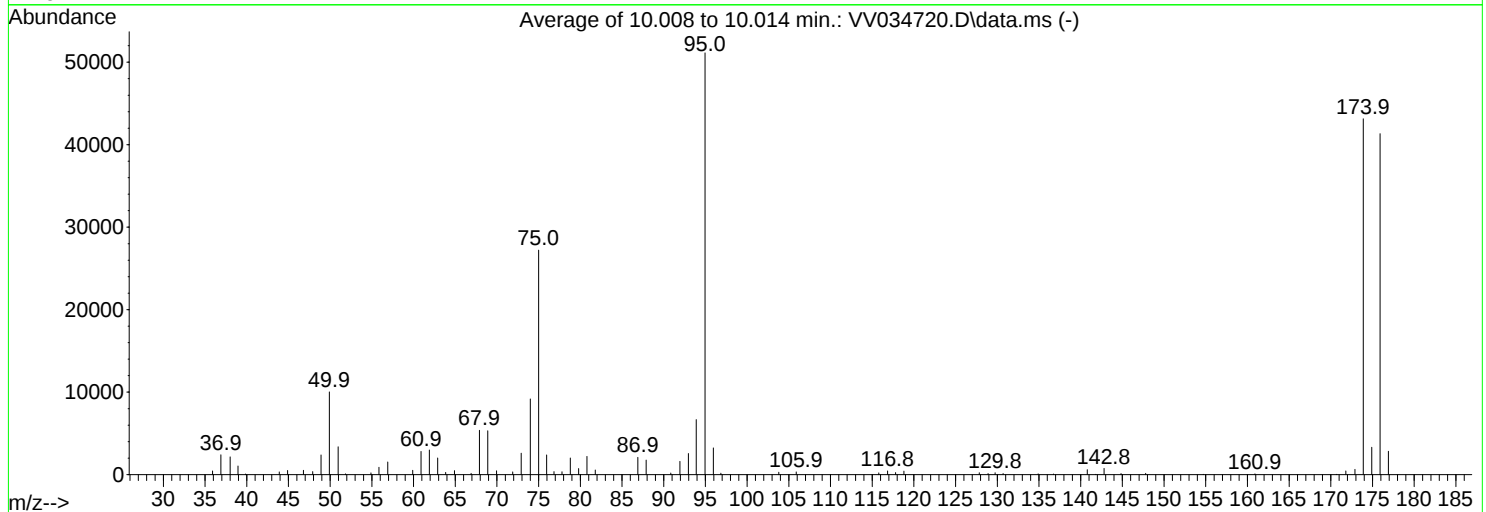


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034720.D
Acq On : 19 Mar 2024 08:30
Operator : SY/MD
Sample : BFB271
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB271

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Wed Mar 20 01:19:21 2024

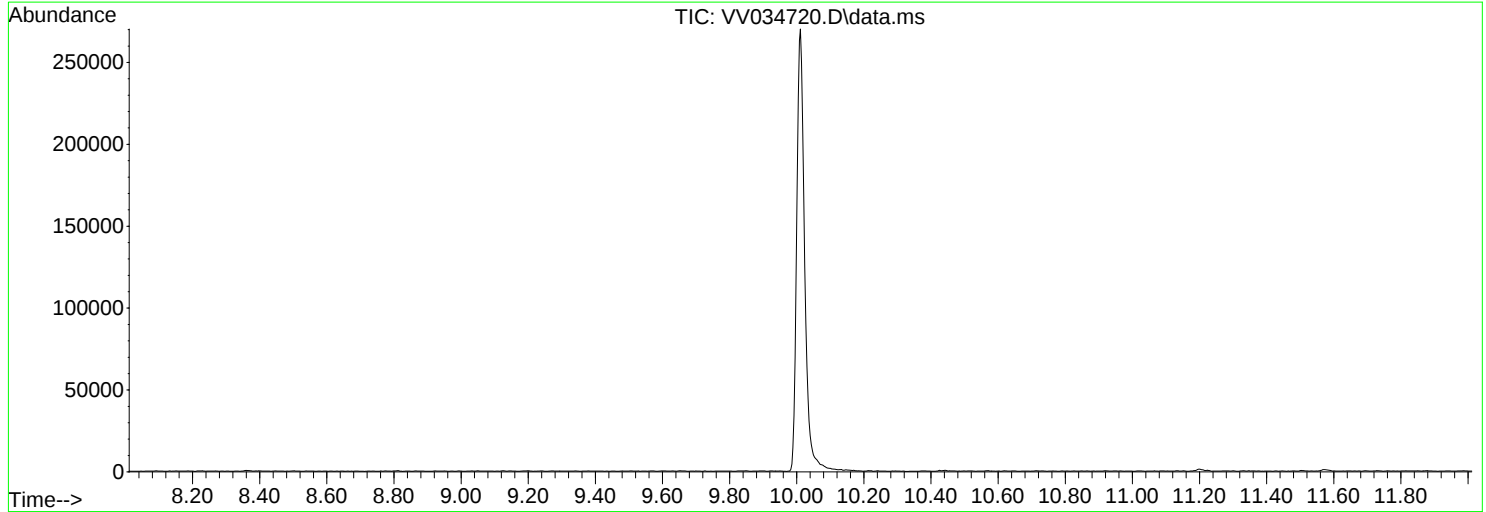

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10035	PASS
75	95	30	80	53.2	27208	PASS
95	95	100	100	100.0	51136	PASS
96	95	5	9	6.3	3245	PASS
173	174	0.00	2	1.5	648	PASS
174	95	50	120	84.4	43141	PASS
175	174	5	9	7.7	3320	PASS
176	174	95	105	95.8	41328	PASS
177	176	5	10	6.8	2829	PASS

m/z	Abundance
39.80	228.0
43.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
35.90	490.0
36.90	2551.0
38.00	2092.0
39.00	984.0
39.90	343.0
43.90	633.0
44.90	542.0
46.80	588.0
47.90	361.0
48.90	2540.0
49.90	10326.0
50.90	3396.0
51.80	175.0
54.90	266.0
55.80	862.0
56.90	1558.0
59.90	526.0
60.90	2859.0
61.90	2966.0
62.90	2124.0
63.80	277.0
64.90	448.0
66.90	141.0
67.90	5335.0
68.90	5272.0
70.00	480.0
71.90	289.0
72.90	2681.0
74.00	9534.0
75.00	27856.0
76.00	2297.0
76.90	394.0
77.80	388.0
78.80	2028.0
79.80	771.0
80.80	2214.0
81.70	558.0
86.90	2245.0
87.90	1785.0
90.80	222.0
91.90	1640.0
93.00	2594.0
93.90	6929.0
95.00	51408.0
96.00	3500.0
96.90	157.0
103.80	285.0
105.90	347.0
115.80	228.0
116.80	456.0
117.80	270.0
118.80	385.0
127.90	214.0
128.90	134.0
129.70	262.0
130.70	110.0
136.70	119.0
140.80	662.0
142.80	729.0
144.90	120.0
147.80	162.0
154.70	145.0
160.90	153.0
170.70	104.0
171.80	480.0
173.00	659.0
173.90	43024.0
174.90	3318.0
175.90	40408.0
176.90	2890.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
35.90	468.0
36.90	2407.0
38.00	2211.0
38.90	1124.0
39.90	316.0
43.90	603.0
44.90	518.0
46.80	508.0
47.90	396.0
48.90	2501.0
49.90	10368.0
50.90	3527.0
51.90	136.0
54.90	239.0
55.90	931.0
56.90	1594.0
59.90	549.0
60.90	2916.0
61.90	3134.0
62.90	2103.0
63.80	287.0
64.90	515.0
66.90	166.0
67.90	5573.0
68.90	5406.0
70.00	483.0
71.90	356.0
72.90	2693.0
74.00	9451.0
75.00	28128.0
76.00	2471.0
76.90	376.0
77.80	401.0
78.80	2100.0
79.80	770.0
80.80	2283.0
81.80	560.0
86.90	2165.0
87.90	1835.0
90.80	194.0
91.90	1662.0
92.90	2664.0
93.90	6977.0
95.00	52776.0
95.90	3308.0
96.80	172.0
103.80	299.0
105.90	348.0
115.80	231.0
116.90	464.0
117.80	281.0
118.80	470.0
127.80	232.0
128.90	165.0
129.80	248.0
130.70	146.0
134.90	145.0
136.80	119.0
140.80	615.0
141.80	101.0
142.80	792.0
144.90	137.0
147.80	166.0
160.90	145.0
171.80	458.0
172.90	661.0
173.90	44728.0
174.90	3457.0
175.90	42728.0
176.90	2956.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
35.90	412.0
36.90	2250.0
38.00	2152.0
38.90	1037.0
39.90	268.0
43.90	533.0
44.90	442.0
46.80	467.0
47.90	364.0
48.90	2123.0
49.90	9412.0
51.00	3228.0
54.90	165.0
55.90	869.0
56.90	1445.0
59.90	508.0
60.90	2689.0
61.90	2889.0
62.90	1839.0
63.90	254.0
64.90	515.0
66.90	160.0
67.90	5241.0
68.90	5244.0
69.90	432.0
71.90	326.0
72.90	2429.0
74.00	8546.0
75.00	25640.0
75.90	2369.0
76.80	326.0
77.80	258.0
78.80	1931.0
79.80	683.0
80.80	2163.0
81.90	548.0
86.90	1899.0
87.90	1666.0
90.90	178.0
92.00	1524.0
92.90	2413.0
93.90	6112.0
94.90	49224.0
95.90	2927.0
96.90	172.0
103.80	276.0
105.90	283.0
115.80	205.0
116.90	432.0
117.80	235.0
118.80	444.0
127.80	257.0
128.90	138.0
129.80	217.0
130.70	137.0
134.90	149.0
140.80	512.0
142.80	744.0
144.80	154.0
147.80	124.0
171.80	403.0
172.80	624.0
173.90	41672.0
174.90	3186.0
175.90	40848.0
176.90	2640.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271