




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030262.D
 Acq On : 20 Mar 2023 17:07
 Operator : SY/MD
 Sample : 01947-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB937

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:57:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

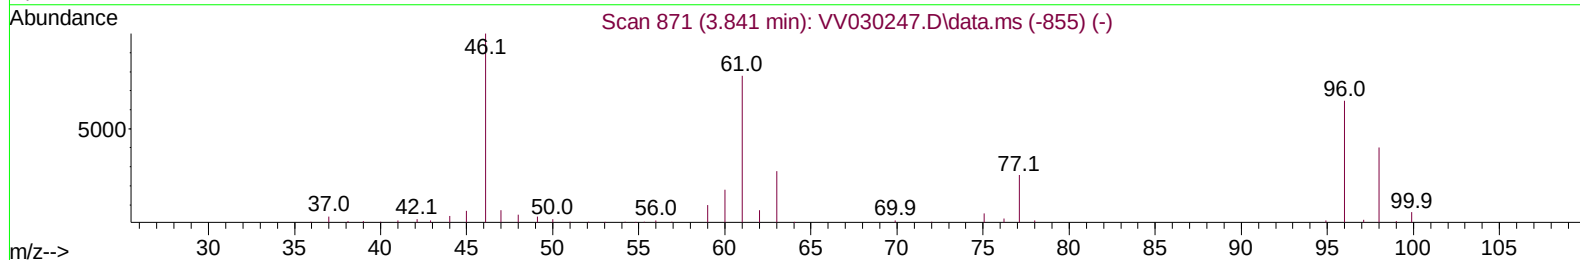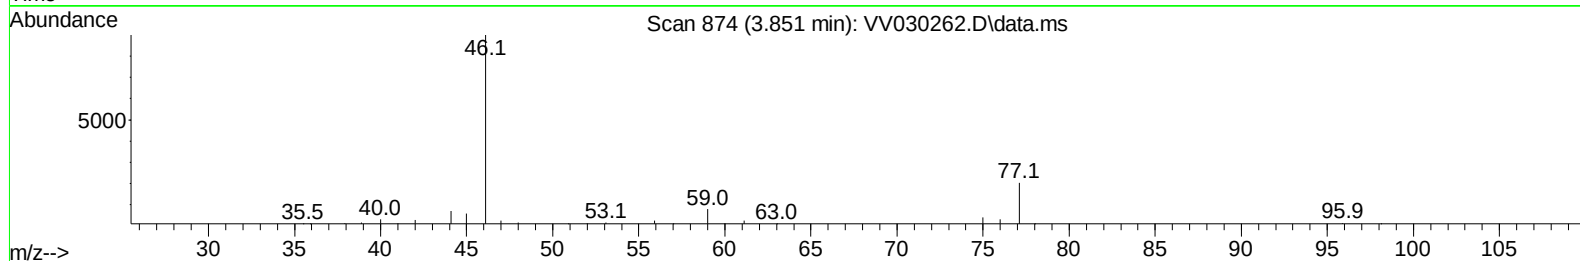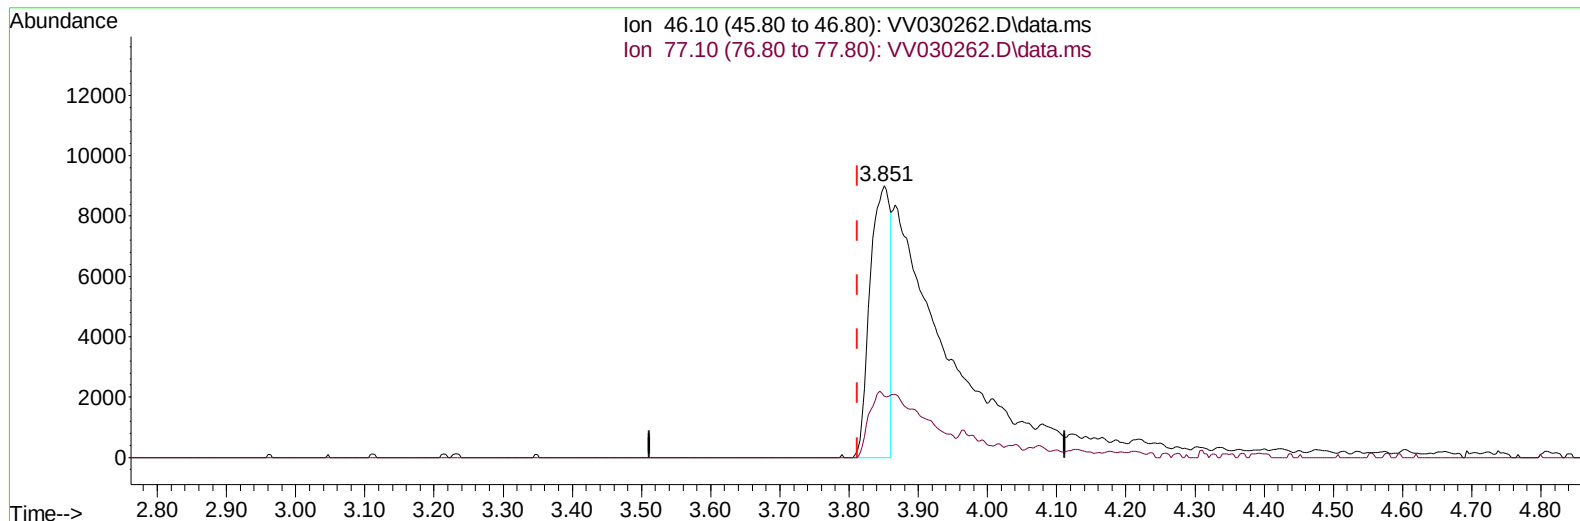

TIC: VV030262.D\data.ms

(20) 2-Butanone-d5 (S)

3.851min (+ 0.039) 13.40 ug/L

response 18199

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	20.47#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030262.D
 Acq On : 20 Mar 2023 17:07
 Operator : SY/MD
 Sample : 01947-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB937

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:57:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

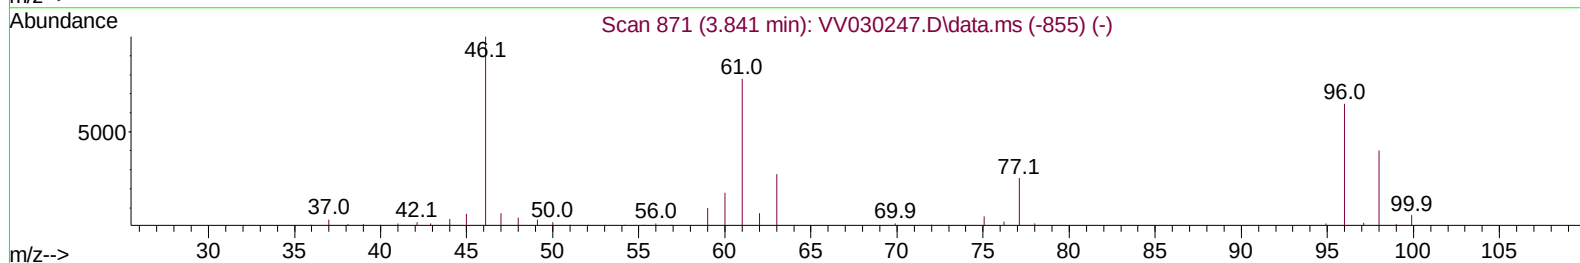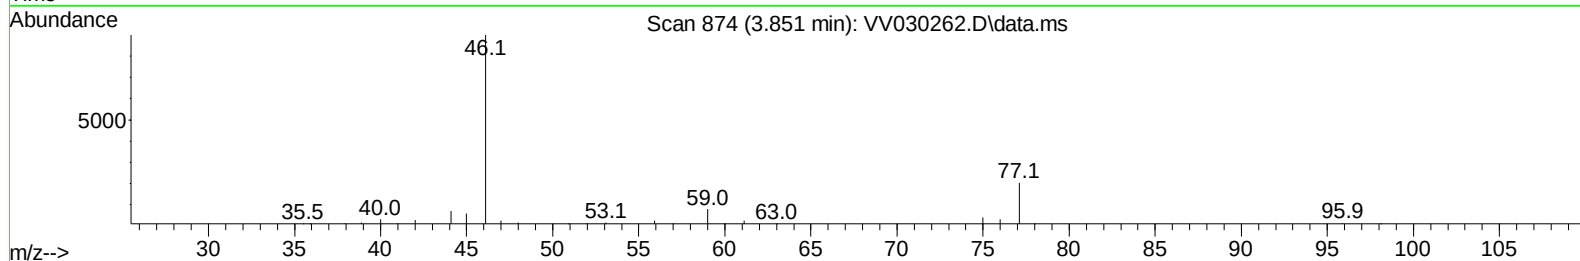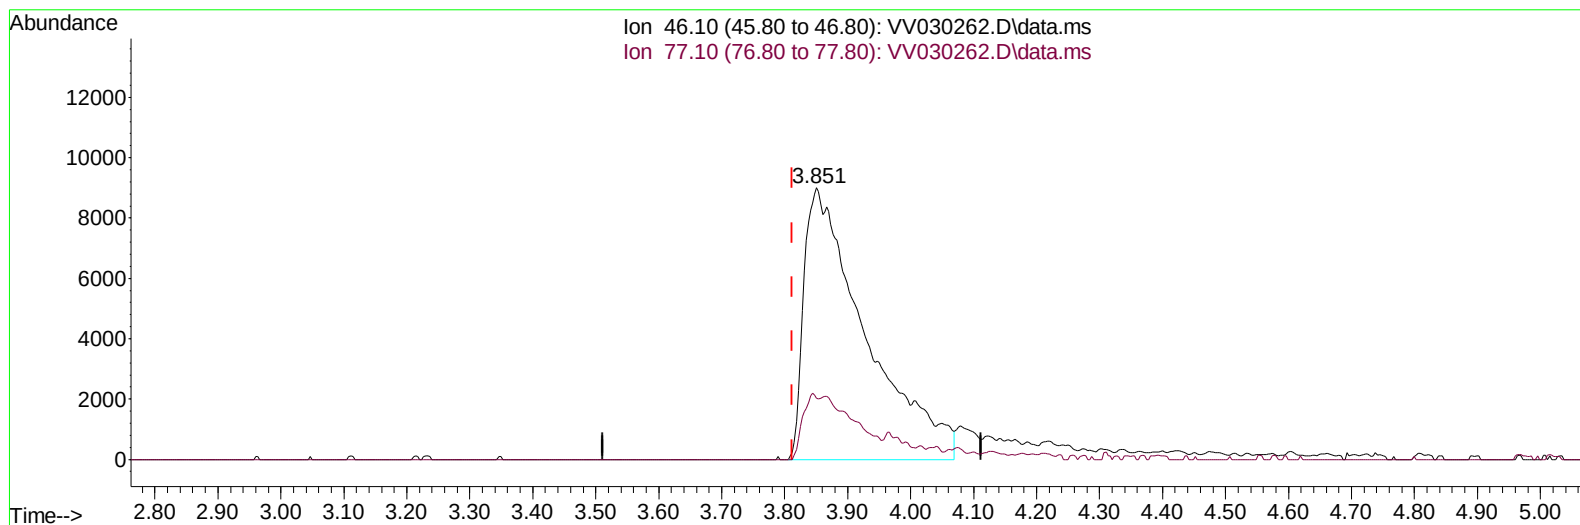

TIC: VV030262.D\data.ms

(20) 2-Butanone-d5 (S)

3.851min (+ 0.039) 44.82 ug/L m

response 60870

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	6.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030262.D
 Acq On : 20 Mar 2023 17:07
 Operator : SY/MD
 Sample : 01947-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB937

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:57:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	113841	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	111311	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	55765	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	27314	3.708	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	74.200%		
7) Chloroethane-d5	1.536	69	26306	3.804	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	76.000%		
11) 1,1-Dichloroethene-d2	2.063	63	46565	3.075	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	61.400%		
20) 2-Butanone-d5	3.851	46	60870m	44.820	ug/L	0.04
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.640%		
24) Chloroform-d	4.259	84	63483	4.219	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.400%		
26) 1,2-Dichloroethane-d4	4.957	65	32752	5.332	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	106.600%		
32) Benzene-d6	4.970	84	108711	3.630	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	72.600%		
36) 1,2-Dichloropropane-d6	5.998	67	33821	3.753	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	75.000%		
41) Toluene-d8	7.252	98	99246	3.496	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	70.000%		
43) trans-1,3-Dichloroprop...	7.564	79	13433	4.357	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	87.200%		
46) 2-Hexanone-d5	8.037	63	53895	42.258	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	84.520%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	26470	4.129	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	82.600%		
66) 1,2-Dichlorobenzene-d4	11.571	152	43467	4.607	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	92.200%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030262.D
Acq On : 20 Mar 2023 17:07
Operator : SY/MD
Sample : 01947-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB937

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:57:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023

