

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030255.D
 Acq On : 20 Mar 2023 13:53
 Operator : SY/MD
 Sample : 02005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA5

Quant Time: Mar 20 14:17:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	125265	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	123950	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	60493	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	28634	3.533	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.600%	
7) Chloroethane-d5	1.536	69	28321	3.722	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	74.400%	
11) 1,1-Dichloroethene-d2	2.066	63	48277	2.897	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.000%#	
20) 2-Butanone-d5	3.815	46	75602	50.591	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	101.180%	
24) Chloroform-d	4.262	84	67279	4.063	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.200%	
26) 1,2-Dichloroethane-d4	4.953	65	35708	5.283	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.600%	
32) Benzene-d6	4.970	84	118449	3.551	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	71.000%	
36) 1,2-Dichloropropane-d6	5.998	67	35761	3.564	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	71.200%	
41) Toluene-d8	7.252	98	104336	3.300	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	66.000%#	
43) trans-1,3-Dichloroprop...	7.561	79	13848	4.034	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.600%	
46) 2-Hexanone-d5	8.034	63	58699	41.331	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.660%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	28163	3.945	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	79.000%	
66) 1,2-Dichlorobenzene-d4	11.571	152	43593	4.259	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	85.200%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.220	50	2697	0.168	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030255.D
Acq On : 20 Mar 2023 13:53
Operator : SY/MD
Sample : 02005-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMA5

Quant Time: Mar 20 14:17:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

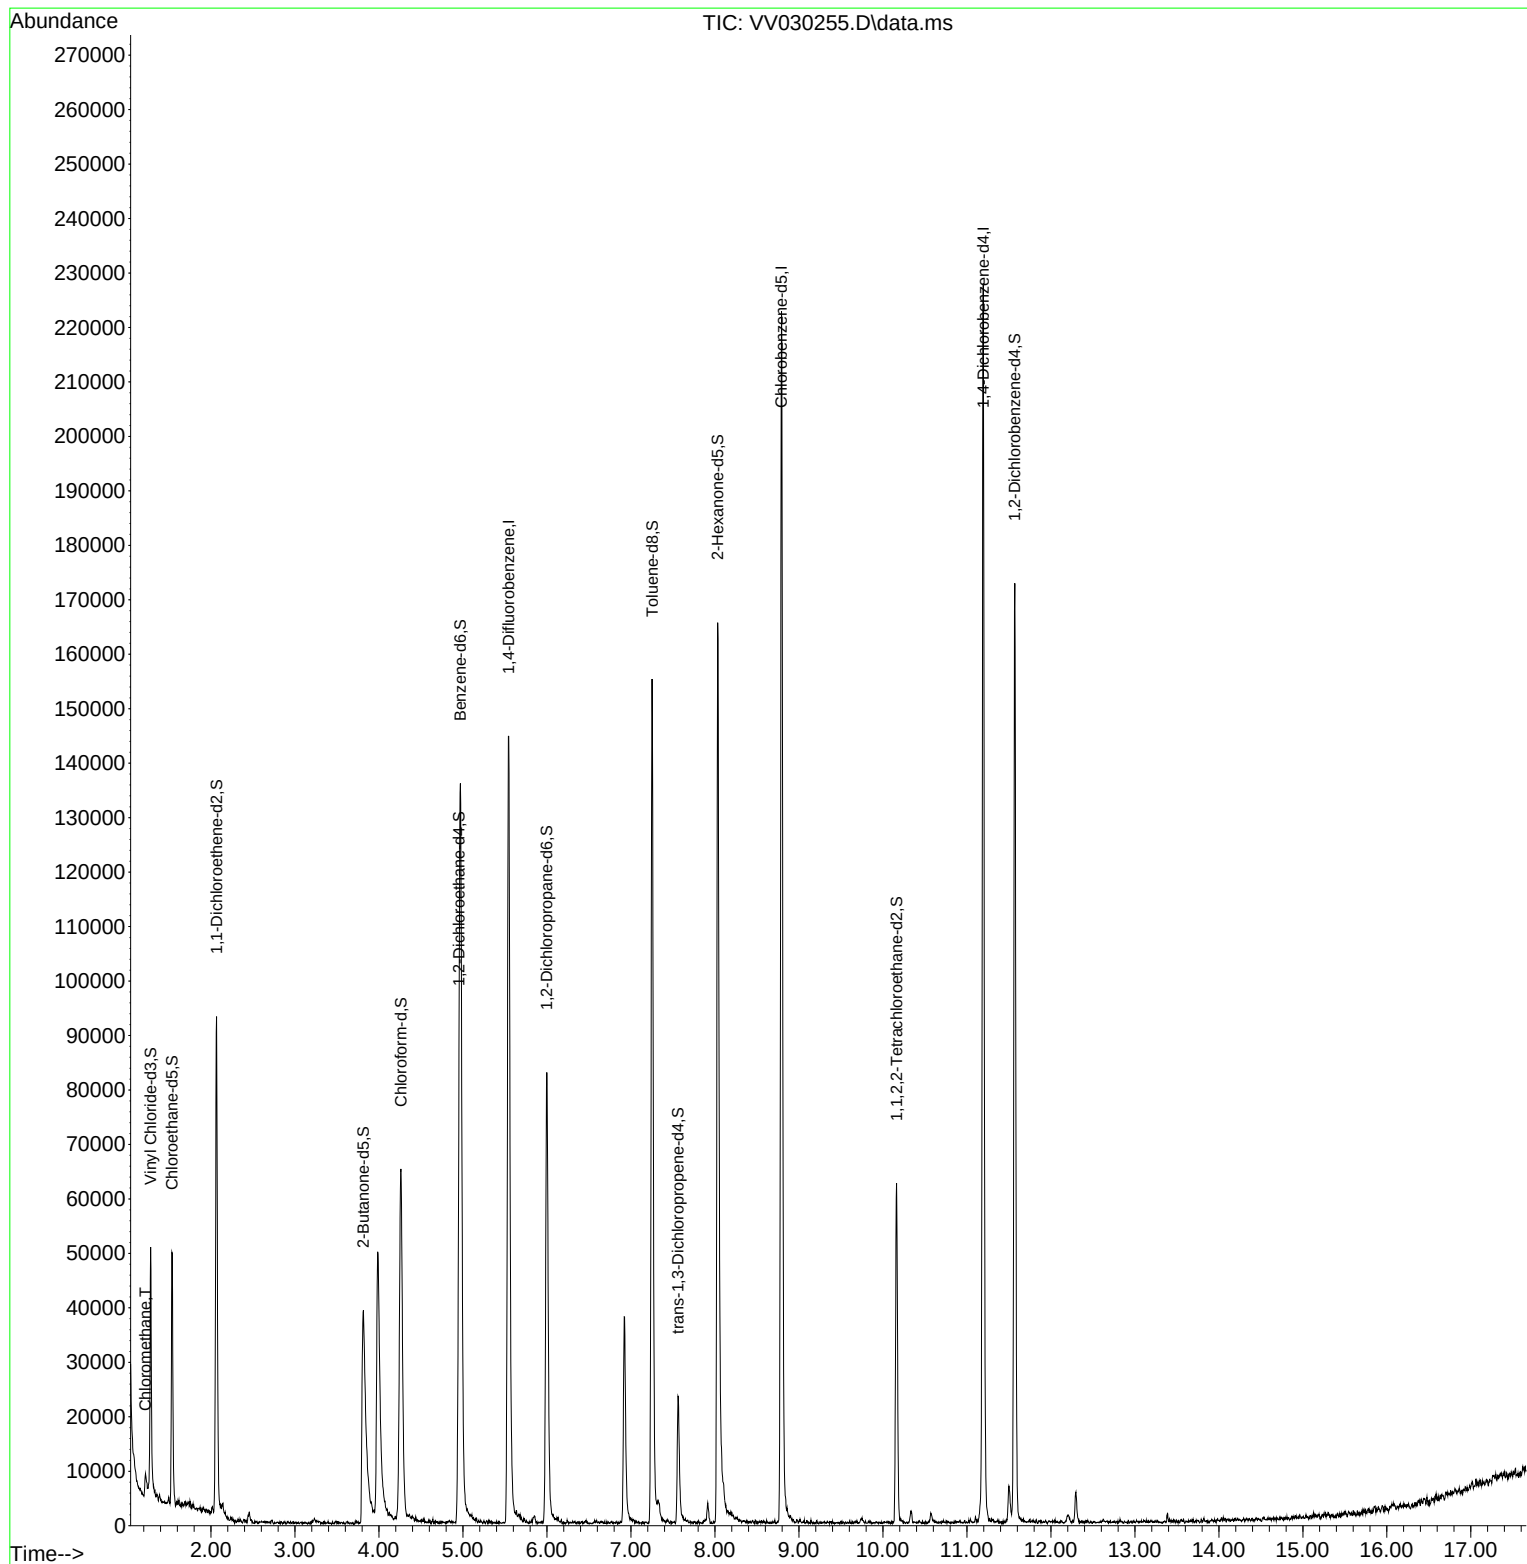

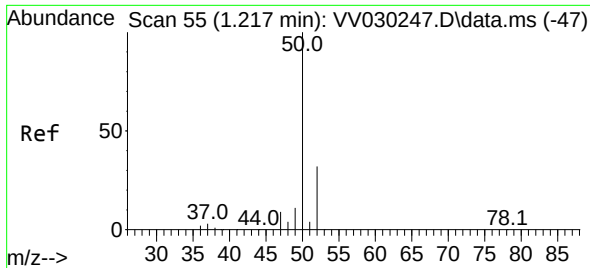

#3
 Chloromethane
 Concen: 0.168 ug/L
 RT: 1.220 min Scan# 50
 Delta R.T. 0.003 min
 Lab File: VV030255.D
 Acq: 20 Mar 2023 13:53

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA5

Tgt Ion: 50 Resp: 2697
 Ion Ratio Lower Upper
 50 100
 52 33.6 23.6 43.8

