

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030263.D
 Acq On : 20 Mar 2023 17:32
 Operator : SY/MD
 Sample : 01947-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB942

Quant Time: Mar 21 02:57:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	120177	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	114852	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	58190	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	26117	3.359	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.539	69	27164	3.721	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	74.400%	
11) 1,1-Dichloroethene-d2	2.066	63	46098	2.884	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	57.600%#	
20) 2-Butanone-d5	3.818	46	74159	51.727	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.460%	
24) Chloroform-d	4.262	84	66417	4.181	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.600%	
26) 1,2-Dichloroethane-d4	4.953	65	33262	5.129	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
32) Benzene-d6	4.969	84	115645	3.742	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	74.800%	
36) 1,2-Dichloropropane-d6	5.998	67	35048	3.770	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	75.400%	
41) Toluene-d8	7.252	98	102786	3.509	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.200%	
43) trans-1,3-Dichloroprop...	7.564	79	12891	4.053	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.037	63	58043	44.107	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.220%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	27410	4.144	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	82.800%	
66) 1,2-Dichlorobenzene-d4	11.570	152	41648	4.230	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	84.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.146	43	5119	4.831	ug/L #	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030263.D
Acq On : 20 Mar 2023 17:32
Operator : SY/MD
Sample : 01947-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB942

Quant Time: Mar 21 02:57:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

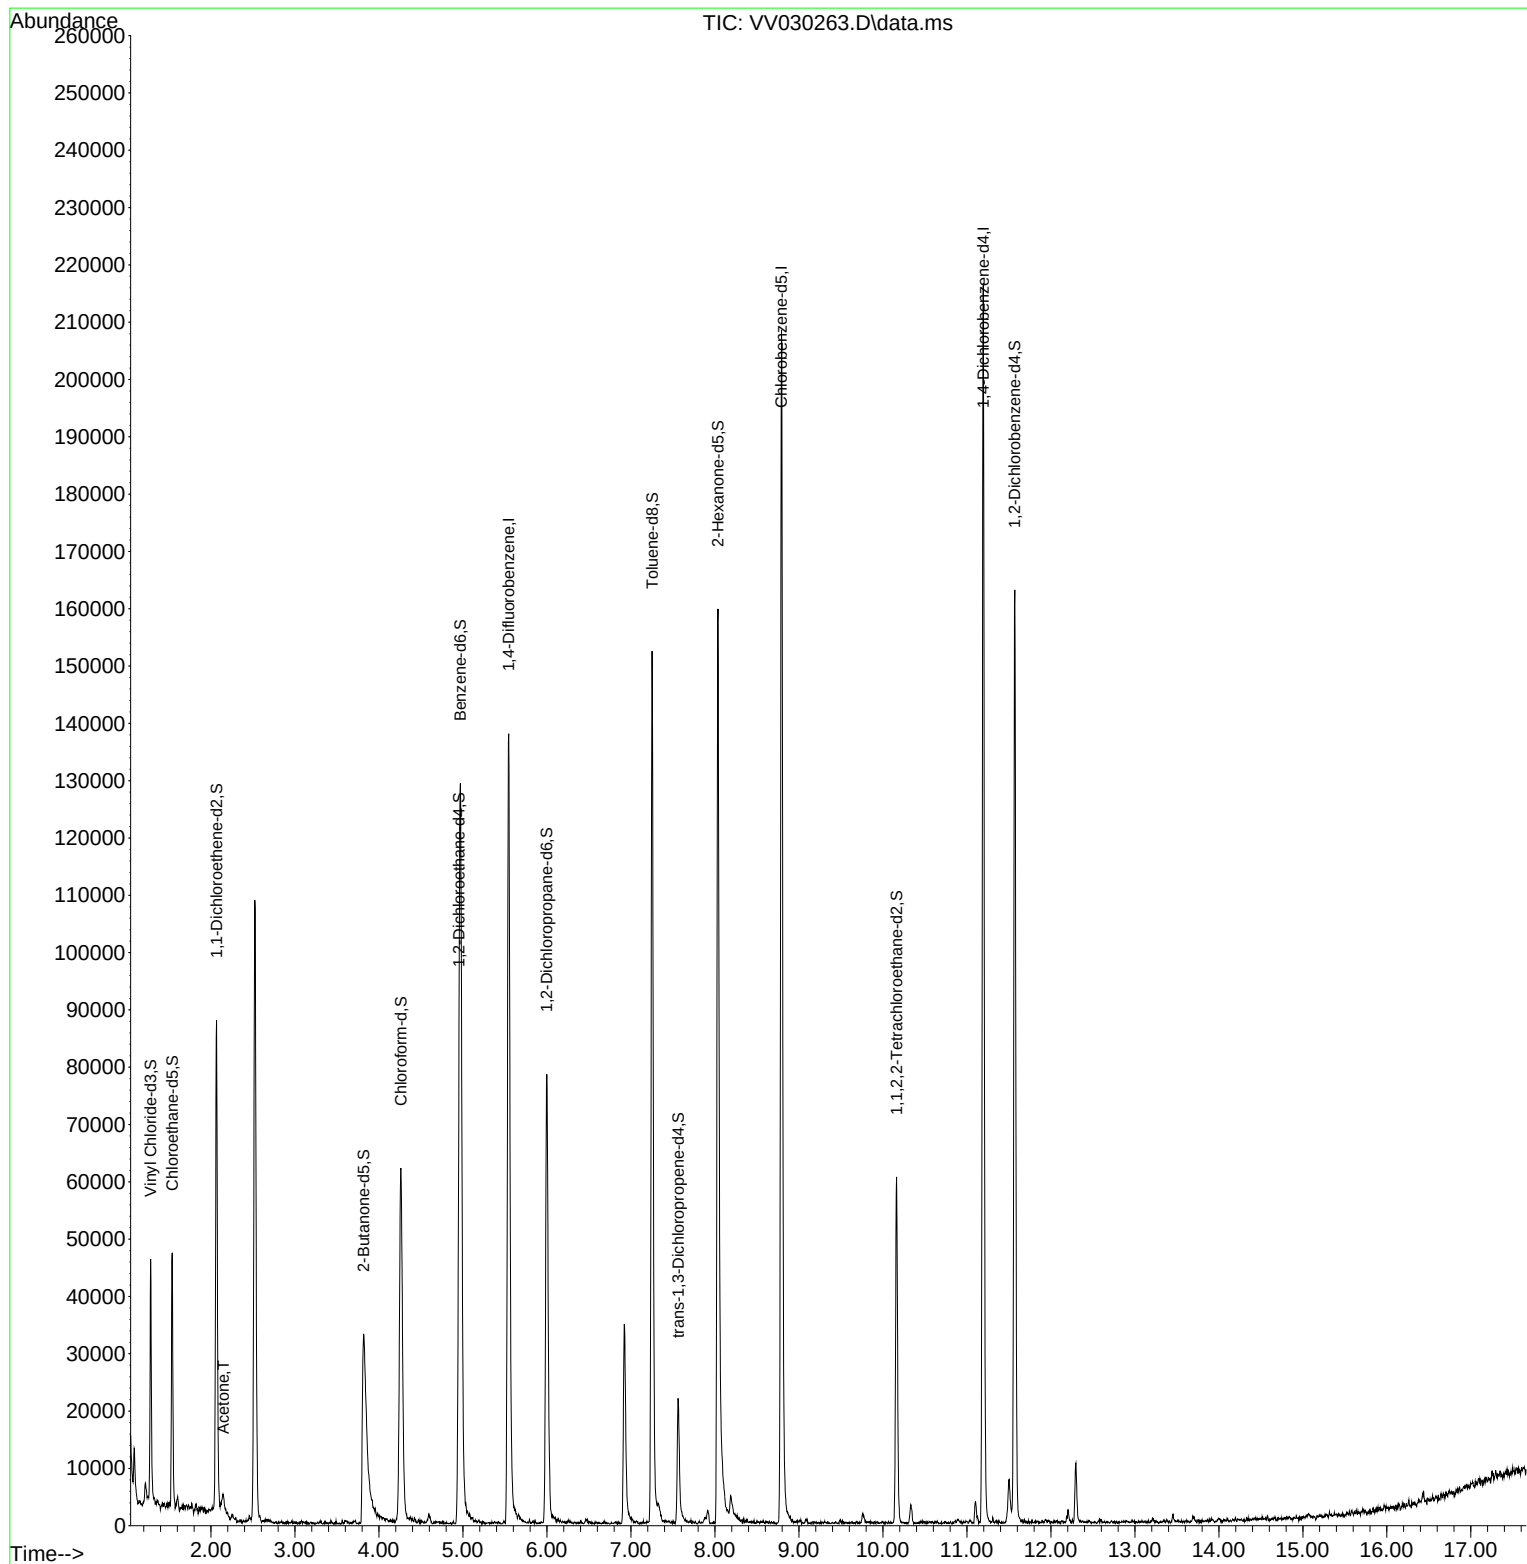

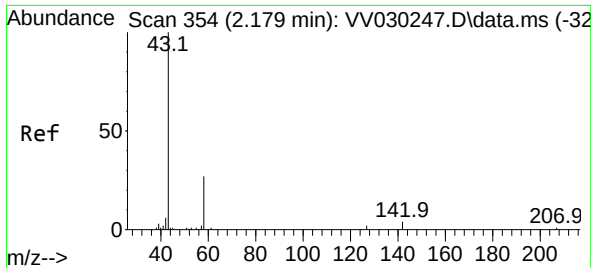

#13

Acetone

Concen: 4.831 ug/L

RT: 2.146 min Scan# 34

Delta R.T. 0.003 min

Lab File: VV030263.D


Acq: 20 Mar 2023 17:32

Instrument :

MSVOA_V

ClientSampleId :

CB942

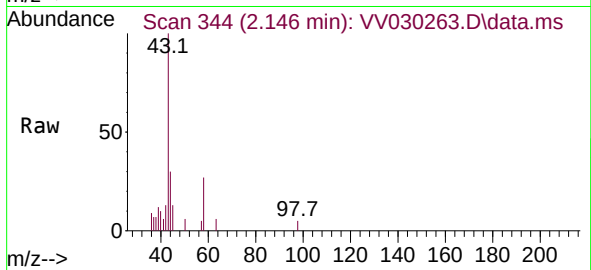

Tgt Ion: 43 Resp: 5119

Ion Ratio Lower Upper

43 100

58 37.6 0.0 29.4#

