

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030248.D
 Acq On : 20 Mar 2023 11:05
 Operator : SY/MD
 Sample : VV0320WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	62	rBV2	4666	5766	1.61%	0.183%
2	1.278	68	74	92	rVB	50389	59733	16.68%	1.896%
3	1.536	146	154	168	rVB	51097	60621	16.93%	1.924%
4	2.063	309	318	331	rVB	102252	144753	40.42%	4.595%
5	2.455	430	440	453	rVB2	10720	18259	5.10%	0.580%
6	2.973	593	601	612	rVB8	2589	5367	1.50%	0.170%
7	3.851	856	874	895	rBV2	18095	86635	24.19%	2.750%
8	4.259	983	1001	1024	rBV	66034	173643	48.48%	5.512%
9	4.966	1203	1221	1245	rBV2	137263	358159	100.00%	11.370%
10	5.542	1386	1400	1422	rBV	140611	296907	82.90%	9.425%
11	5.995	1528	1541	1560	rBV3	82679	179794	50.20%	5.708%
12	6.921	1819	1829	1842	rBV2	39611	72712	20.30%	2.308%
13	7.249	1919	1931	1959	rBV	160159	293466	81.94%	9.316%
14	7.561	2019	2028	2045	rBV3	22979	44861	12.53%	1.424%
15	7.915	2130	2138	2148	rBV6	3794	5773	1.61%	0.183%
16	8.037	2166	2176	2209	rBV	140083	314224	87.73%	9.975%
17	8.793	2398	2411	2431	rBV	205162	347306	96.97%	11.025%
18	10.162	2825	2837	2854	rBV2	61027	99104	27.67%	3.146%
19	11.194	3147	3158	3181	rBV	205114	325233	90.81%	10.325%
20	11.567	3261	3274	3291	rBV	157092	257740	71.96%	8.182%




Sum of corrected areas: 3150056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030248.D
Acq On : 20 Mar 2023 11:05
Operator : SY/MD
Sample : VV0320WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

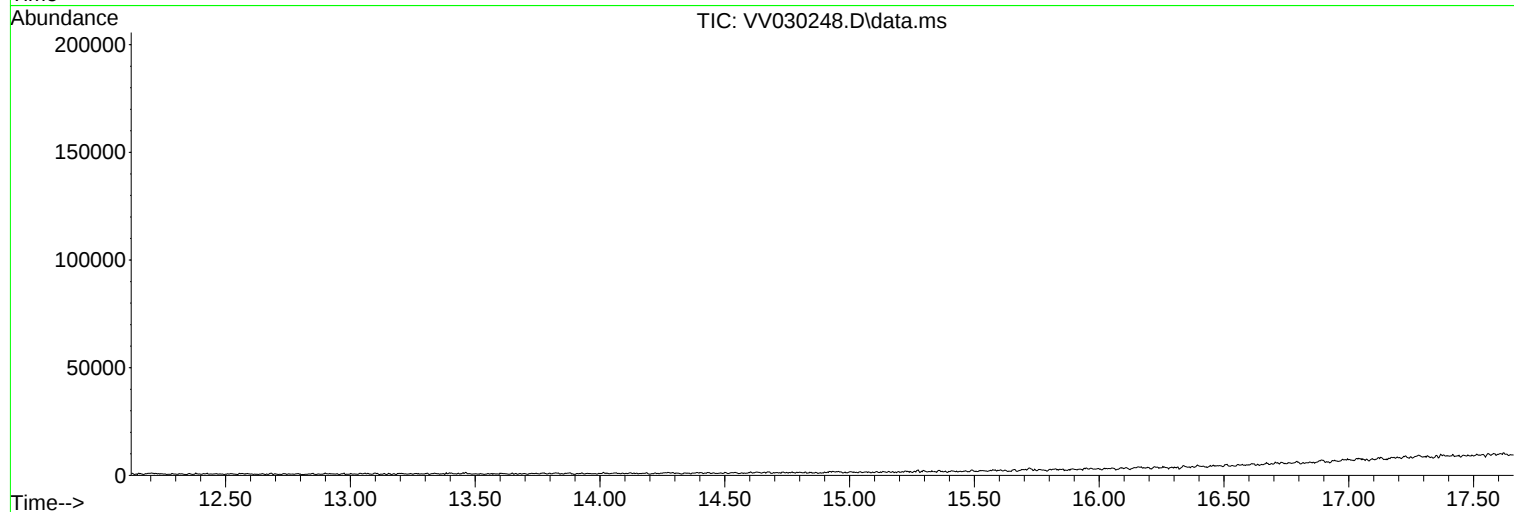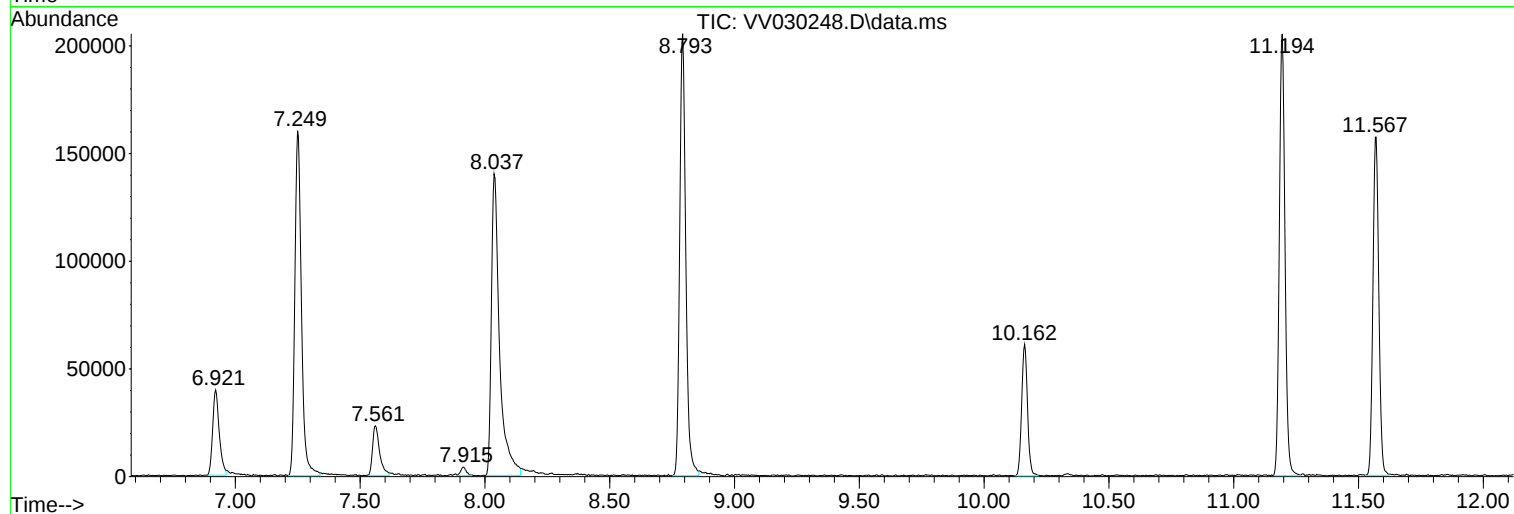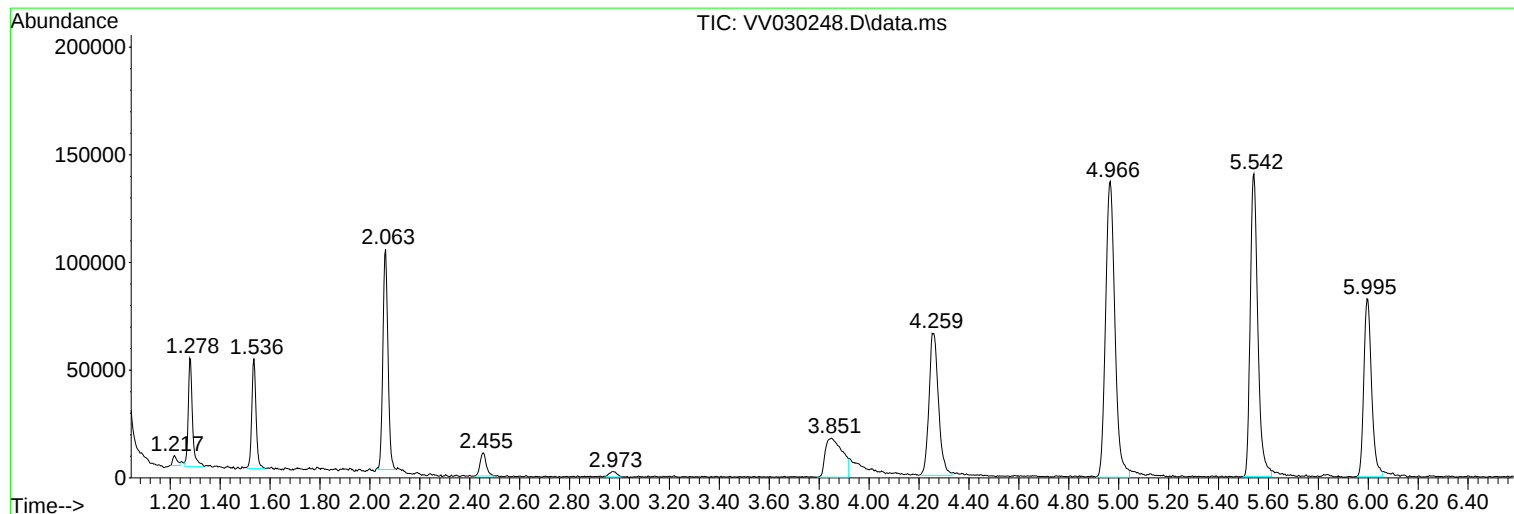

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030248.D
Acq On : 20 Mar 2023 11:05
Operator : SY/MD
Sample : VV0320WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030248.D
Acq On : 20 Mar 2023 11:05
Operator : SY/MD
Sample : VV0320WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------