

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030249.D
 Acq On : 20 Mar 2023 11:29
 Operator : SY/MD
 Sample : 02005-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM99

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	50	56	63	rBV2	4918	7547	2.04%	0.230%
2	1.282	69	75	90	rVB	47951	53620	14.46%	1.637%
3	1.536	147	154	165	rVB	48202	55356	14.93%	1.690%
4	2.063	305	318	338	rBV	97529	147399	39.75%	4.499%
5	2.455	430	440	452	rVB4	6430	11977	3.23%	0.366%
6	3.835	856	869	907	rBV	24350	119444	32.21%	3.646%
7	4.262	985	1002	1027	rBV	67817	175772	47.40%	5.365%
8	4.970	1205	1222	1248	rBV2	140770	368636	99.42%	11.252%
9	5.542	1388	1400	1421	rBV	139654	294558	79.44%	8.991%
10	5.998	1528	1542	1561	rBV2	85482	183052	49.37%	5.587%
11	6.921	1816	1829	1846	rBV	39423	75368	20.33%	2.300%
12	7.252	1918	1932	1956	rBV	163231	297084	80.12%	9.068%
13	7.561	2016	2028	2050	rBV3	24609	49362	13.31%	1.507%
14	8.037	2166	2176	2206	rBV	156655	332178	89.59%	10.139%
15	8.793	2400	2411	2433	rBV	219077	370793	100.00%	11.318%
16	10.162	2826	2837	2850	rBV	63018	104077	28.07%	3.177%
17	10.336	2883	2891	2900	rVB3	3896	5698	1.54%	0.174%
18	11.194	3147	3158	3177	rBV	218183	344376	92.88%	10.511%
19	11.506	3247	3255	3263	rBV7	3112	5178	1.40%	0.158%
20	11.571	3263	3275	3293	rVB	169873	274752	74.10%	8.386%




Sum of corrected areas: 3276227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030249.D
Acq On : 20 Mar 2023 11:29
Operator : SY/MD
Sample : 02005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

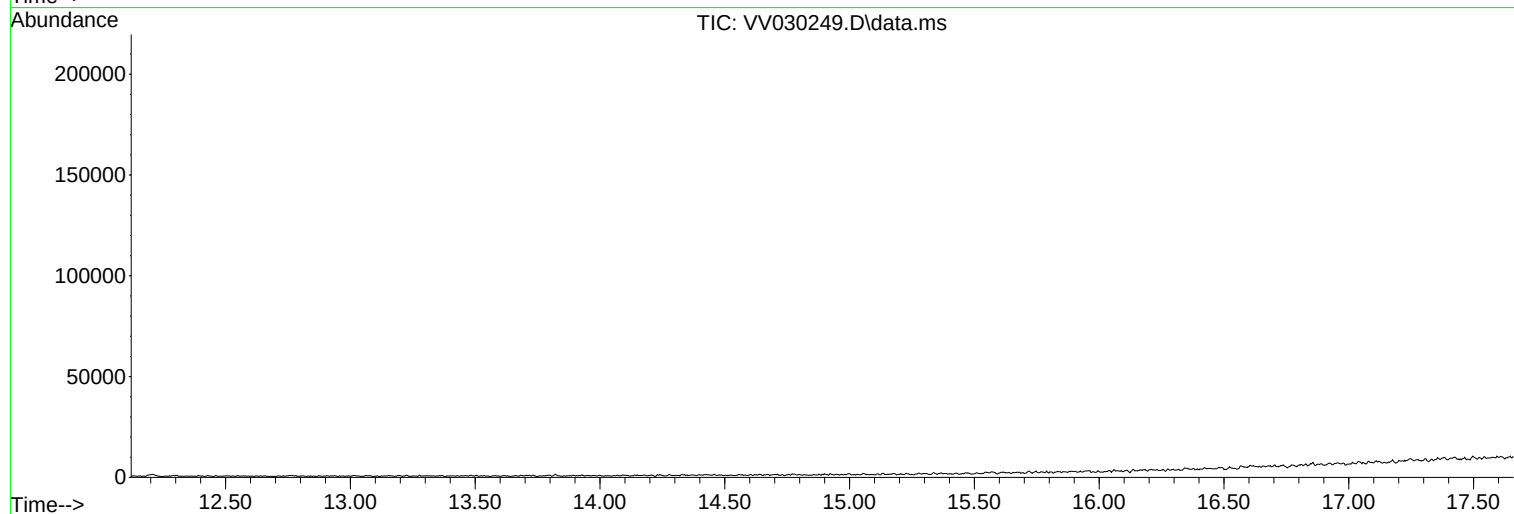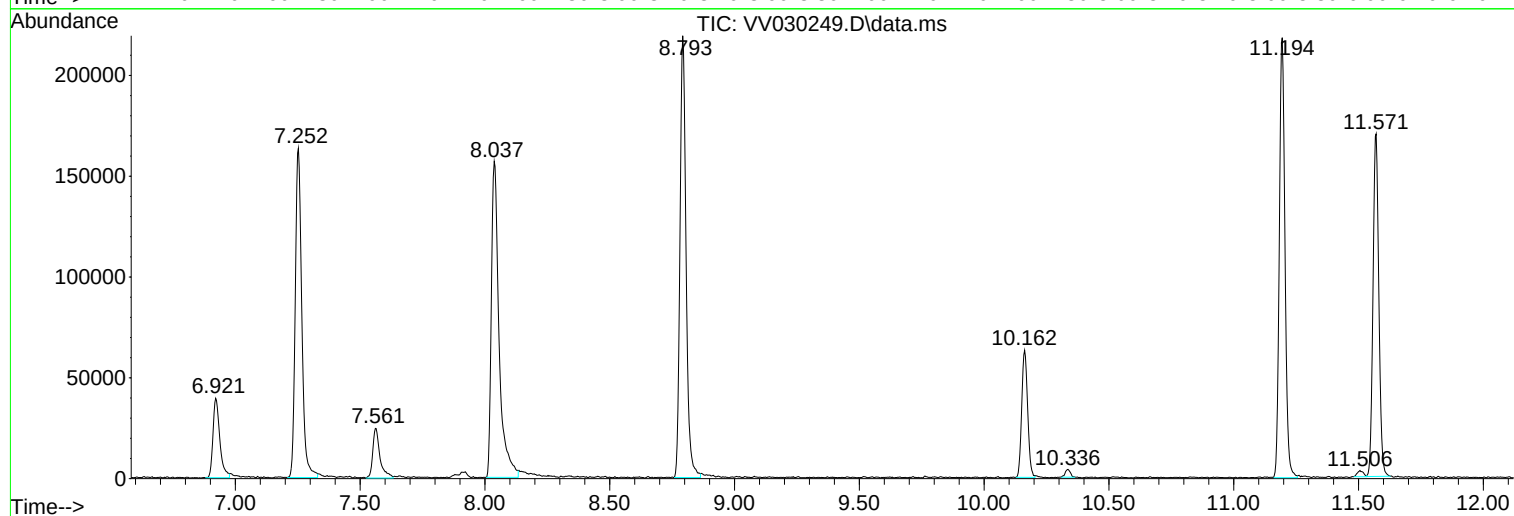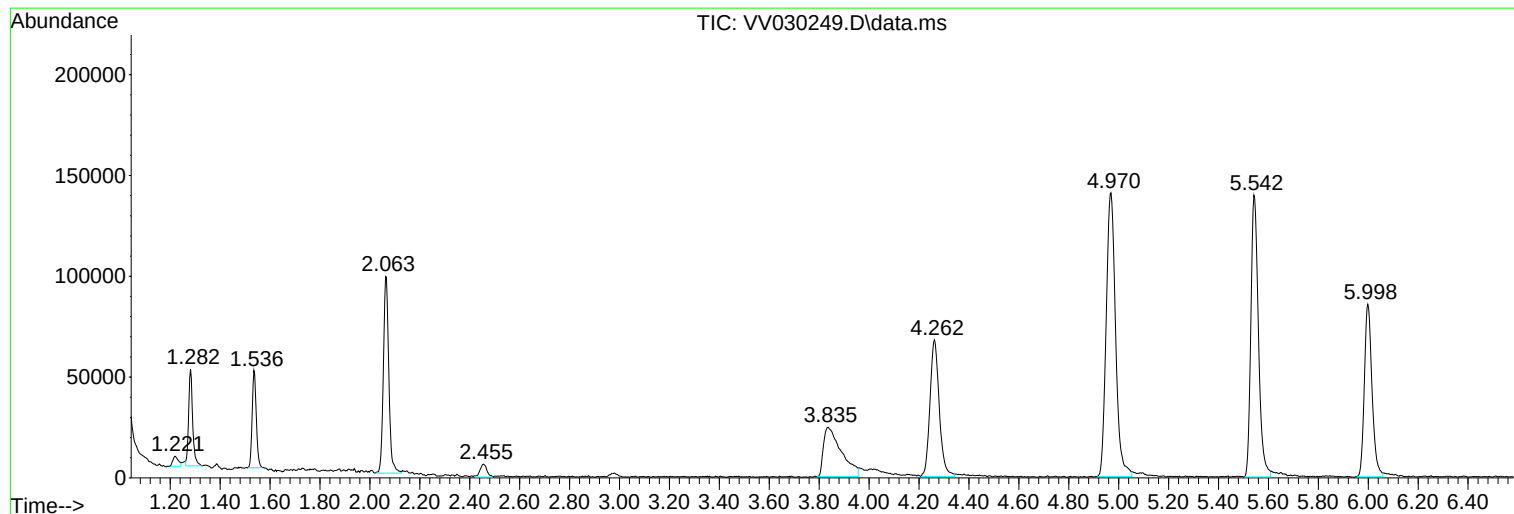

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030249.D
Acq On : 20 Mar 2023 11:29
Operator : SY/MD
Sample : 02005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030249.D
Acq On : 20 Mar 2023 11:29
Operator : SY/MD
Sample : 02005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc