

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030250.D
 Acq On : 20 Mar 2023 11:53
 Operator : SY/MD
 Sample : 02005-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	50	56	66	rBV2	4632	6744	1.89%	0.201%
2	1.282	69	75	86	rVB	48220	53895	15.08%	1.605%
3	1.539	147	155	166	rVB	47863	56333	15.76%	1.677%
4	2.063	308	318	336	rBV	98260	144524	40.43%	4.303%
5	3.825	852	866	888	rBV3	43436	144622	40.46%	4.306%
6	4.262	984	1002	1027	rBV2	64368	166686	46.63%	4.963%
7	4.966	1203	1221	1242	rBV2	135992	350801	98.13%	10.445%
8	5.542	1386	1400	1427	rBV	135887	290283	81.20%	8.643%
9	5.844	1482	1494	1515	rBV3	61870	129983	36.36%	3.870%
10	5.998	1526	1542	1564	rBV	85583	175380	49.06%	5.222%
11	6.921	1815	1829	1854	rBV2	37950	74388	20.81%	2.215%
12	7.252	1918	1932	1948	rBV	155099	282319	78.97%	8.406%
13	7.326	1951	1955	1966	rVB	6958	11354	3.18%	0.338%
14	7.561	2019	2028	2042	rBV2	24444	43713	12.23%	1.302%
15	7.886	2118	2129	2131	rBV3	2614	3643	1.02%	0.108%
16	7.915	2131	2138	2148	rVB6	4205	8008	2.24%	0.238%
17	8.037	2163	2176	2209	rBV	156391	321055	89.81%	9.559%
18	8.793	2400	2411	2434	rBV	209171	357483	100.00%	10.644%
19	10.162	2826	2837	2849	rBV	63821	102142	28.57%	3.041%
20	10.333	2876	2890	2902	rBV3	8208	13647	3.82%	0.406%
21	11.194	3138	3158	3179	rBV	210081	337762	94.48%	10.057%
22	11.503	3246	3254	3262	rBV6	4320	7383	2.07%	0.220%
23	11.571	3263	3275	3298	rVB	164240	267436	74.81%	7.963%
24	12.204	3463	3472	3485	rVB2	2483	4450	1.24%	0.132%
25	12.297	3491	3501	3512	rVB7	2782	4473	1.25%	0.133%




Sum of corrected areas: 3358507

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030250.D
Acq On : 20 Mar 2023 11:53
Operator : SY/MD
Sample : 02005-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

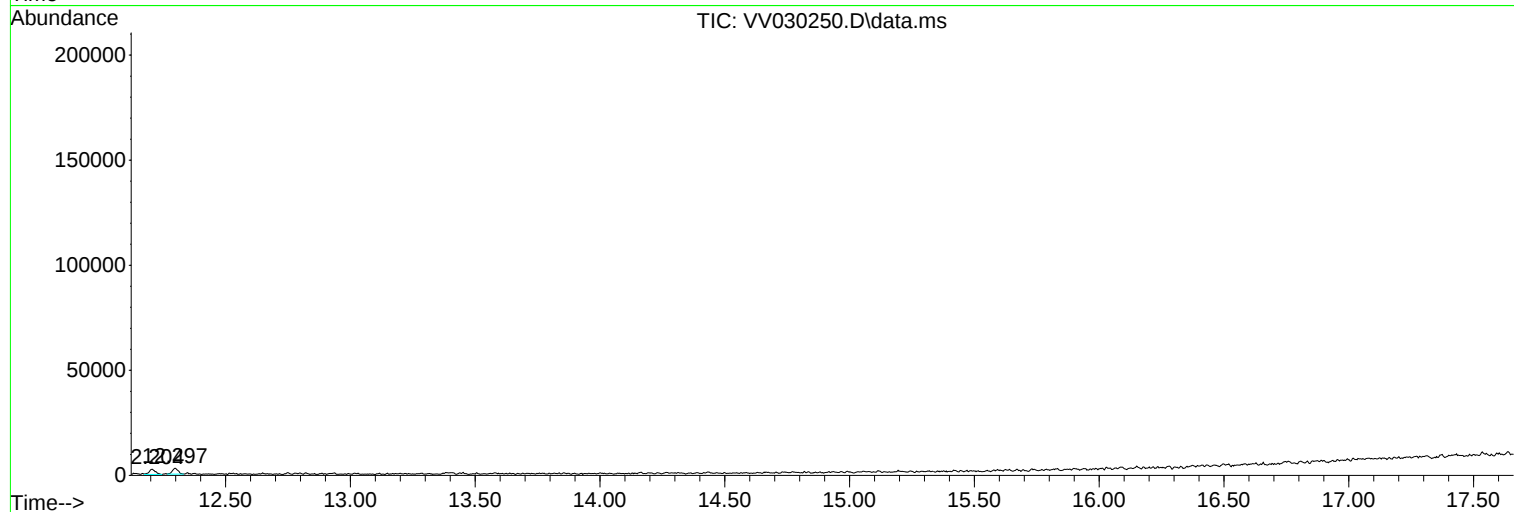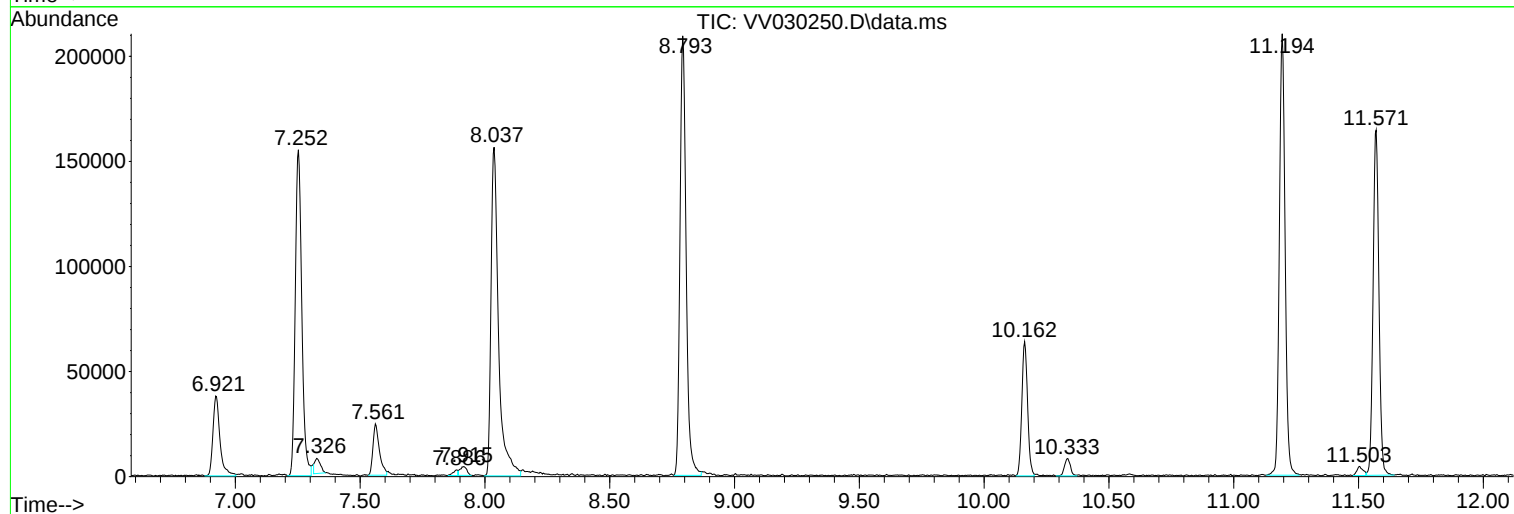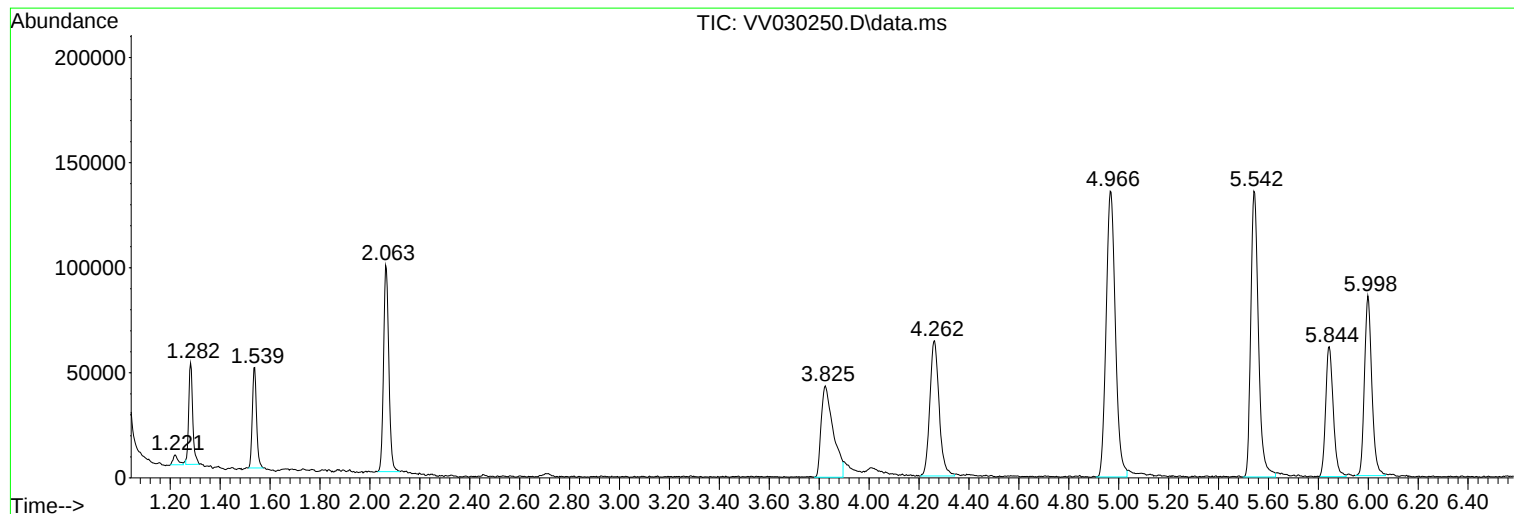

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030250.D
Acq On : 20 Mar 2023 11:53
Operator : SY/MD
Sample : 02005-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030250.D
Acq On : 20 Mar 2023 11:53
Operator : SY/MD
Sample : 02005-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
