

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV0302023\
 Data File : VV030254.D
 Acq On : 20 Mar 2023 13:29
 Operator : SY/MD
 Sample : 02005-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0MA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	64	rBV2	4681	6547	1.88%	0.210%
2	1.282	69	75	88	rVB	44386	51465	14.79%	1.649%
3	1.539	145	155	165	rVB	46220	56283	16.18%	1.803%
4	2.066	307	319	333	rBV	89867	133229	38.30%	4.269%
5	3.812	849	862	894	rBV2	38506	124718	35.85%	3.996%
6	4.262	985	1002	1023	rBV2	63884	161646	46.47%	5.180%
7	4.969	1203	1222	1245	rBV2	131204	342873	98.56%	10.987%
8	5.545	1388	1401	1423	rBV	134350	279454	80.33%	8.955%
9	5.998	1526	1542	1560	rBV	79311	170846	49.11%	5.474%
10	6.924	1818	1830	1846	rBV	36356	69854	20.08%	2.238%
11	7.252	1917	1932	1949	rBV	153904	276918	79.60%	8.873%
12	7.326	1949	1955	1965	rVB3	5224	9618	2.76%	0.308%
13	7.564	2018	2029	2042	rBV2	23529	43643	12.55%	1.398%
14	7.915	2132	2138	2148	rVB5	3405	4975	1.43%	0.159%
15	8.034	2163	2175	2203	rBV	161390	313548	90.13%	10.047%
16	8.792	2400	2411	2439	rBV	205424	347866	100.00%	11.147%
17	10.162	2822	2837	2850	rBV	63047	99899	28.72%	3.201%
18	11.194	3139	3158	3176	rBV	213776	337882	97.13%	10.827%
19	11.503	3245	3254	3264	rBV5	6111	12257	3.52%	0.393%
20	11.570	3264	3275	3290	rVB	164266	263627	75.78%	8.447%
21	12.294	3491	3500	3519	rBV6	8011	13669	3.93%	0.438%




Sum of corrected areas: 3120817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030254.D
Acq On : 20 Mar 2023 13:29
Operator : SY/MD
Sample : 02005-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

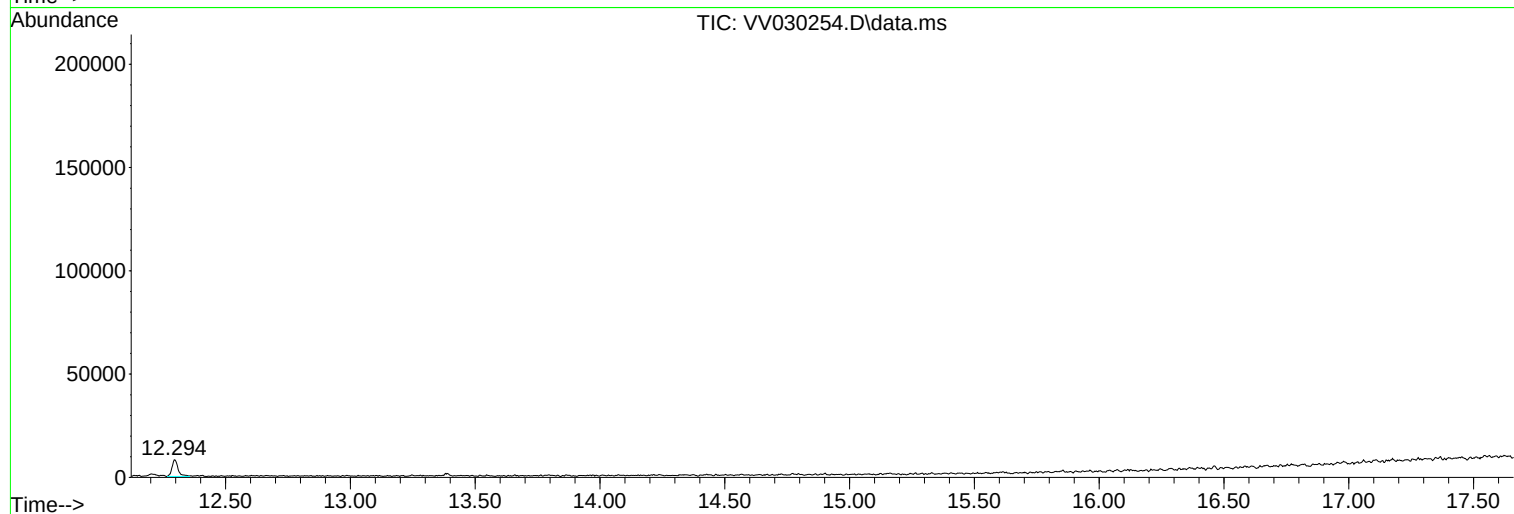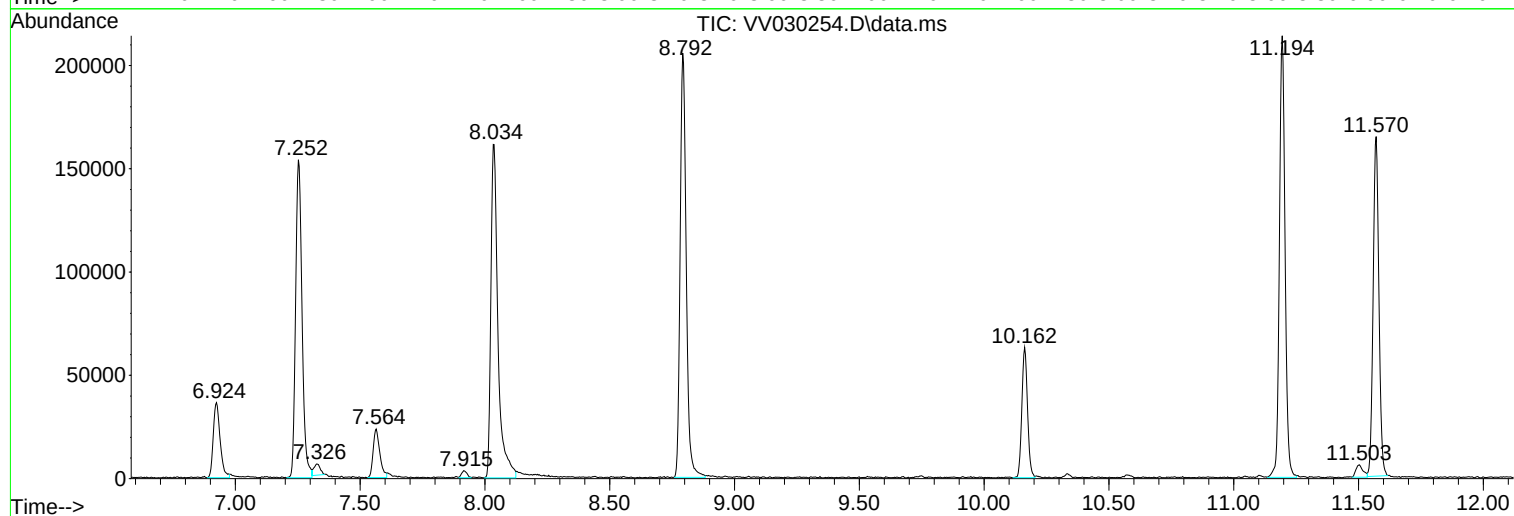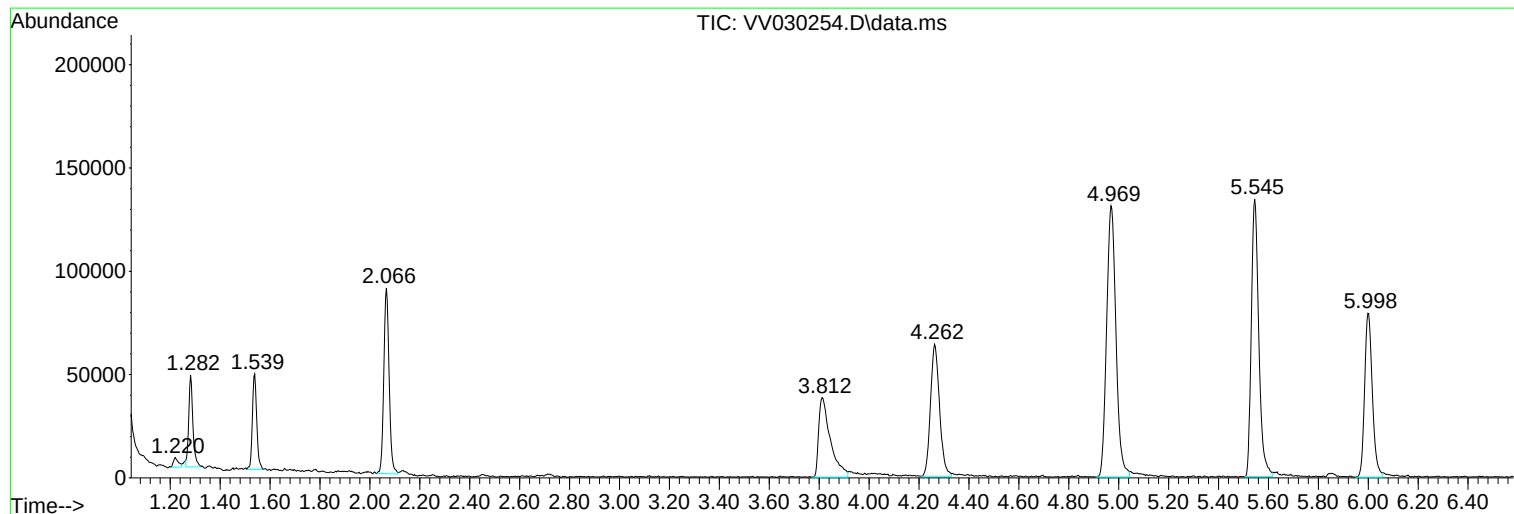

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030254.D
Acq On : 20 Mar 2023 13:29
Operator : SY/MD
Sample : 02005-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030254.D
Acq On : 20 Mar 2023 13:29
Operator : SY/MD
Sample : 02005-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc