

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030256.D
 Acq On : 20 Mar 2023 14:18
 Operator : SY/MD
 Sample : 01997-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	50	56	63	rBV3	4387	6599	1.68%	0.189%
2	1.281	69	75	92	rVB	48932	55352	14.06%	1.588%
3	1.539	145	155	169	rVB	49401	60837	15.45%	1.746%
4	2.066	308	319	332	rBV	98859	146532	37.22%	4.205%
5	2.455	432	440	452	rVB4	8208	15605	3.96%	0.448%
6	3.815	851	863	902	rBV2	40313	150278	38.17%	4.312%
7	4.262	985	1002	1029	rBV	69994	181898	46.20%	5.220%
8	4.969	1203	1222	1252	rBV3	147568	384552	97.67%	11.035%
9	5.542	1383	1400	1430	rBV	153814	320567	81.42%	9.199%
10	5.998	1528	1542	1562	rBV2	91699	193295	49.09%	5.547%
11	6.921	1819	1829	1846	rBV	40913	76130	19.34%	2.185%
12	7.252	1919	1932	1950	rBV	167015	306296	77.79%	8.789%
13	7.561	2018	2028	2046	rBV2	25364	48635	12.35%	1.396%
14	7.915	2131	2138	2146	rVB7	2633	4954	1.26%	0.142%
15	8.034	2164	2175	2207	rBV	182077	355540	90.30%	10.202%
16	8.792	2399	2411	2432	rBV	235914	393722	100.00%	11.298%
17	10.162	2824	2837	2855	rVB	68891	109847	27.90%	3.152%
18	10.336	2882	2891	2898	rVB3	3029	4349	1.10%	0.125%
19	11.194	3142	3158	3177	rBV	232664	374465	95.11%	10.745%
20	11.570	3263	3275	3292	rVB	182475	290244	73.72%	8.329%
21	12.297	3493	3501	3511	rVB5	3623	5178	1.32%	0.149%




Sum of corrected areas: 3484875

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030256.D
Acq On : 20 Mar 2023 14:18
Operator : SY/MD
Sample : 01997-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

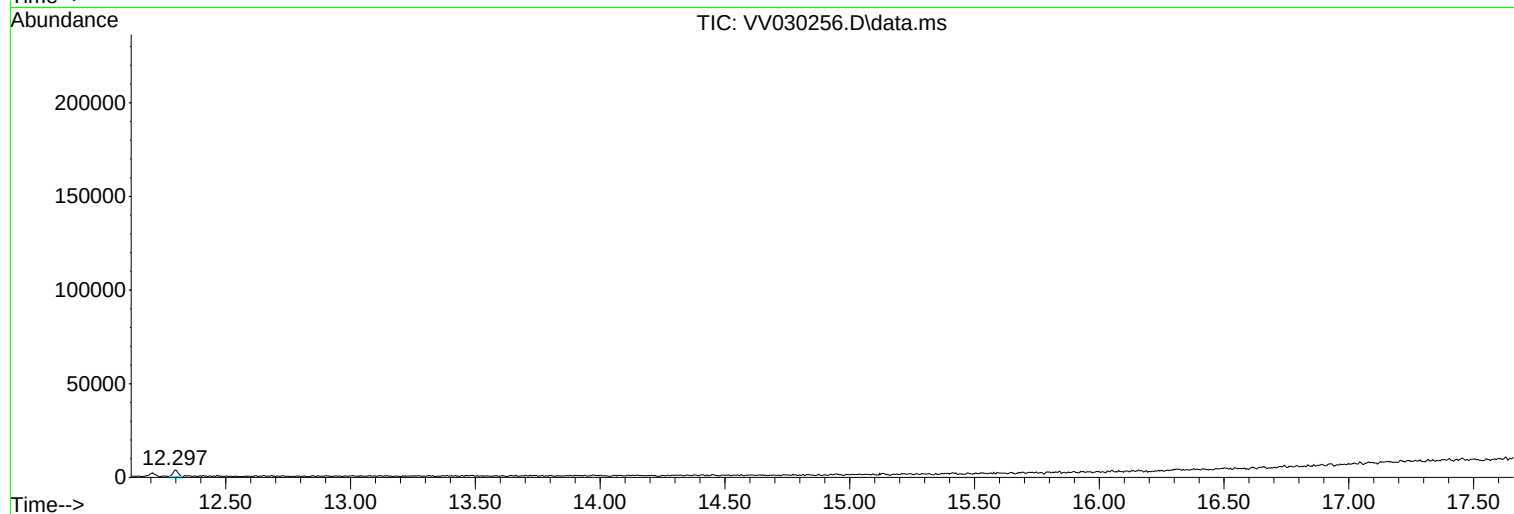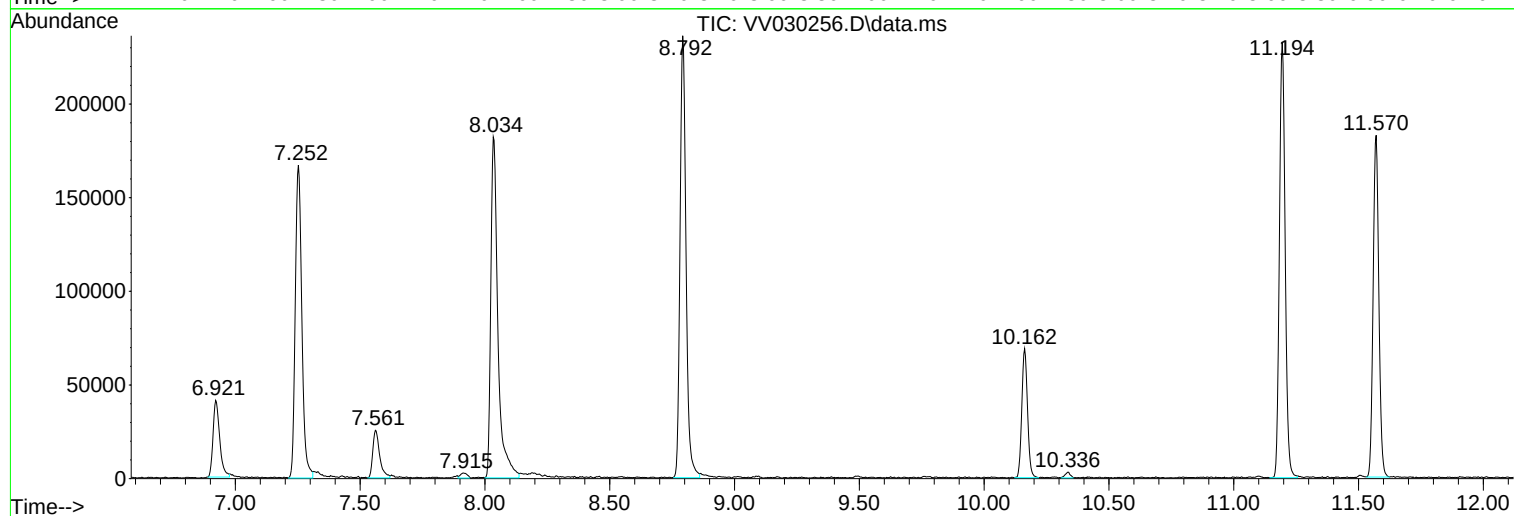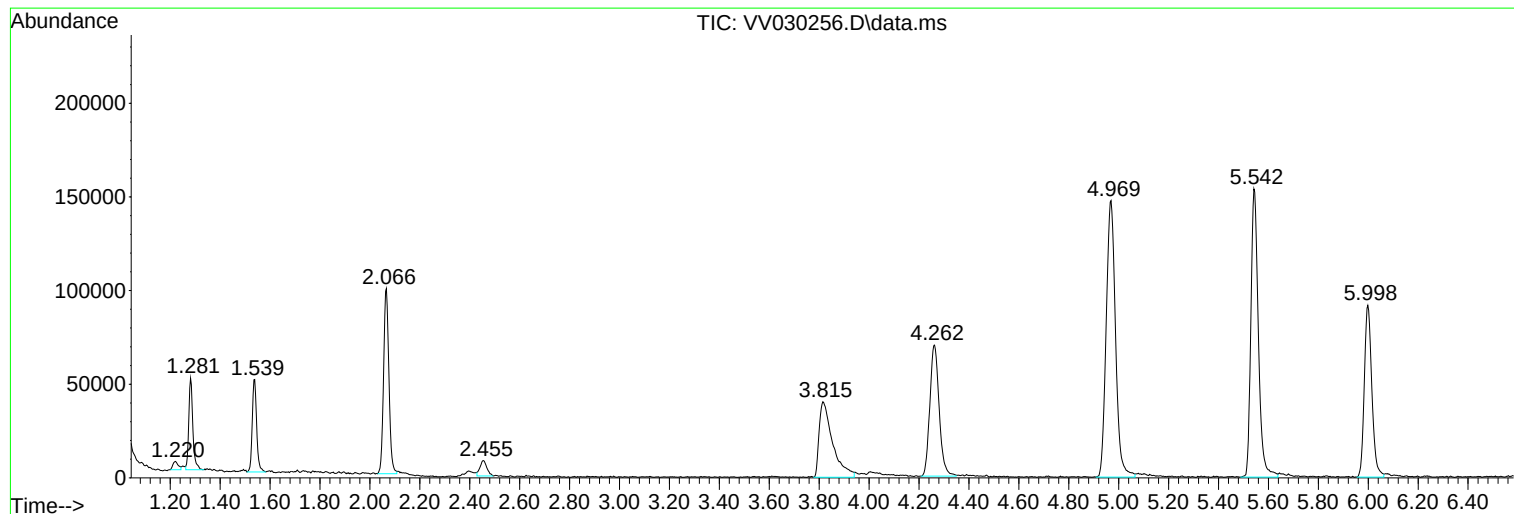

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030256.D
Acq On : 20 Mar 2023 14:18
Operator : SY/MD
Sample : 01997-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030256.D
Acq On : 20 Mar 2023 14:18
Operator : SY/MD
Sample : 01997-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc