

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030258.D
 Acq On : 20 Mar 2023 15:07
 Operator : SY/MD
 Sample : 01997-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	51	57	61	rBV4	3581	4466	1.25%	0.143%
2	1.282	69	75	89	rVB	45399	50956	14.23%	1.628%
3	1.539	147	155	169	rVB	45254	53646	14.98%	1.713%
4	2.066	308	319	335	rVB	87963	130298	36.39%	4.162%
5	3.825	854	866	899	rBV2	29872	116665	32.58%	3.726%
6	4.259	986	1001	1026	rBV	61547	160028	44.70%	5.111%
7	4.970	1202	1222	1244	rBV3	126437	334545	93.44%	10.686%
8	5.545	1385	1401	1425	rBV	139641	292842	81.79%	9.354%
9	5.998	1529	1542	1561	rBV2	77438	165920	46.34%	5.300%
10	6.921	1816	1829	1849	rBV2	35413	70039	19.56%	2.237%
11	7.252	1920	1932	1952	rBV	147692	268970	75.12%	8.591%
12	7.561	2018	2028	2042	rBV2	21769	41746	11.66%	1.333%
13	7.915	2122	2138	2157	rVB2	43155	78166	21.83%	2.497%
14	8.037	2165	2176	2201	rBV	151359	299884	83.76%	9.578%
15	8.793	2399	2411	2435	rBV	209218	358039	100.00%	11.436%
16	10.162	2819	2837	2849	rBV	61712	97165	27.14%	3.103%
17	10.336	2882	2891	2901	rBV5	4182	6549	1.83%	0.209%
18	11.194	3146	3158	3177	rBV	215986	343713	96.00%	10.978%
19	11.571	3264	3275	3294	rVB	161165	257184	71.83%	8.215%




Sum of corrected areas: 3130821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030258.D
Acq On : 20 Mar 2023 15:07
Operator : SY/MD
Sample : 01997-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

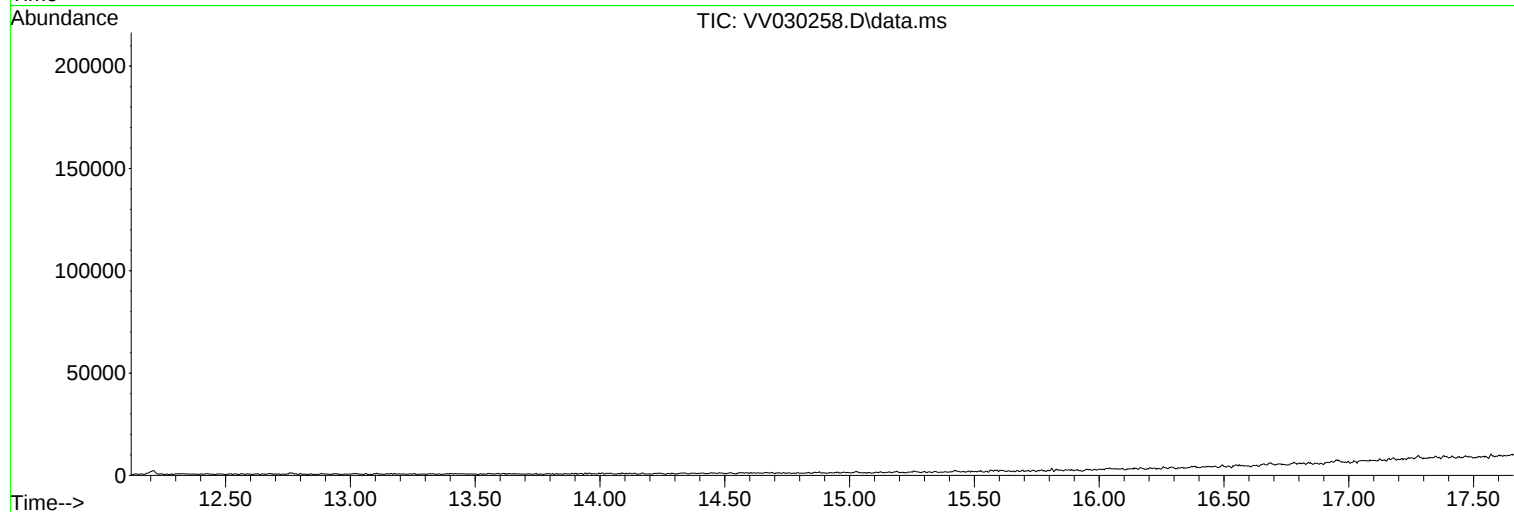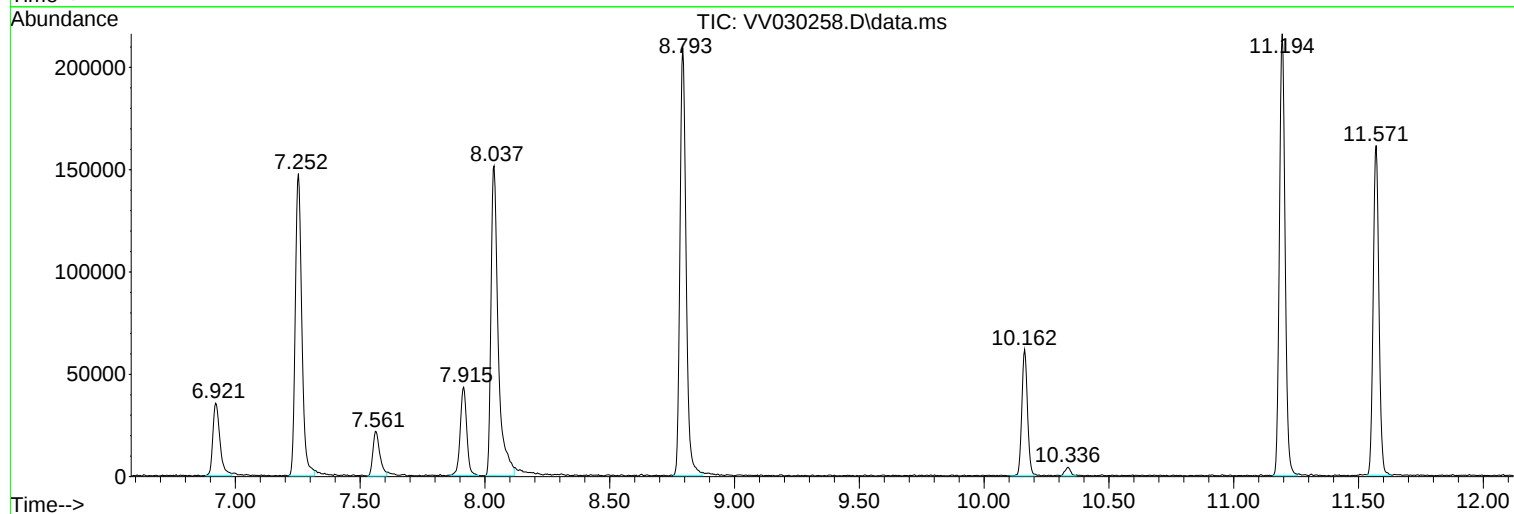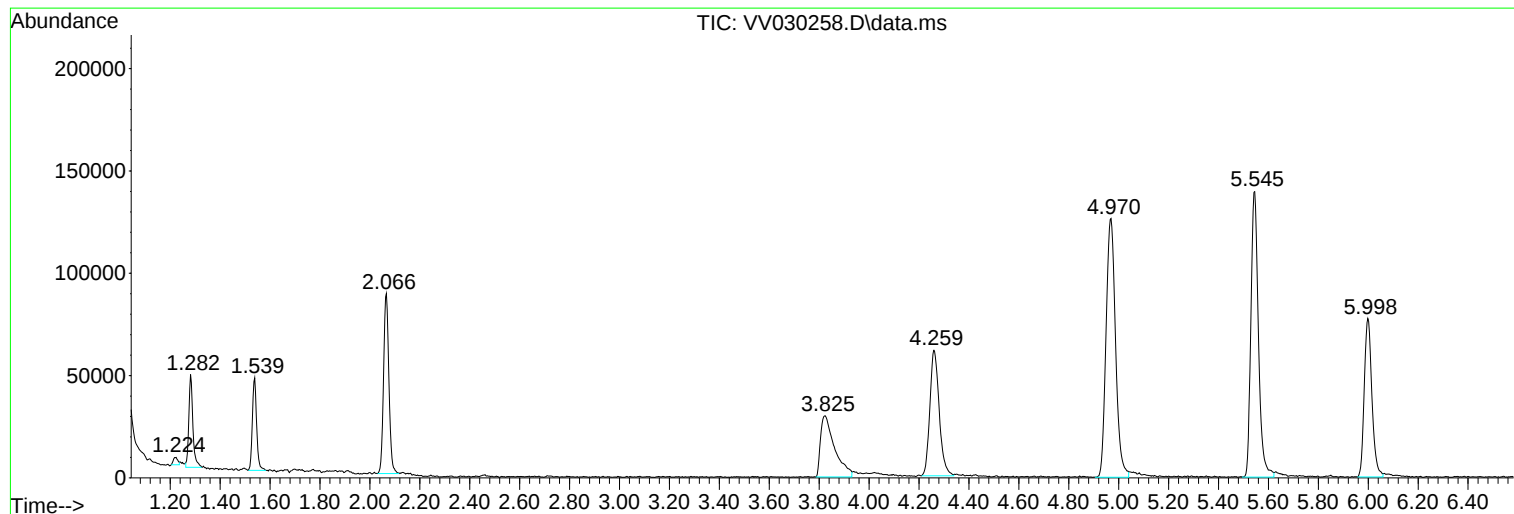

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030258.D
Acq On : 20 Mar 2023 15:07
Operator : SY/MD
Sample : 01997-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030258.D
Acq On : 20 Mar 2023 15:07
Operator : SY/MD
Sample : 01997-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
