

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030265.D
 Acq On : 20 Mar 2023 18:21
 Operator : SY/MD
 Sample : 01996-04DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A25DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	41662	44493	6.03%	1.149%
2	1.539	147	155	164	rBV	44147	52079	7.06%	1.345%
3	2.066	307	319	335	rBV2	94130	149568	20.28%	3.862%
4	2.455	431	440	453	rBV2	7555	12651	1.72%	0.327%
5	3.815	851	863	894	rBV	36844	130095	17.64%	3.359%
6	4.262	983	1002	1025	rBV	62304	160150	21.72%	4.135%
7	4.969	1204	1222	1242	rBV2	131488	335344	45.48%	8.659%
8	5.545	1387	1401	1418	rBV	134807	280104	37.99%	7.233%
9	5.844	1483	1494	1511	rBV2	36020	73783	10.01%	1.905%
10	5.998	1529	1542	1560	rBV2	78122	165136	22.40%	4.264%
11	6.924	1819	1830	1847	rBV	35835	67609	9.17%	1.746%
12	7.252	1919	1932	1954	rBV	151419	272529	36.96%	7.037%
13	7.561	2017	2028	2047	rBV3	21671	41506	5.63%	1.072%
14	7.915	2124	2138	2160	rBV	432322	737348	100.00%	19.040%
15	8.034	2165	2175	2211	rVV	165571	316404	42.91%	8.170%
16	8.792	2400	2411	2431	rBV	208062	344399	46.71%	8.893%
17	10.162	2826	2837	2855	rVB	60459	97792	13.26%	2.525%
18	11.194	3145	3158	3174	rBV	207495	331402	44.95%	8.558%
19	11.571	3264	3275	3288	rBV	164486	260244	35.29%	6.720%




Sum of corrected areas: 3872636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030265.D
Acq On : 20 Mar 2023 18:21
Operator : SY/MD
Sample : 01996-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

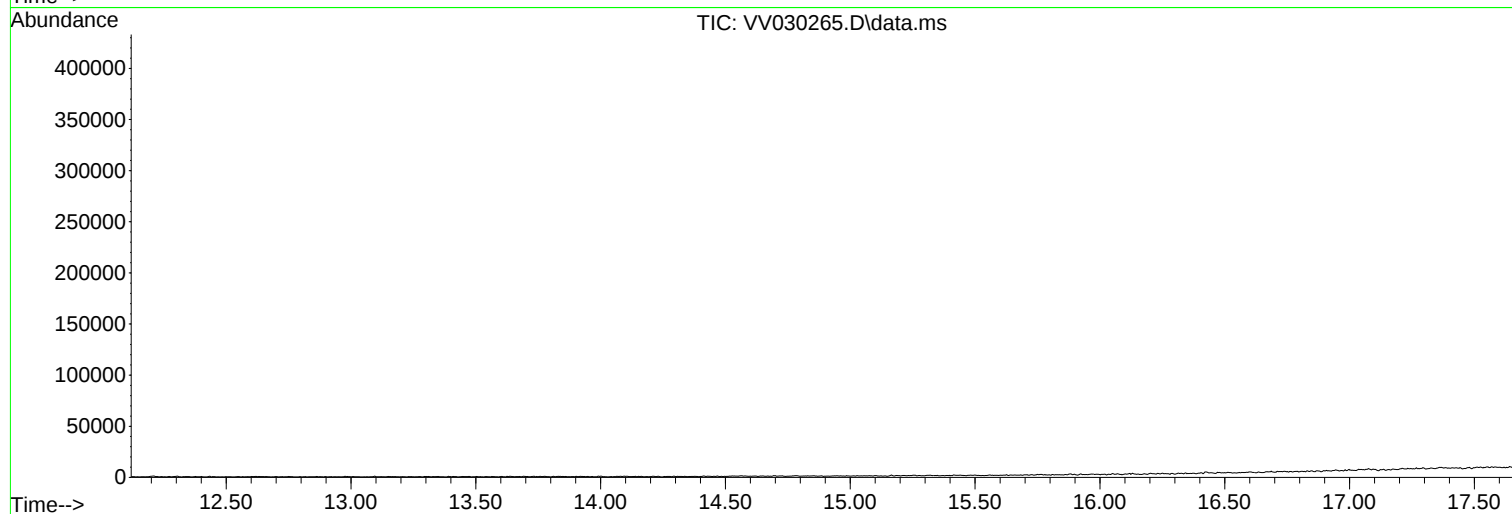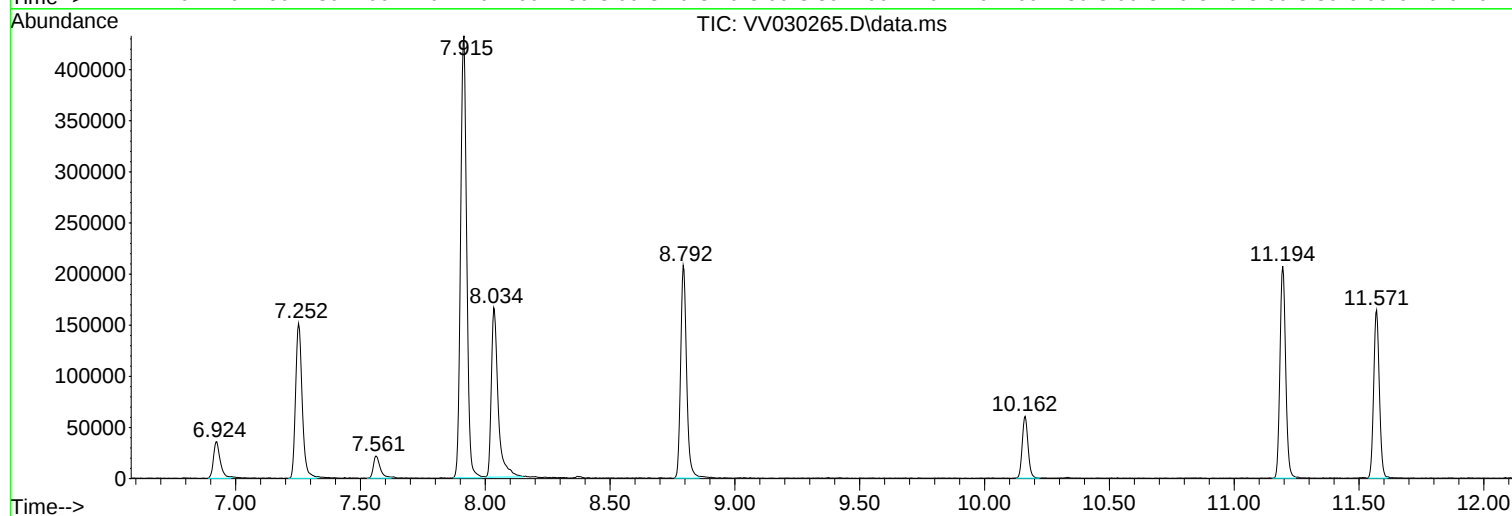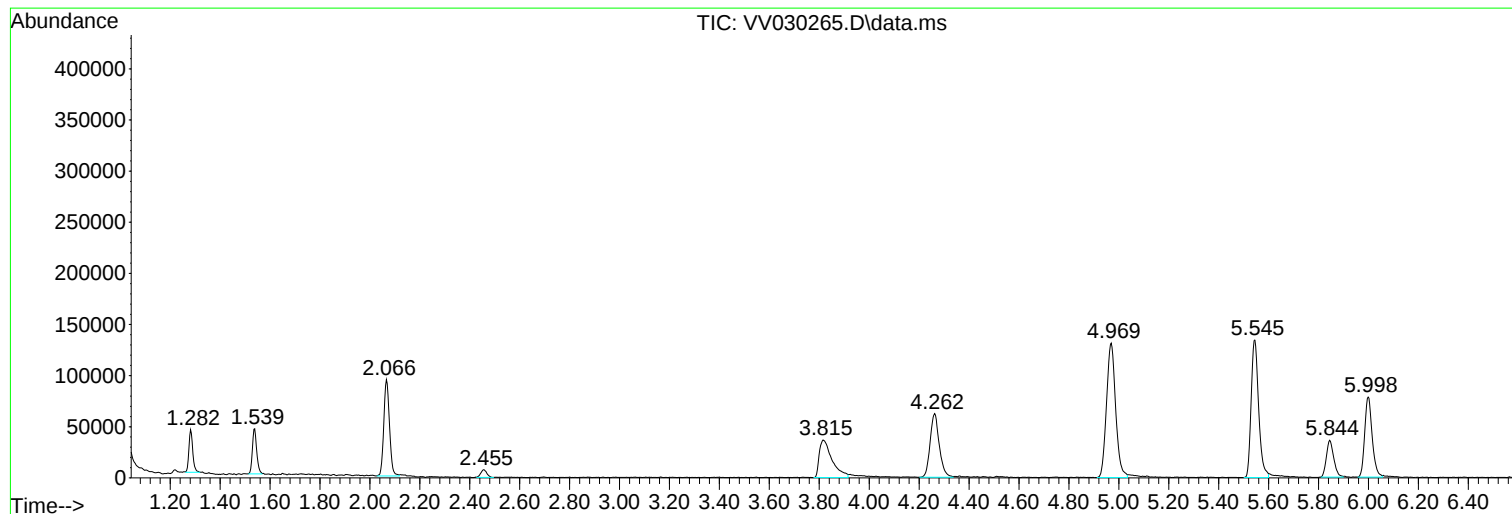

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030265.D
Acq On : 20 Mar 2023 18:21
Operator : SY/MD
Sample : 01996-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030265.D
Acq On : 20 Mar 2023 18:21
Operator : SY/MD
Sample : 01996-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------