

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
 Data File : VV030267.D
 Acq On : 20 Mar 2023 19:10
 Operator : SY/MD
 Sample : 01996-06DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A27DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	40415	45011	4.62%	1.089%
2	1.539	147	155	166	rBV	43678	52282	5.37%	1.265%
3	2.069	306	320	337	rBV2	111165	186352	19.14%	4.510%
4	2.455	428	440	453	rBV3	9066	15338	1.58%	0.371%
5	3.815	853	863	895	rBV	32797	115718	11.89%	2.801%
6	4.262	984	1002	1028	rBV2	60800	163630	16.81%	3.960%
7	4.526	1072	1084	1099	rVB6	4085	9961	1.02%	0.241%
8	4.969	1205	1222	1261	rBV2	124269	327347	33.63%	7.923%
9	5.545	1388	1401	1423	rBV	130248	274075	28.15%	6.634%
10	5.844	1482	1494	1522	rBV2	65556	134459	13.81%	3.254%
11	5.998	1527	1542	1559	rBV	77330	161291	16.57%	3.904%
12	6.924	1819	1830	1845	rBV	33767	64246	6.60%	1.555%
13	7.252	1918	1932	1957	rBV	145300	263124	27.03%	6.368%
14	7.564	2016	2029	2043	rBV2	21942	39656	4.07%	0.960%
15	7.915	2124	2138	2162	rBV	567818	973490	100.00%	23.562%
16	8.034	2165	2175	2214	rVV	154856	301558	30.98%	7.299%
17	8.792	2399	2411	2436	rBV	198527	338234	34.74%	8.186%
18	10.162	2827	2837	2850	rBV	57617	91283	9.38%	2.209%
19	11.194	3147	3158	3180	rBV	204931	321708	33.05%	7.786%
20	11.570	3264	3275	3290	rBV	158713	252906	25.98%	6.121%




Sum of corrected areas: 4131669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030267.D
Acq On : 20 Mar 2023 19:10
Operator : SY/MD
Sample : 01996-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

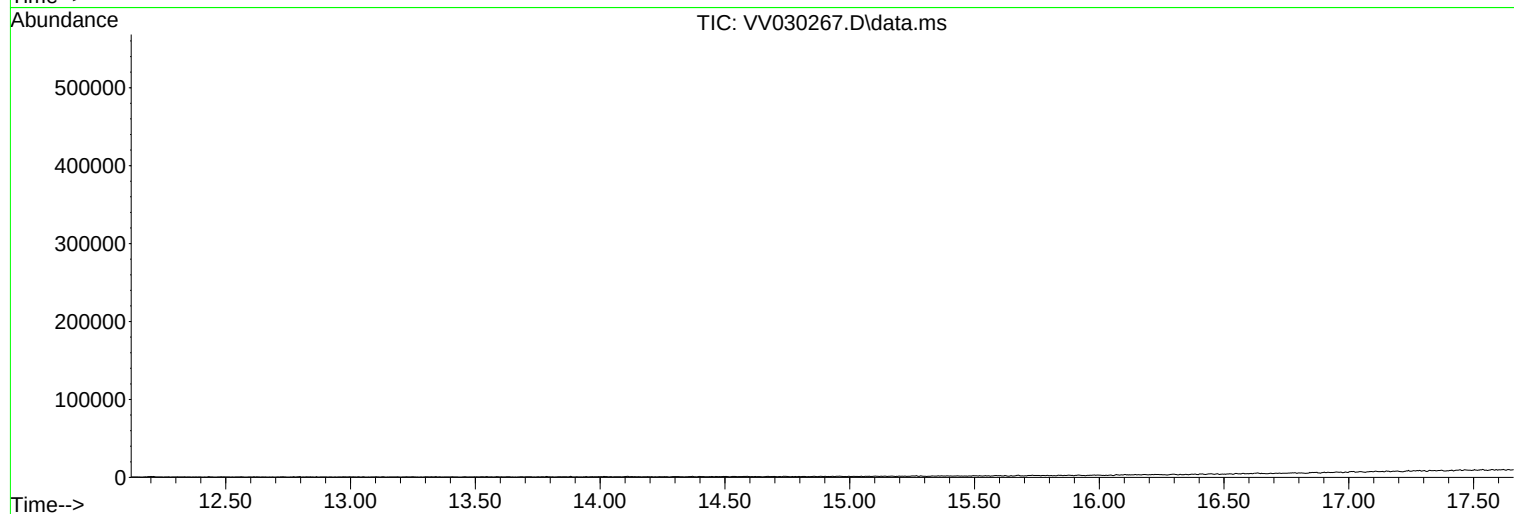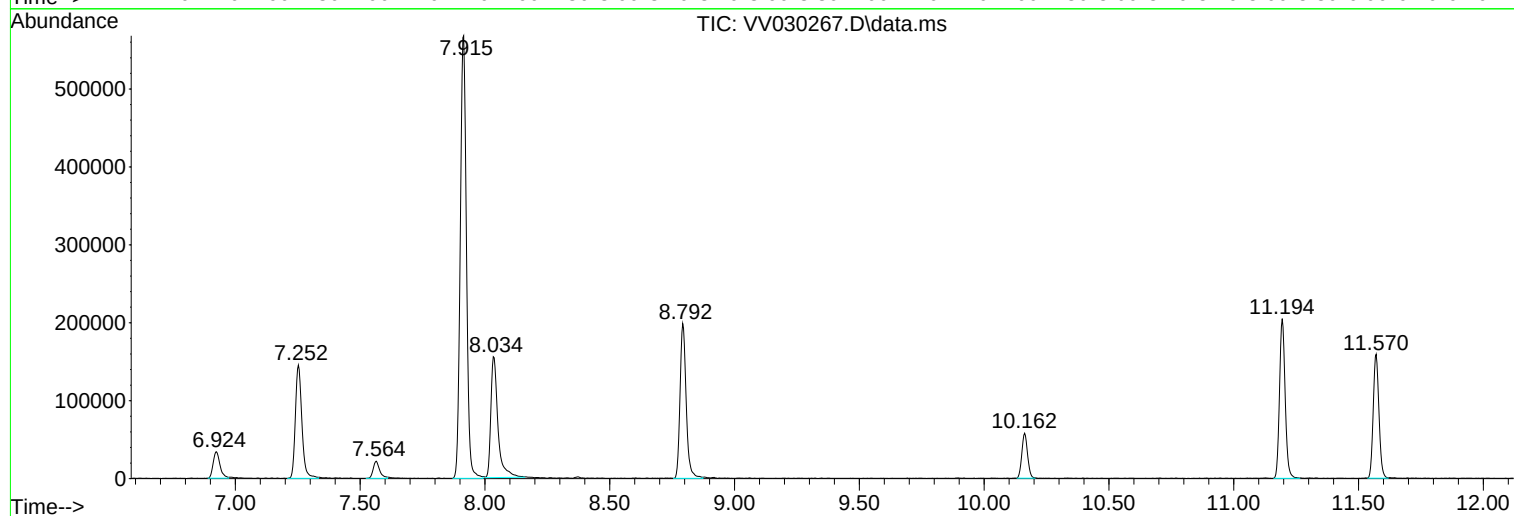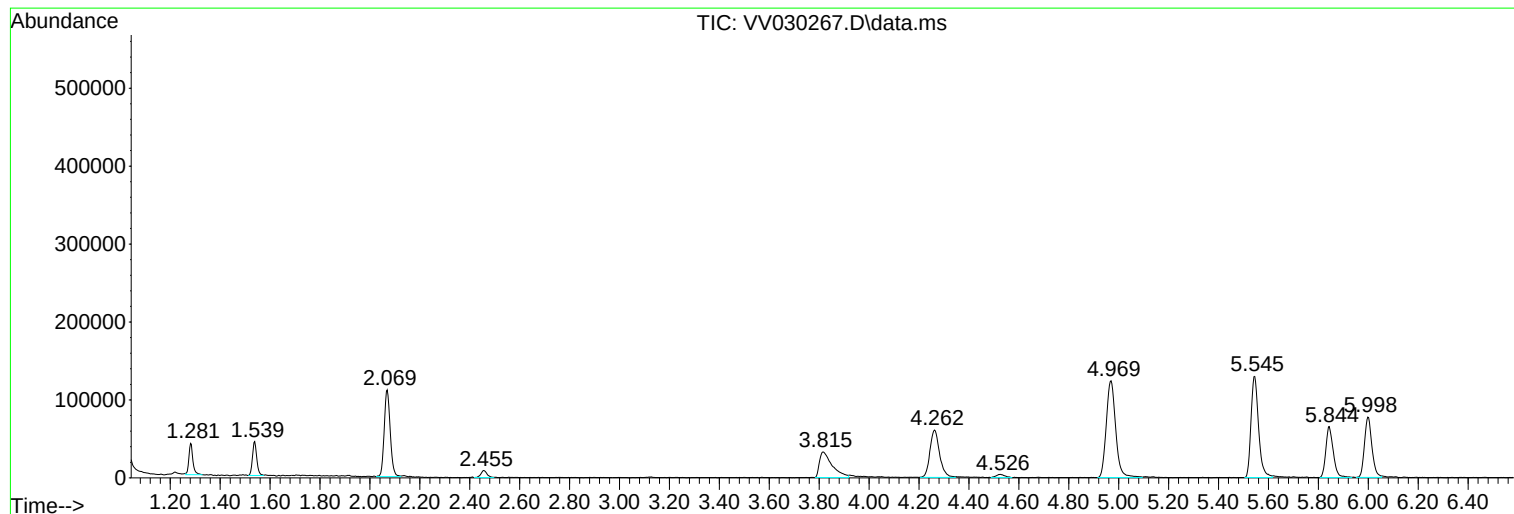

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030267.D
Acq On : 20 Mar 2023 19:10
Operator : SY/MD
Sample : 01996-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030267.D
Acq On : 20 Mar 2023 19:10
Operator : SY/MD
Sample : 01996-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------