


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032023\
Data File : VV030246.D
Acq On : 20 Mar 2023 08:42
Operator : SY/MD
Sample : BFB235
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB235

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 17 22:49:08 2023

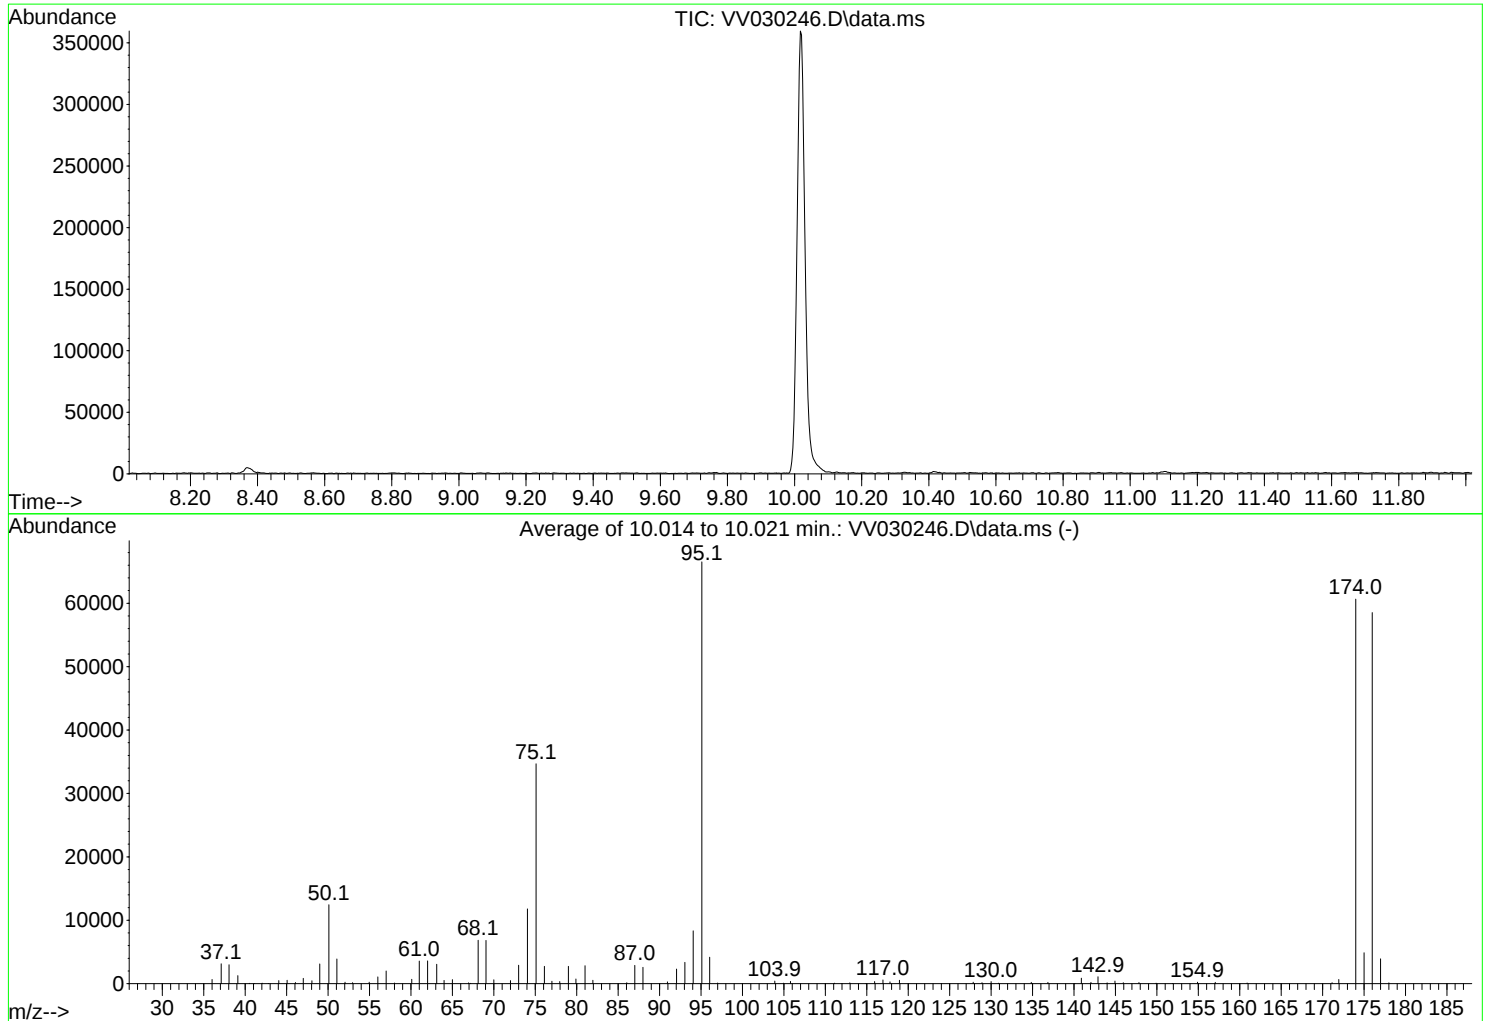

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	12452	PASS
75	95	30	80	52.1	34680	PASS
95	95	100	100	100.0	66531	PASS
96	95	5	9	6.3	4173	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.1	60643	PASS
175	174	5	9	8.0	4881	PASS
176	174	95	105	96.5	58536	PASS
177	176	5	10	6.7	3919	PASS

m/z	Abundance
39.90	265.0
43.70	161.0
44.20	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	604.0
37.10	3096.0
38.00	2825.0
39.10	1210.0
39.90	249.0
42.00	115.0
44.10	675.0
45.10	467.0
46.10	163.0
47.00	731.0
48.00	465.0
49.00	2998.0
50.10	11934.0
51.00	3837.0
52.00	198.0
52.90	152.0
55.00	212.0
56.00	1114.0
57.00	1943.0
60.10	643.0
61.00	3352.0
62.00	3335.0
63.10	2833.0
64.00	454.0
65.00	574.0
66.90	192.0
68.10	6664.0
69.00	6630.0
70.00	575.0
72.00	480.0
73.00	2633.0
74.00	11429.0
75.10	32664.0
76.10	2723.0
77.00	311.0
78.00	374.0
79.00	2587.0
79.90	626.0
81.00	2530.0
81.90	487.0
86.10	166.0
87.00	2886.0
88.00	2452.0
91.00	246.0
92.00	2157.0
93.00	3040.0
94.10	8031.0
95.10	63264.0
96.10	4181.0
97.00	190.0
103.90	382.0
105.80	339.0
111.10	146.0
113.00	138.0
114.90	110.0
115.90	308.0
117.00	579.0
117.80	274.0
118.90	473.0
127.80	210.0
128.90	142.0
130.00	325.0
130.90	123.0
134.90	180.0
136.80	186.0
140.90	785.0
142.00	223.0
142.90	1042.0
144.00	103.0
145.00	384.0
145.90	161.0
147.90	149.0
151.90	106.0
154.90	218.0
157.10	186.0
171.20	148.0
172.00	579.0
174.00	56304.0
175.00	4590.0
176.00	54344.0
177.00	3661.0
178.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	679.0
37.10	3207.0
38.10	3023.0
39.10	1265.0
39.90	232.0
42.10	102.0
42.80	100.0
44.00	627.0
45.00	539.0
46.10	177.0
47.00	889.0
48.10	429.0
49.00	3220.0
50.10	12836.0
51.10	3967.0
52.00	239.0
53.00	169.0
55.00	238.0
56.00	1118.0
57.00	2079.0
58.00	117.0
60.10	711.0
61.00	3716.0
62.00	3691.0
63.10	3162.0
64.00	520.0
65.00	677.0
67.00	197.0
68.10	7098.0
69.10	7053.0
70.00	613.0
72.00	476.0
73.00	3003.0
74.10	12090.0
75.10	35832.0
76.10	2780.0
77.00	396.0
78.00	346.0
79.00	2811.0
79.90	775.0
81.00	2933.0
81.90	544.0
86.10	155.0
87.00	2980.0
88.00	2670.0
90.90	288.0
92.00	2362.0
93.10	3552.0
94.10	8573.0
95.10	68760.0
96.00	4268.0
97.00	150.0
103.90	417.0
105.00	114.0
105.80	375.0
111.10	109.0
112.90	126.0
115.90	346.0
117.00	585.0
117.80	294.0
118.90	516.0
127.80	217.0
128.90	155.0
130.00	355.0
130.90	110.0
134.80	207.0
136.80	206.0
140.90	880.0
142.10	209.0
142.90	1125.0
144.00	121.0
145.00	407.0
146.00	172.0
147.90	183.0
149.90	107.0
154.90	246.0
157.10	207.0
160.90	138.0
171.10	156.0
171.90	682.0
174.00	62536.0
175.00	5060.0
176.00	60648.0
177.00	4037.0
178.00	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	674.0
37.10	3107.0
38.10	3075.0
39.10	1298.0
40.00	213.0
40.50	149.0
41.10	110.0
44.00	575.0
45.00	622.0
46.00	165.0
47.00	897.0
48.00	446.0
49.00	3076.0
50.10	12587.0
51.10	3825.0
52.10	260.0
53.00	173.0
54.90	221.0
56.00	982.0
57.00	1955.0
58.00	159.0
60.10	664.0
61.00	3625.0
62.00	3742.0
63.10	3203.0
64.00	570.0
65.00	669.0
67.20	182.0
68.10	6722.0
69.10	6750.0
70.00	610.0
72.00	456.0
73.00	3109.0
74.10	11836.0
75.10	35544.0
76.10	2704.0
77.00	466.0
77.90	306.0
79.00	2777.0
79.90	802.0
81.00	3049.0
82.00	555.0
86.00	136.0
87.00	2786.0
88.00	2597.0
90.90	305.0
92.10	2400.0
93.10	3487.0
94.00	8402.0
95.10	67568.0
96.00	4070.0
103.90	432.0
104.90	104.0
105.80	365.0
112.00	103.0
112.90	106.0
116.00	335.0
116.90	570.0
117.80	251.0
119.00	608.0
124.00	103.0
127.90	244.0
128.90	156.0
130.00	326.0
134.80	204.0
136.90	207.0
140.10	110.0
140.90	898.0
142.10	165.0
142.90	1114.0
144.00	136.0
144.90	392.0
146.00	132.0
147.80	183.0
149.90	104.0
154.90	245.0
157.00	214.0
160.90	166.0
171.10	125.0
171.90	715.0
174.00	63088.0
175.00	4993.0
176.00	60616.0
177.00	4059.0
178.00	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235