
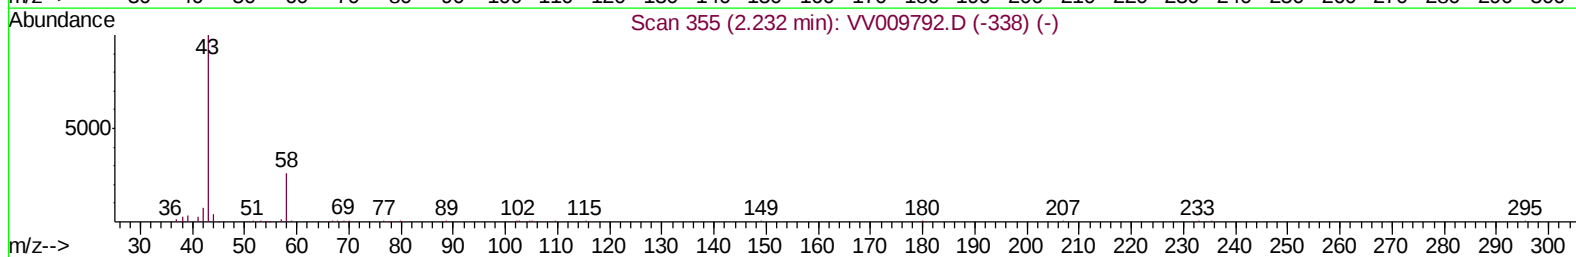
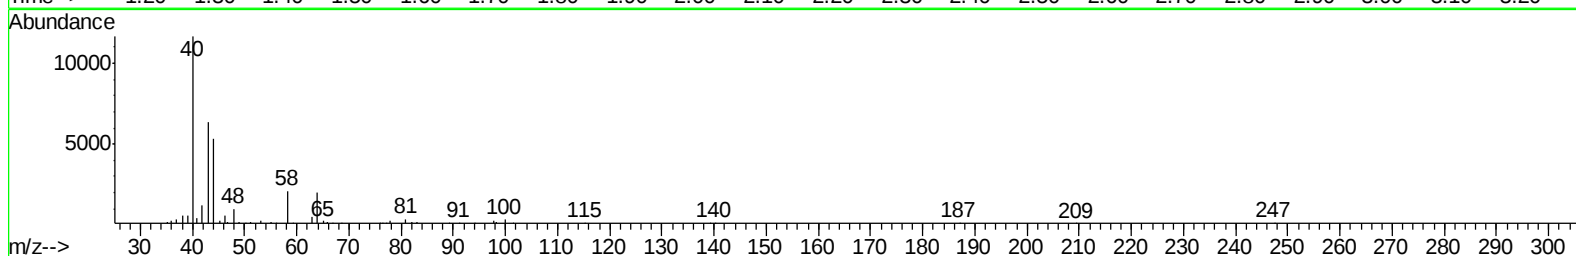


Data File : VV009797.D
Acq On : 21 Mar 2019 15:35
Operator : SY/MD
Sample : K1955-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 22 07:56:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 21 15:15:58 2019
Response via : Initial Calibration

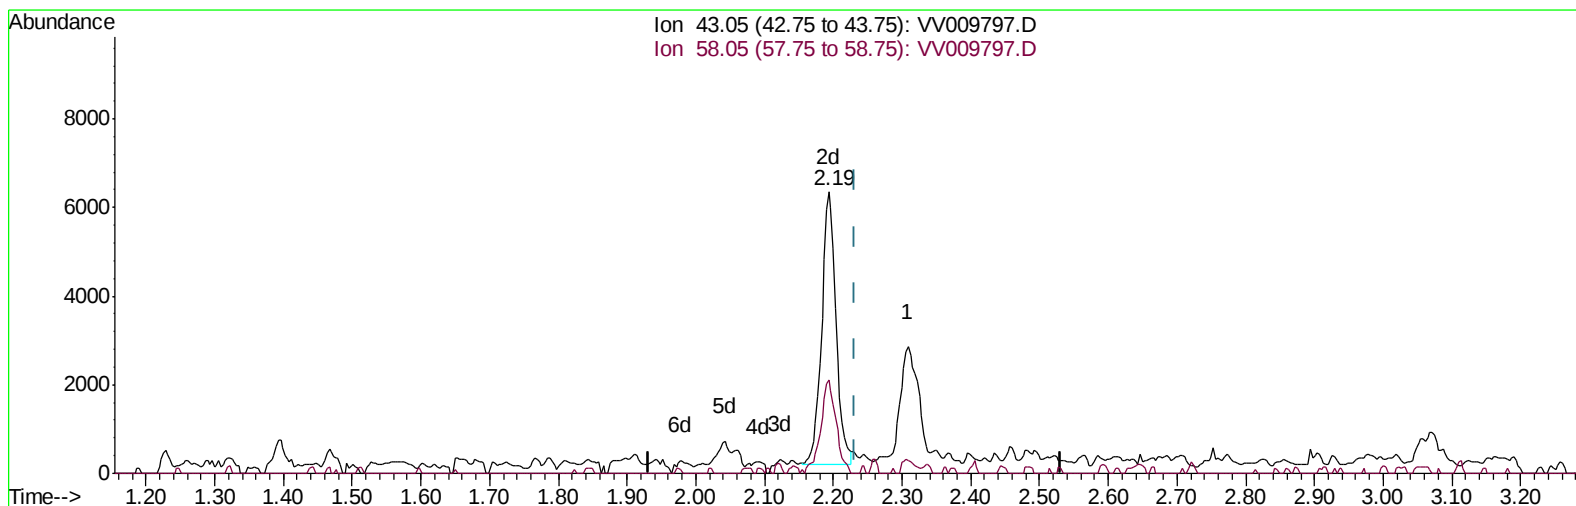

TIC: VV009797.D

(13) Acetone (T)

2.193min (-0.039) 4.25ug/L m

response 8963

Ion	Exp%	Act%
43.05	100	100
58.05	11.50	4.40
0.00	0.00	0.00
0.00	0.00	0.00