

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

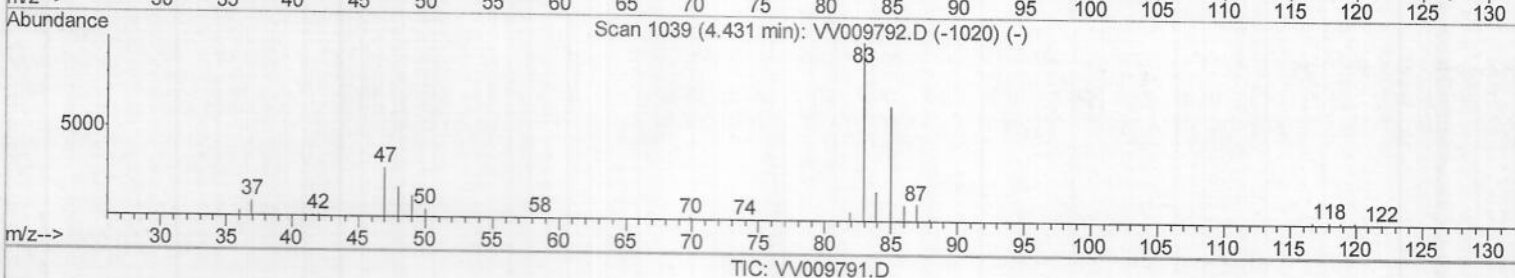
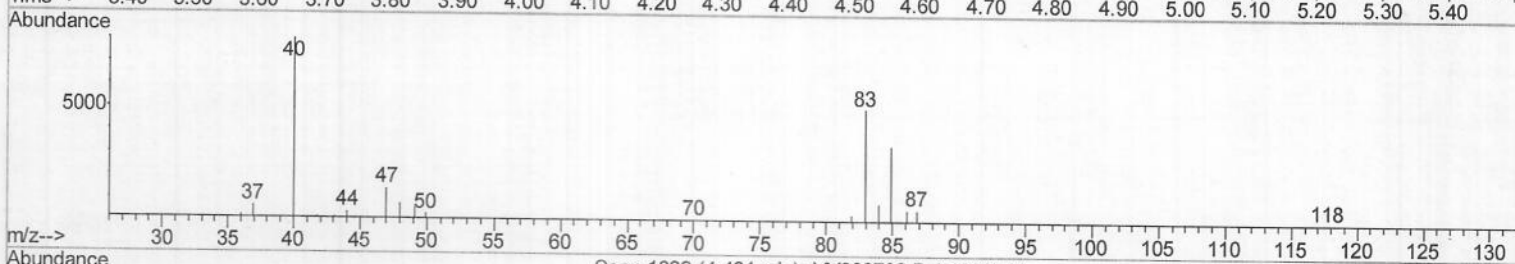
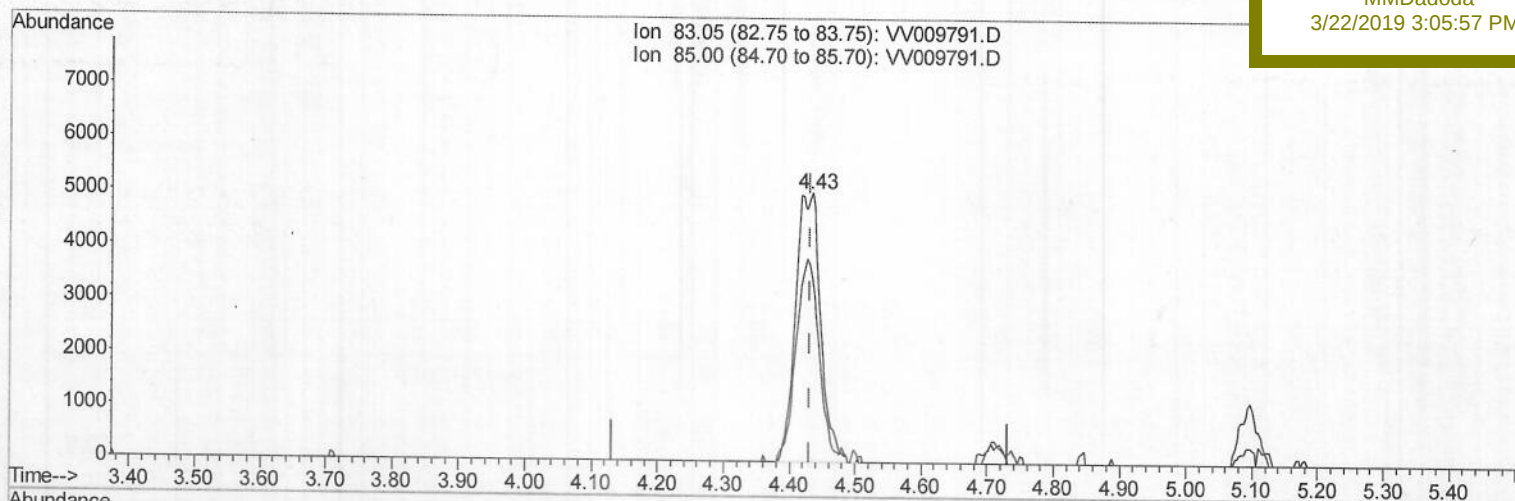
Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampled :

VSTD00132

Manual Integrations
APPROVEDMMDadoda
3/22/2019 3:05:57 PM

(25) Chloroform (T)

4.434min (+0.003) 0.99ug/L m

response 13246

Ion Exp% Act%

83.05 100 100

85.00 65.30 67.71

0.00 0.00 0.00

0.00 0.00 0.00

m.p
03/26/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

Client Sampled :

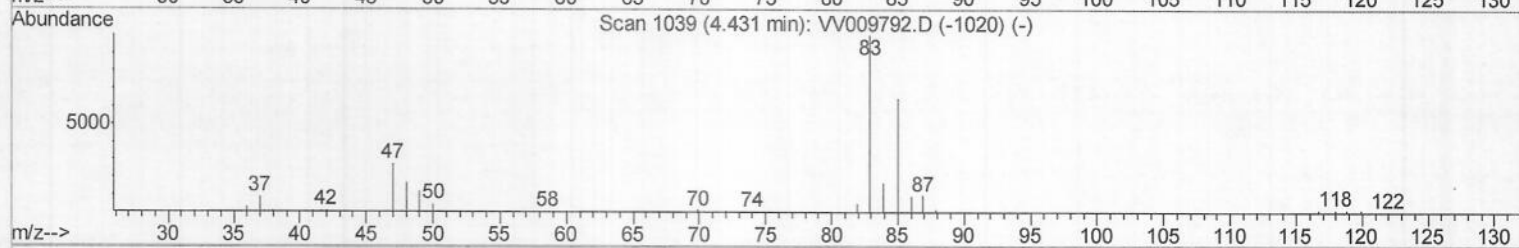
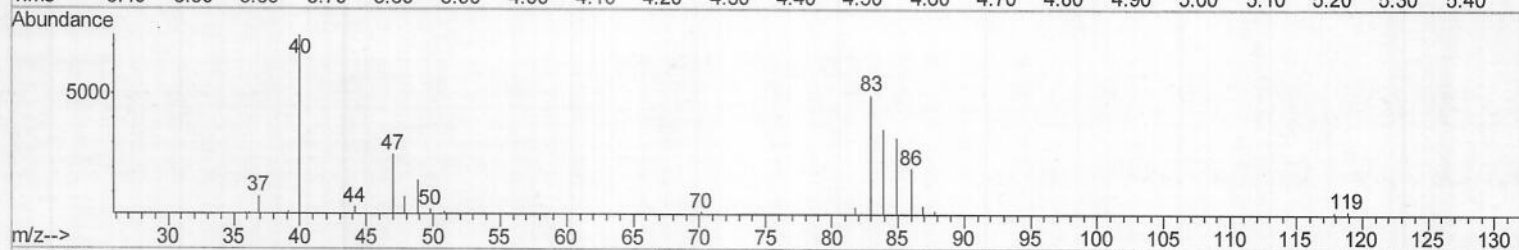
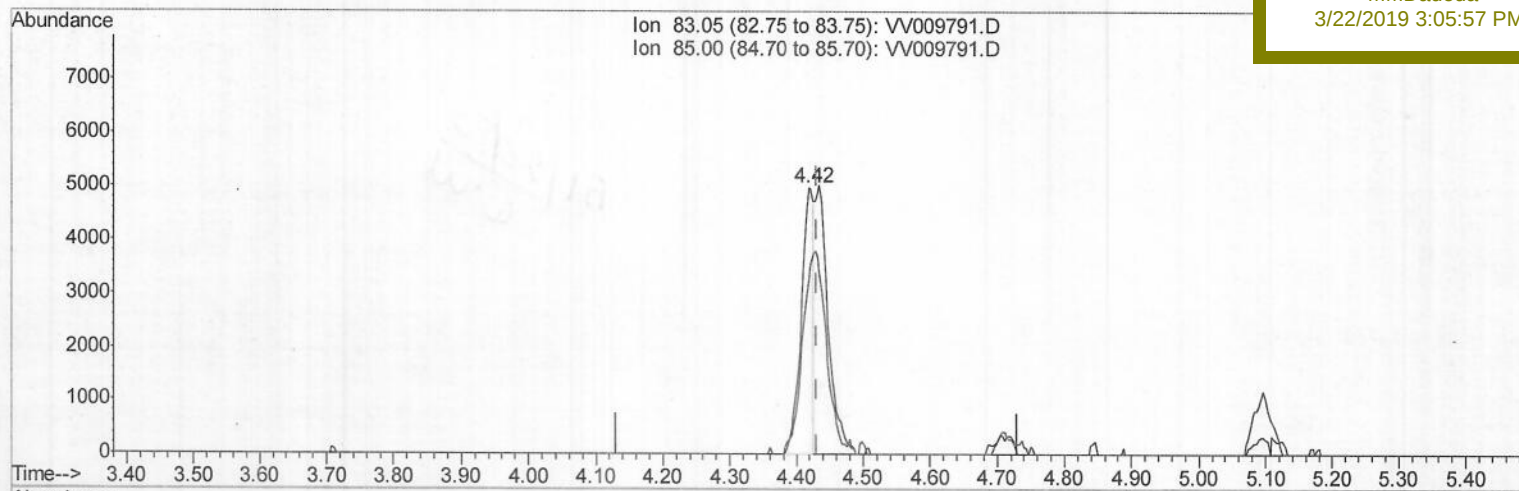
VSTD00132

Manual Integrations

APPROVED

MMDadoda

3/22/2019 3:05:57 PM



TIC: VV009791.D

(25) Chloroform (T)

4.418min (-0.013) 0.46ug/L

response 6156

Ion	Exp%	Act%
83.05	100	100
85.00	65.30	65.74
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

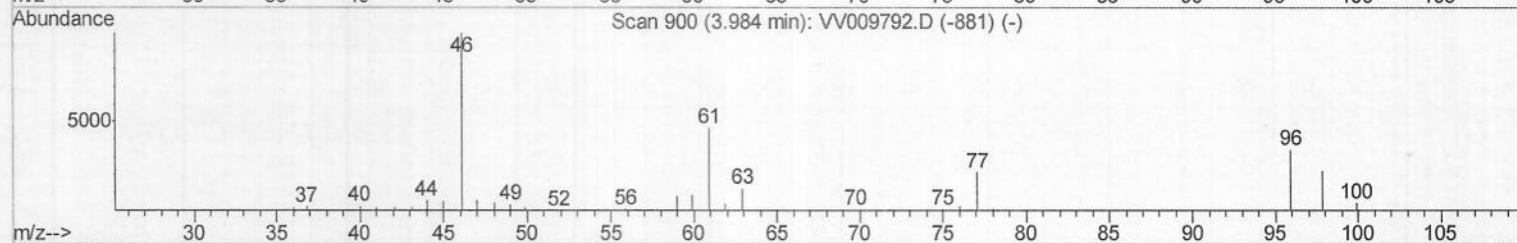
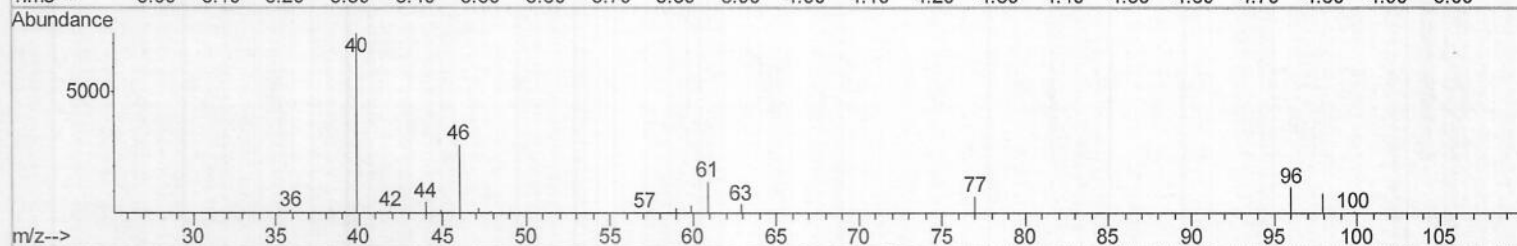
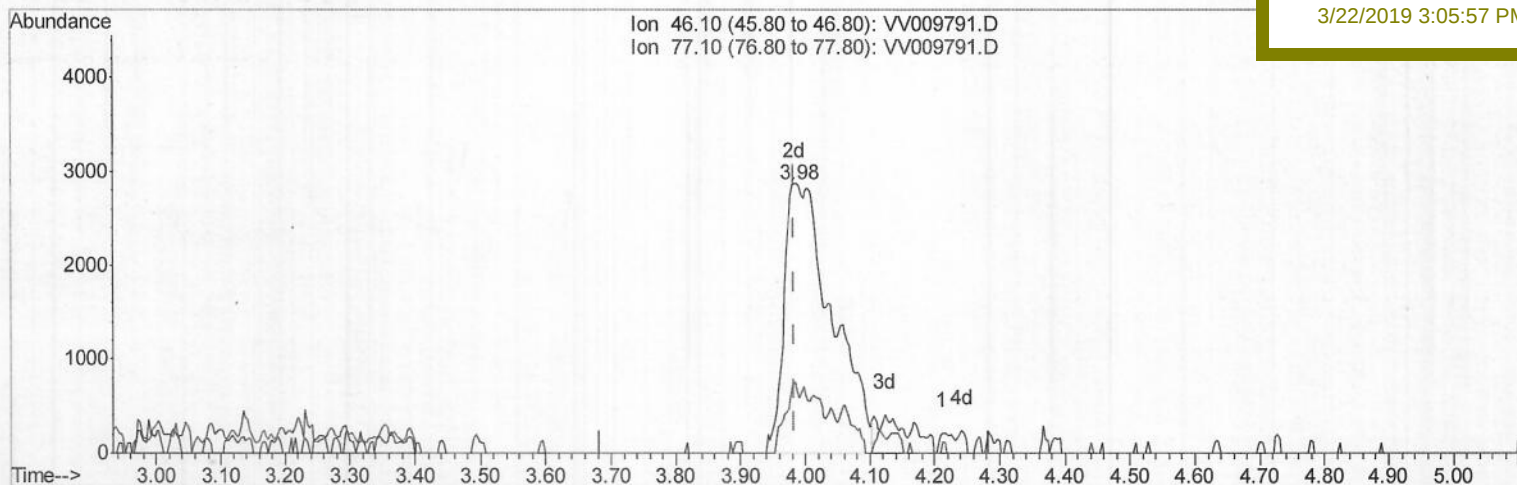
Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampled :

VSTD00132

Manual Integrations
APPROVEDMMDadoda
3/22/2019 3:05:57 PM

(20) 2-Butanone-d5 (S)

3.984min (-0.000) 11.25ug/L m

response 14776

Ion	Exp%	Act%
46.10	100	100
77.10	12.20	0.28#
0.00	0.00	0.00
0.00	0.00	0.00

M.P
03/26/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

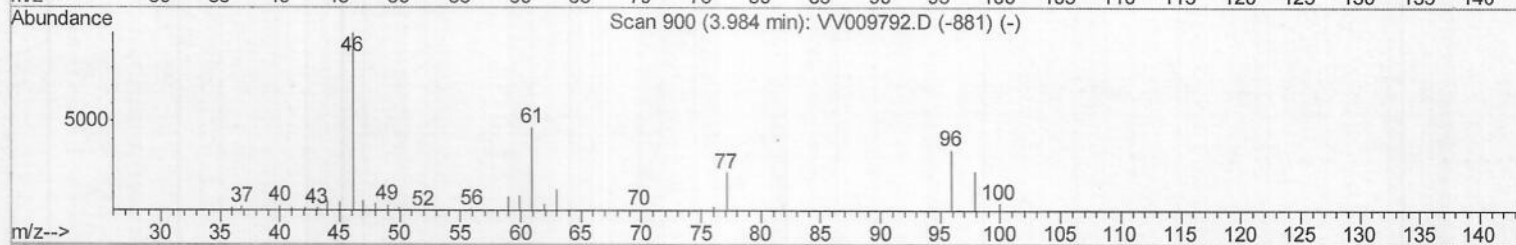
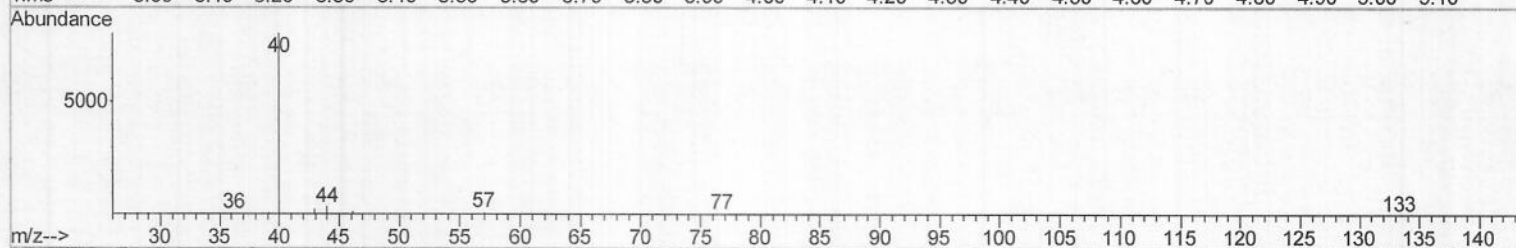
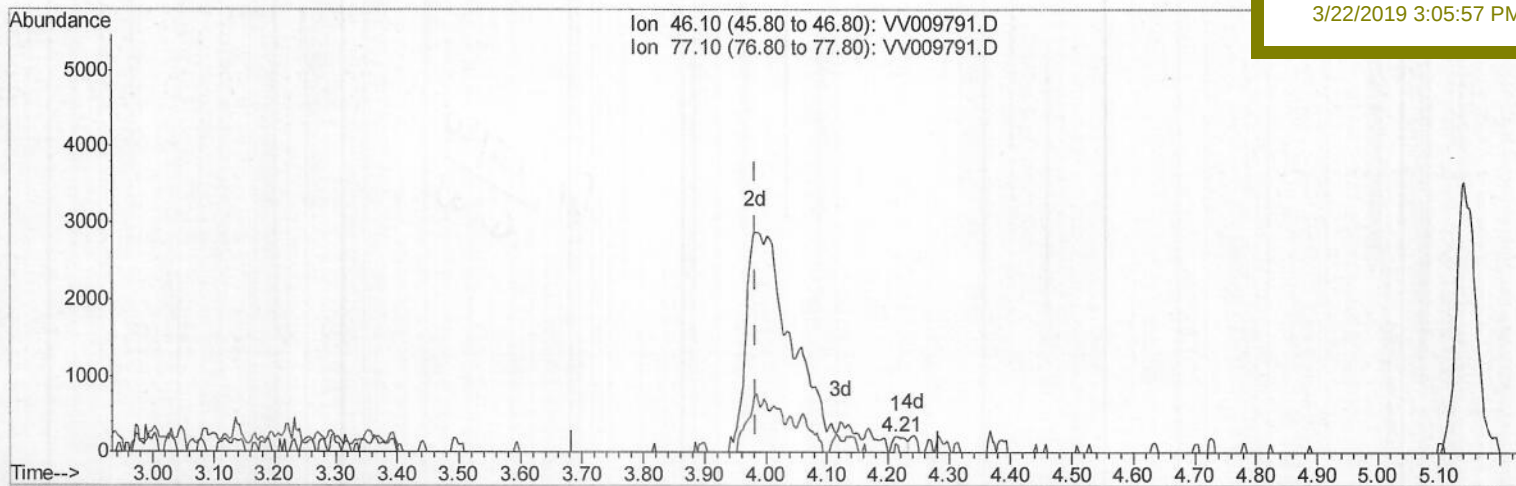
Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampled :

VSTD00132

Manual Integrations
APPROVEDMMDadoda
3/22/2019 3:05:57 PM

TIC: VV009791.D

(20) 2-Butanone-d5 (S)

4.213min (+0.228) 0.24ug/L

response 311

Ion	Exp%	Act%
46.10	100	100
77.10	12.20	13.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

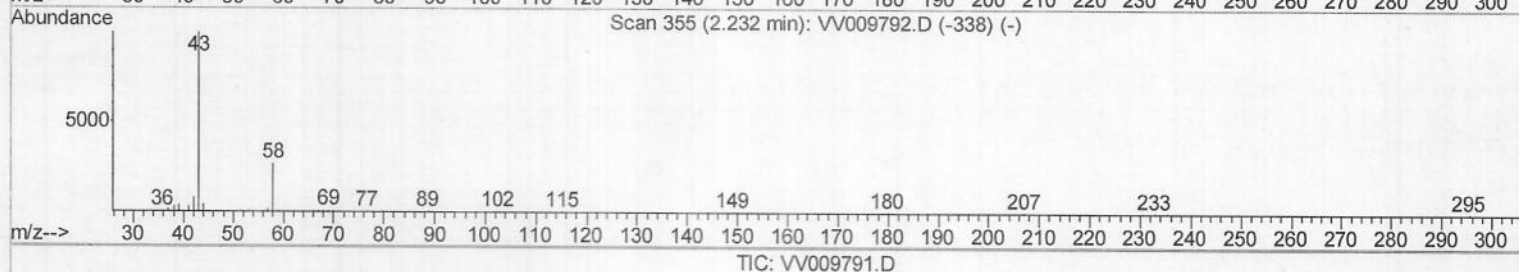
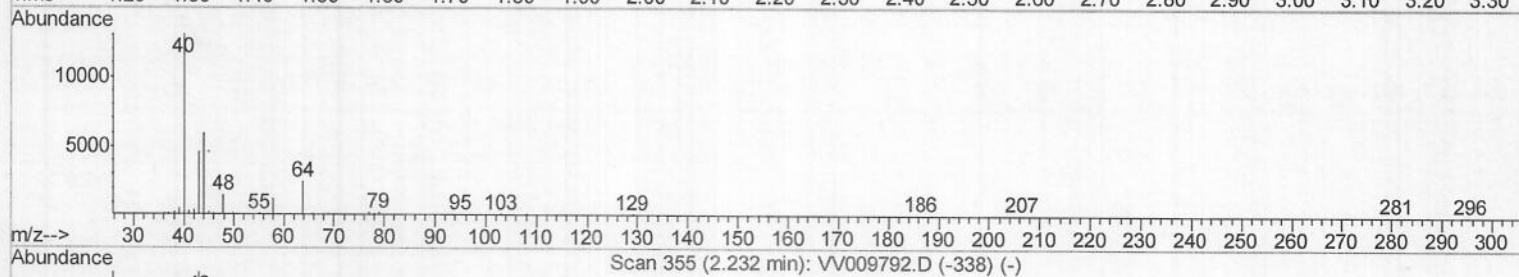
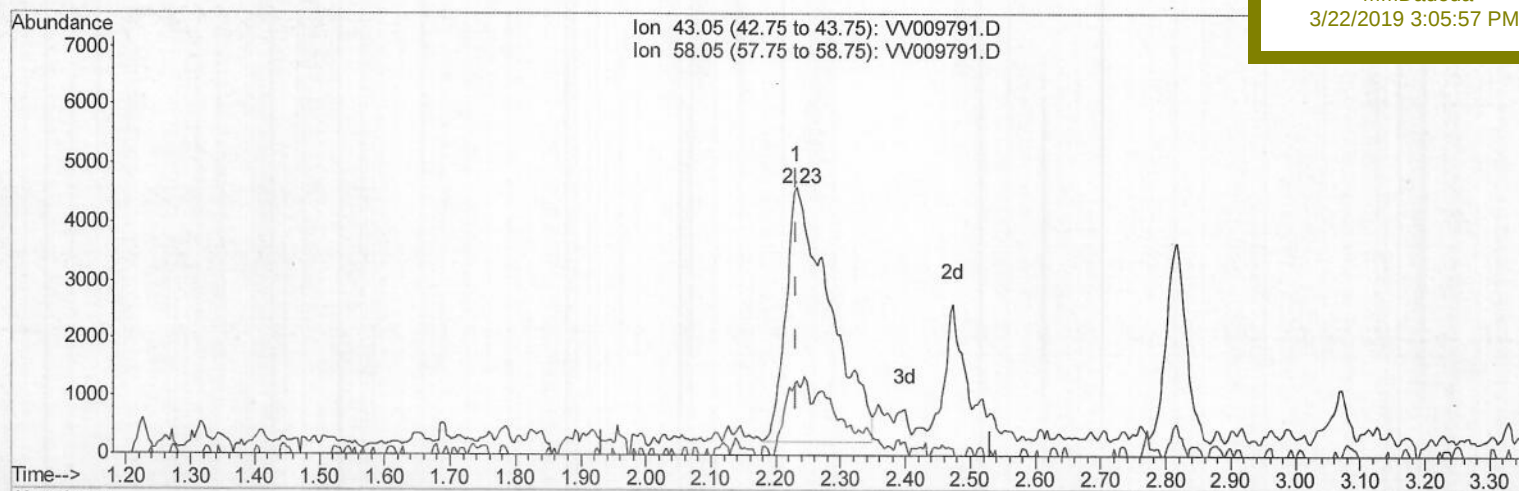
Response via : Initial Calibration

Instrument :

MSVOA_V

Client Sampled :

VSTD00132

Manual Integrations
APPROVEDMMDadoda
3/22/2019 3:05:57 PM

(13) Acetone (T)

2.232min (-0.000) 17.84ug/L m

response 20515

Ion	Exp%	Act%
43.05	100	100
58.05	11.50	10.58
0.00	0.00	0.00
0.00	0.00	0.00

m.p
03/26/19

Instrument :
MSVOA_V
ClientSampleId :
VSTD00132

Manual Integrations
APPROVED

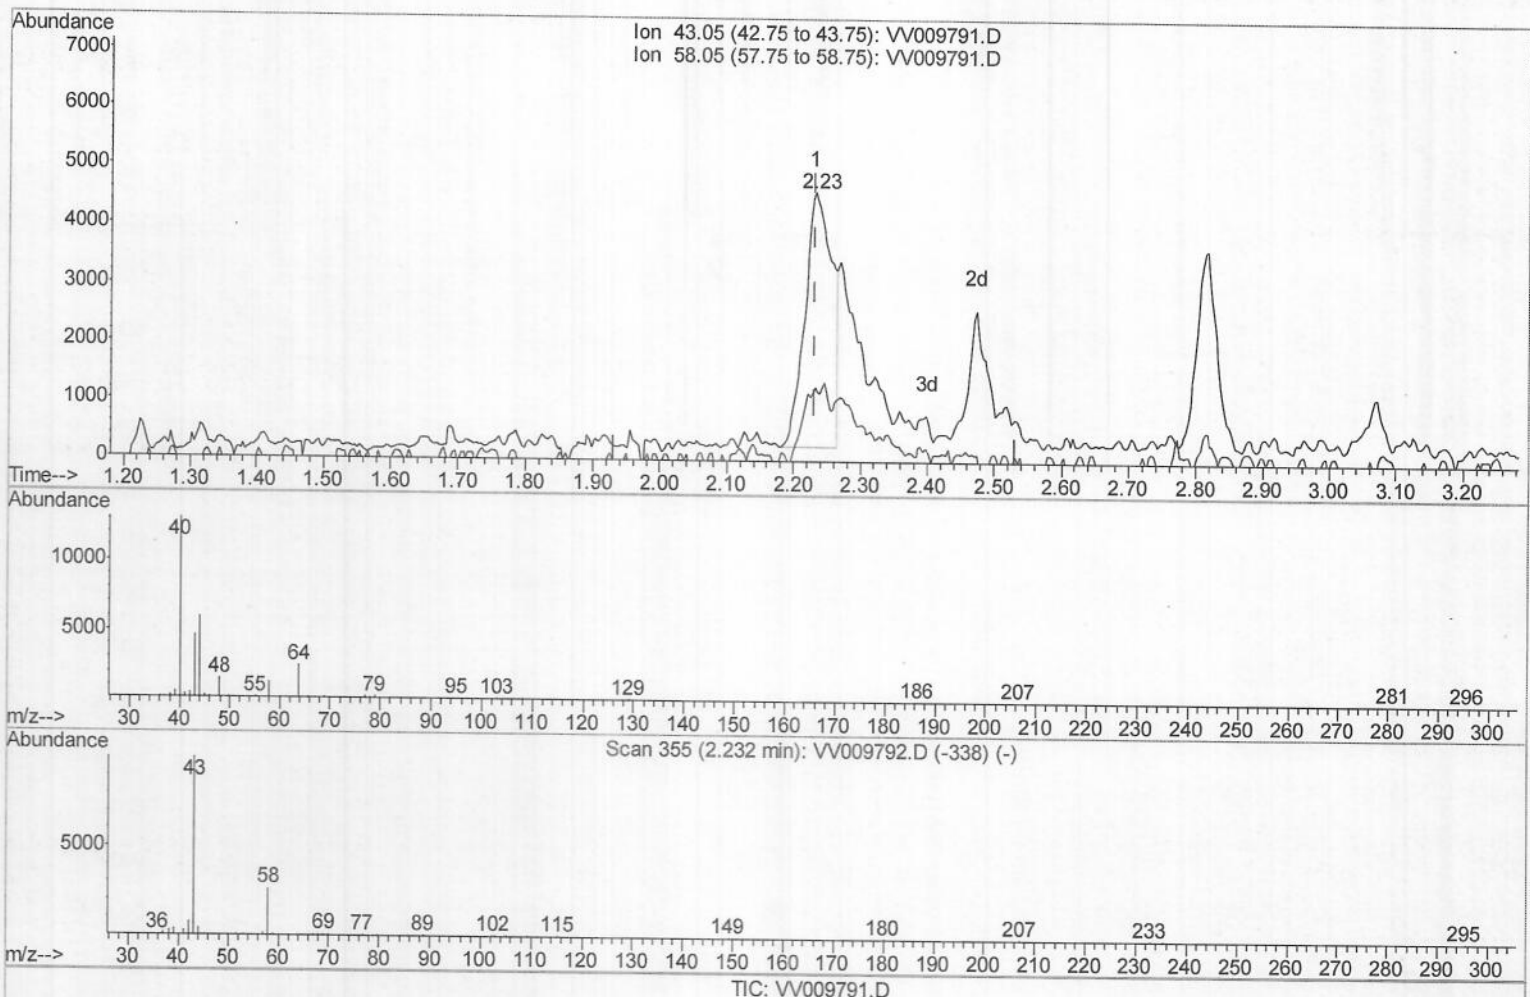
MMDadoda
3/22/2019 3:05:57 PM

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032119\
Data File : VV009791.D
Acq On : 21 Mar 2019 12:35
Operator : SY/MD
Sample : VSTD00132

Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 13:49:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 21 13:22:13 2019
Response via : Initial Calibration



(13) Acetone (T)

2.232min (-0.000) 10.61ug/L

response 12196

Ion	Exp%	Act%
43.05	100	100
58.05	11.50	17.79
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032119\
 Data File : VV009791.D
 Acq On : 21 Mar 2019 12:35
 Operator : SY/MD
 Sample : VSTD00132
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 14:04:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 21 13:22:13 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD00132

Manual Integrations
 APPROVED

MMDadoda
 3/22/2019 3:05:57 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
42) Toluene	7.43	91	33207	0.994	ug/L	97
44) trans-1,3-Dichloropropene	7.69	75	7463	0.845	ug/L	96
45) 1,1,2-Trichloroethane	7.89	97	5340	1.061	ug/L	91
47) Tetrachloroethene	8.02	164	7286	1.146	ug/L	85
48) 2-Hexanone	8.20	43	29152	10.918	ug/L #	96
49) Dibromochloromethane	8.29	129	5186	0.798	ug/L	82
50) 1,2-Dibromoethane	8.40	107	4950	1.010	ug/L #	96
51) Chlorobenzene	8.92	112	21056	0.954	ug/L	97
52) Ethylbenzene	9.05	91	35976	0.937	ug/L	100
53) m,p-xylene	9.18	106	13295	0.911	ug/L	89
54) o-xylene	9.59	106	12958	0.901	ug/L	87
55) Styrene	9.60	104	20567	0.883	ug/L	92
56) Isopropylbenzene	9.97	105	33186	0.851	ug/L	99
58) 1,1,2,2-Tetrachloroethane	10.29	83	6429	1.037	ug/L	90
59) 1,2,3-Trichloropropane	10.32	75	4700	1.078	ug/L	99
61) Bromoform	9.77	173	2493	0.790	ug/L #	53
62) 1,3-Dichlorobenzene	11.23	146	16309	0.997	ug/L	92
63) 1,4-Dichlorobenzene	11.32	146	16486	1.002	ug/L	95
65) 1,2-Dichlorobenzene	11.69	146	14417	0.947	ug/L	92
66) 1,2-Dibromo-3-chloropropane	12.48	75	850	0.873	ug/L #	60
67) 1,3,5-Trichlorobenzene	12.69	180	12807	1.058	ug/L	94
68) 1,2,4-trichlorobenzene	13.31	180	8157	0.857	ug/L	90
69) Naphthalene	13.56	128	11158	0.701	ug/L	97
70) 1,2,3-Trichlorobenzene	13.80	180	7857	0.914	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032119\

Data File : VV009791.D

Acq On : 21 Mar 2019 12:35

Operator : SY/MD

Sample : VSTD00132

Misc : 25.0mL/MSVOA V/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 21 14:04:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Mar 21 13:22:13 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampled :

VSTD00132

Manual Integrations

APPROVED

MMDadoda

3/22/2019 3:05:57 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	110214	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	107654	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	50857	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	15012	2.00	ug/L	0.00
7) Chloroethane-d5	1.58	69	12245	1.85	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.13	63	35120	1.90	ug/L	0.00
20) 2-Butanone-d5	3.98	46	14776m	11.25	ug/L	0.00
24) Chloroform-d	4.40	84	15141	1.16	ug/L	0.00
26) 1,2-Dichloroethane-d4	5.09	65	6573	1.02	ug/L	0.00
32) Benzene-d6	5.09	84	29432	1.12	ug/L	0.00
36) 1,2-Dichloropropane-d6	6.12	67	9218	1.18	ug/L	0.00
41) Toluene-d8	7.36	98	27183	1.03	ug/L	0.00
43) trans-1,3-Dichloropropene-	7.66	79	3205	0.96	ug/L	0.00
46) 2-Hexanone-d5	8.14	63	12269	10.99	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	10.26	84	6734	1.13	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	11.68	152	9271	1.02	ug/L	0.00

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.14	85	10322	1.497	ug/L	96
3) Chloromethane	1.25	50	15031	1.959	ug/L	97
5) Vinyl chloride	1.32	62	17239	2.033	ug/L	96
6) Bromomethane	1.53	94	9622	1.765	ug/L	92
8) Chloroethane	1.60	64	12751	2.236	ug/L	84
9) Trichlorofluoromethane	1.77	101	32641	1.776	ug/L	99
10) 1,1,2-Trichloro-1,2,2-trif	2.14	101	16982	1.834	ug/L	94
12) 1,1-Dichloroethene	2.14	96	14312	1.784	ug/L	97
13) Acetone	2.23	43	20515m	17.843	ug/L	
14) Carbon disulfide	2.32	76	41086	1.571	ug/L	98
15) Methyl Acetate	2.47	43	3967	1.262	ug/L #	85
16) Methylene chloride	2.53	84	19499	2.085	ug/L	98
17) Methyl tert-butyl Ether	2.81	73	34260	1.692	ug/L	100
18) trans-1,2-Dichloroethene	2.79	96	16812	1.914	ug/L	87
19) 1,1-Dichloroethane	3.23	63	29082	2.305	ug/L	97
21) 2-Butanone	4.08	43	15478	10.856	ug/L	73
22) cis-1,2-Dichloroethene	3.96	96	6982	0.892	ug/L	92
23) Bromochloromethane	4.30	128	2903	0.940	ug/L	82
25) Chloroform	4.43	83	13246m	0.993	ug/L	
27) 1,2-Dichloroethane	5.18	62	8058	1.000	ug/L	99
29) 1,1,1-Trichloroethane	4.66	97	12109	0.968	ug/L	99
30) Cyclohexane	4.71	56	11932	1.002	ug/L	93
31) Carbon tetrachloride	4.87	117	9974	0.980	ug/L	98
33) Benzene	5.15	78	30427	1.042	ug/L	100
34) Trichloroethene	5.96	95	7521	0.911	ug/L	93
35) Methylcyclohexane	6.17	83	13487	1.023	ug/L	97
37) 1,2-Dichloropropane	6.22	63	7783	1.095	ug/L #	90
38) Bromodichloromethane	6.56	83	8058	0.808	ug/L #	95
39) cis-1,3-Dichloropropene	7.07	75	9247	0.830	ug/L	96
40) 4-Methyl-2-pentanone	7.29	43	40955	10.591	ug/L	95

M.D
3/26/19M.D
3/26/19