

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032119\
 Data File : VV009809.D
 Acq On : 21 Mar 2019 21:16
 Operator : SY/MD
 Sample : K2049-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P015-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.119	5	9	13	rVB4	5054	4371	1.20%	0.126%
2	1.257	41	52	53	rBV3	7583	11568	3.18%	0.333%
3	1.319	62	71	87	rBV	106285	120918	33.26%	3.478%
4	1.585	147	154	162	rBV	84802	99529	27.37%	2.863%
5	2.132	315	324	336	rVB	214741	297050	81.70%	8.545%
6	3.981	882	899	921	rBV	36172	120218	33.06%	3.458%
7	4.402	1014	1030	1048	rBV2	63327	150896	41.50%	4.341%
8	5.096	1230	1246	1265	rBV3	154730	362434	99.68%	10.426%
9	5.666	1409	1423	1437	rBV	109647	217542	59.83%	6.258%
10	6.122	1547	1565	1587	rBV2	85469	178839	49.19%	5.145%
11	7.032	1836	1848	1860	rBV4	40254	74606	20.52%	2.146%
12	7.360	1935	1950	1965	rBV	178226	307245	84.50%	8.839%
13	7.666	2034	2045	2057	rBV3	23686	42665	11.73%	1.227%
14	7.984	2132	2144	2150	rBV3	25530	48915	13.45%	1.407%
15	8.145	2185	2194	2215	rVB2	187349	363591	100.00%	10.459%
16	8.897	2415	2428	2442	rBV2	179185	298067	81.98%	8.575%
17	10.264	2843	2853	2867	rBV2	62440	102340	28.15%	2.944%
18	10.450	2893	2911	2912	rBV8	46946	82715	22.75%	2.379%
19	10.678	2976	2982	2987	rBV3	2546	3707	1.02%	0.107%
20	11.296	3163	3174	3187	rBV	164919	269942	74.24%	7.765%
21	11.672	3277	3291	3309	rBV	171010	281347	77.38%	8.094%
22	12.305	3477	3488	3498	rBV	19645	33744	9.28%	0.971%
23	14.080	4033	4040	4045	rBV5	2981	3950	1.09%	0.114%


Sum of corrected areas: 3476199

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032119\
Data File : VV009809.D
Acq On : 21 Mar 2019 21:16
Operator : SY/MD
Sample : K2049-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P015-TW001-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

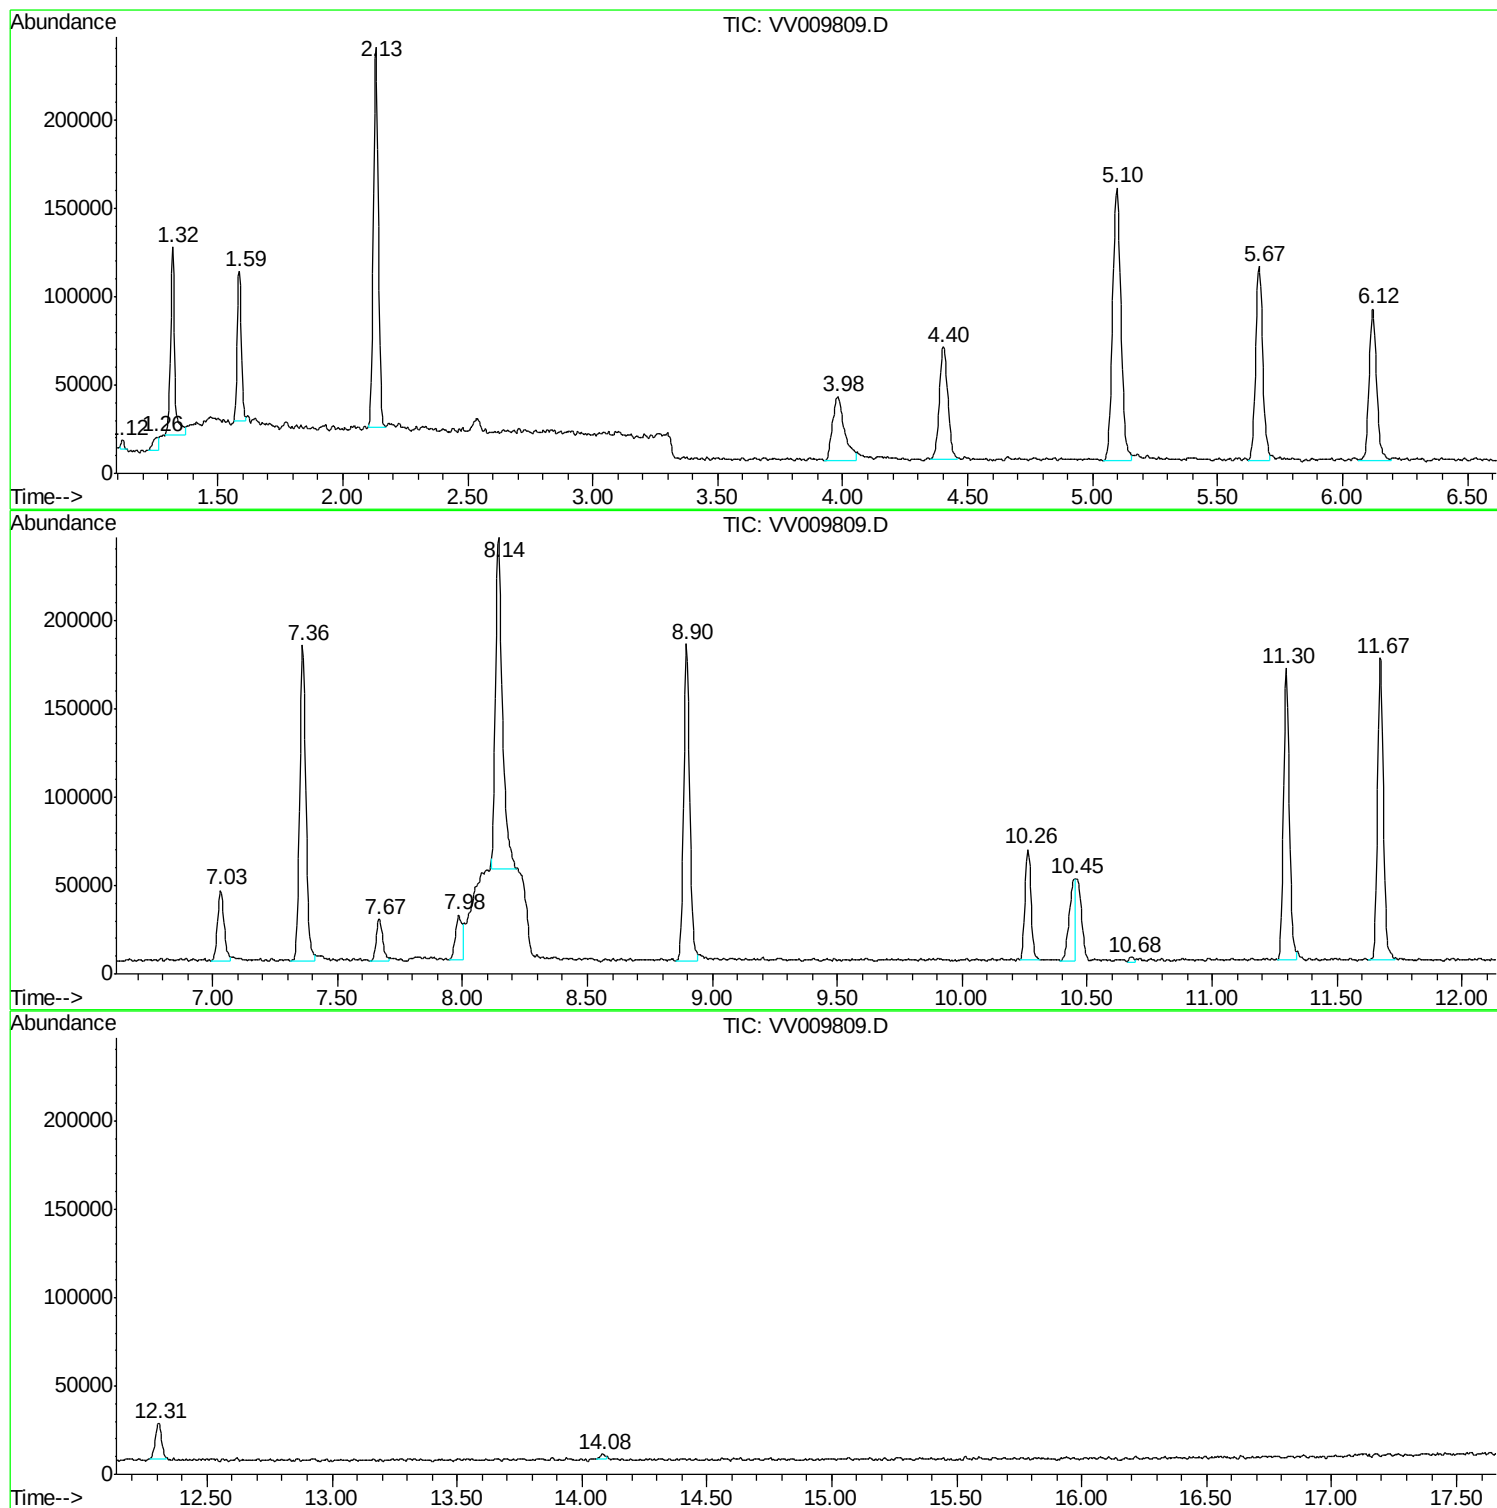

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032119\
Data File : VV009809.D
Acq On : 21 Mar 2019 21:16
Operator : SY/MD
Sample : K2049-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P015-TW001-01










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown-01 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.31	0.63 ug/L	33744	1,4-Dichlorobenzene-d4	11.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Benzoic acid, 2-[(trimethylsilyl)oxy]-, trimethyl...	282	C13H22O3Si2	003789-85-3	42
2		Benzoic acid, 2-[(trimethylsilyl)oxy]-, trimethyl...	282	C13H22O3Si2	003789-85-3	42
3		Benzeneethanamine, N-[(pentafluorophenyl)methyl]...	475	C21H26F5N02Si2	055429-85-1	38
4		Benzoic acid, 2-[(trimethylsilyl)oxy]-, trimethyl...	282	C13H22O3Si2	003789-85-3	36
5		11H-Dibenzo[b,e][1,4]diazepin-11-one	267	C16H17N3O	013450-73-2	27

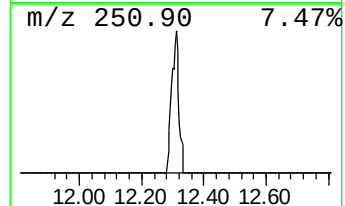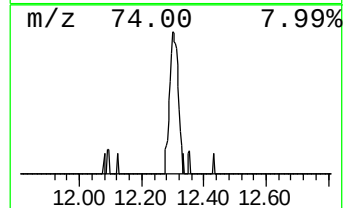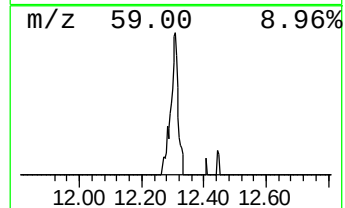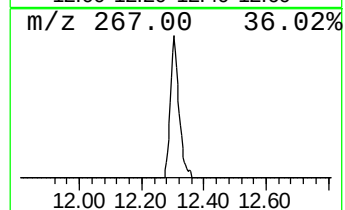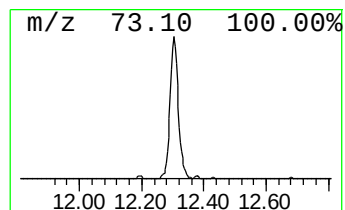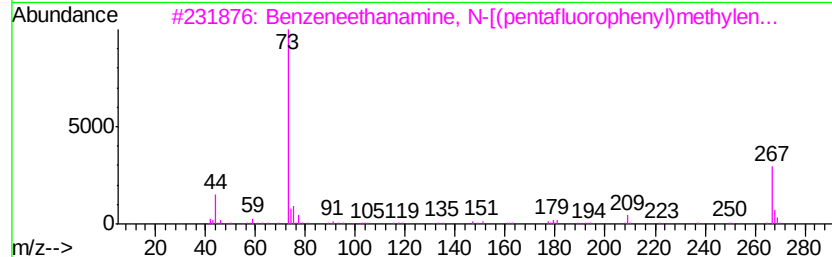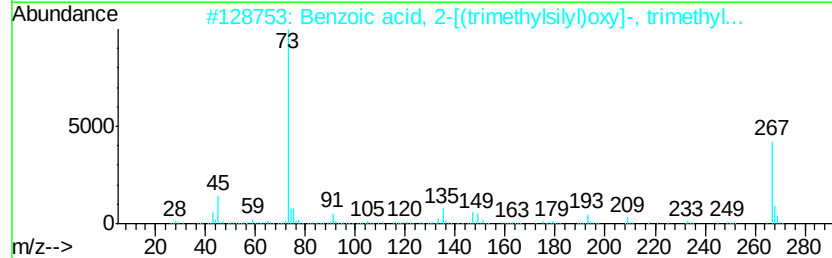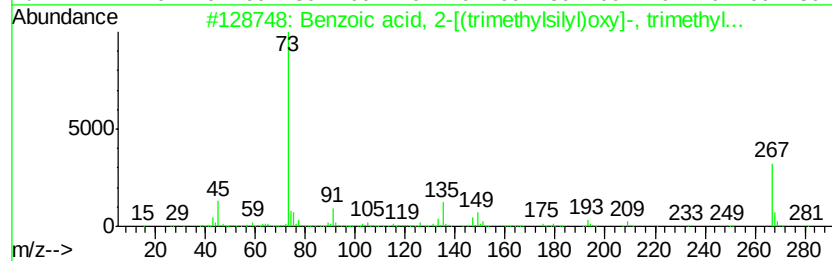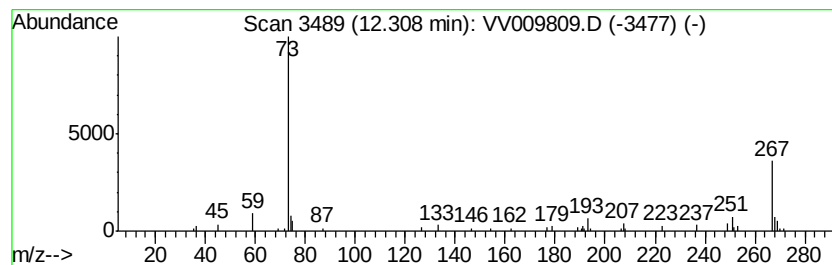

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032119\
Data File : VV009809.D
Acq On : 21 Mar 2019 21:16
Operator : SY/MD
Sample : K2049-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P015-TW001-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.31	0.6	ug/L	33744	3	11.30	269942	5.0