


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032119\
 Data File : VV009789.D
 Acq On : 21 Mar 2019 10:29
 Operator : SY/MD
 Sample : BFB31
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 23 21:59:27 2019

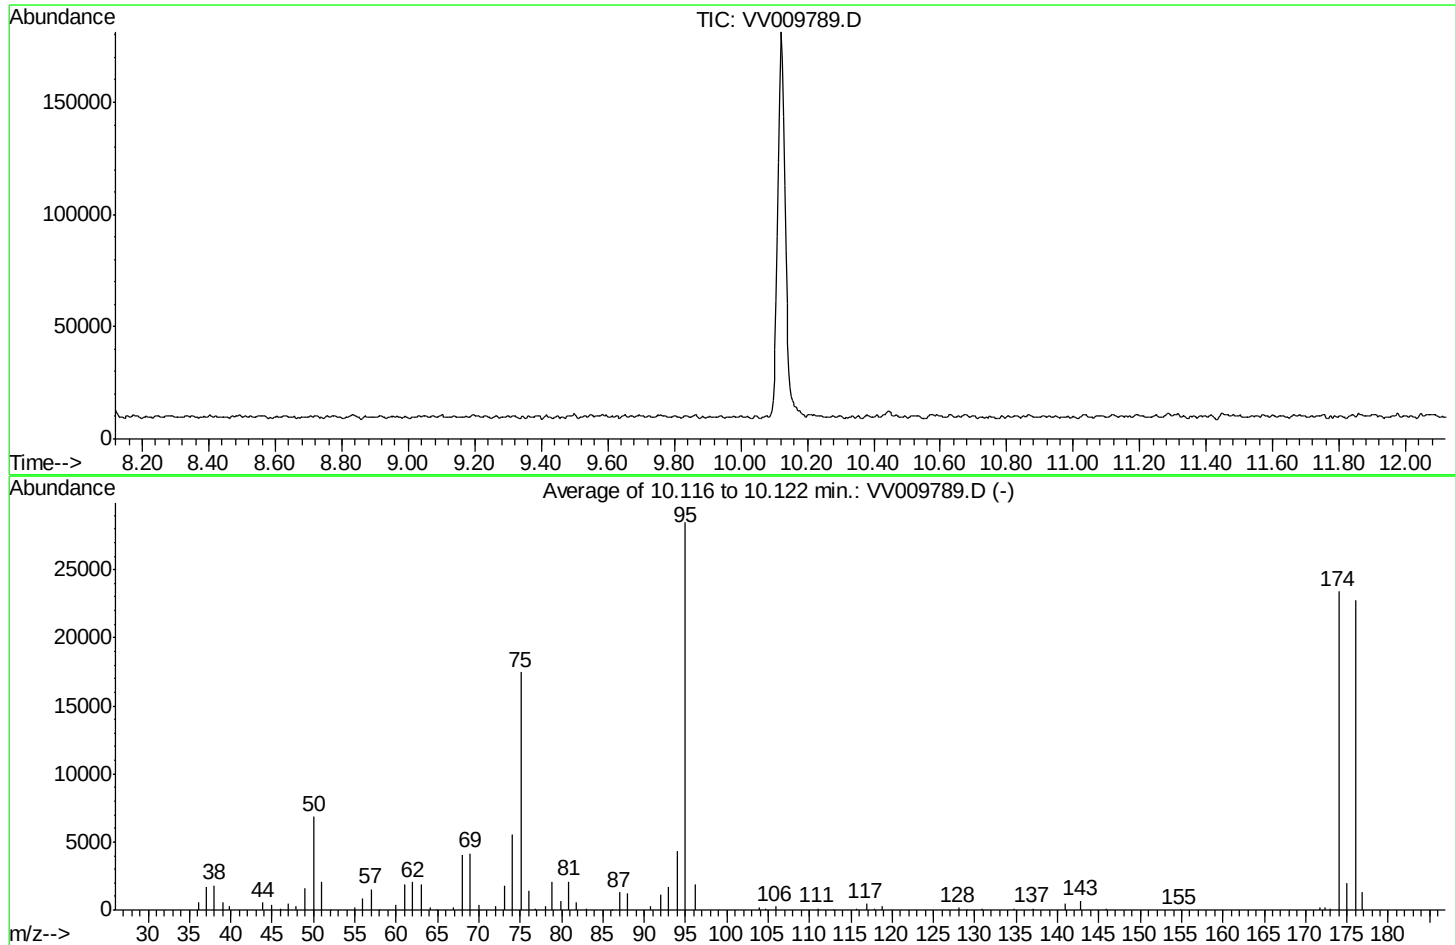

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	6830	PASS
75	95	30	80	61.3	17468	PASS
95	95	100	100	100.0	28485	PASS
96	95	5	9	6.8	1930	PASS
173	174	0.00	2	0.5	114	PASS
174	95	50	120	82.1	23394	PASS
175	174	5	9	8.4	1962	PASS
176	174	95	101	97.4	22789	PASS
177	176	5	9	5.8	1332	PASS

m/z	Abundance
36.10	513.0
37.00	1653.0
38.00	1883.0
39.00	518.0
39.90	9796.0
43.90	748.0
45.00	411.0
46.00	134.0
47.00	326.0
47.90	269.0
49.00	1512.0
50.00	6418.0
51.00	1942.0
52.00	113.0
55.00	190.0
56.00	671.0
56.90	1408.0
57.90	129.0
60.00	292.0
61.10	1739.0
62.00	2013.0
63.00	1655.0
64.10	159.0
66.90	130.0
68.00	3724.0
69.00	3909.0
70.00	307.0
72.10	249.0
73.10	1417.0
74.00	4928.0
75.10	15710.0
76.10	1380.0
76.90	161.0
78.10	229.0
78.90	1844.0
79.90	613.0
80.90	1918.0
81.90	615.0
87.00	1366.0
87.80	979.0
90.80	264.0
92.00	1017.0
93.00	1625.0
94.00	4008.0
95.00	25992.0
96.10	1714.0
103.80	142.0
104.80	102.0
105.80	207.0
111.00	104.0
115.70	135.0
116.90	381.0
118.80	213.0
128.10	109.0
129.00	122.0
134.70	131.0
137.00	111.0
141.00	327.0
142.80	619.0
145.90	143.0
171.80	149.0
172.40	217.0
174.00	20528.0
174.90	1719.0
176.00	19576.0
176.90	1185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	515.0
37.00	1812.0
38.00	1883.0
39.10	553.0
39.90	9924.0
43.90	752.0
45.00	356.0
46.00	100.0
46.90	453.0
47.80	306.0
49.00	1735.0
50.00	7047.0
51.00	2166.0
52.10	116.0
55.00	222.0
56.00	870.0
56.90	1616.0
59.90	370.0
61.10	1976.0
62.00	2139.0
63.00	2051.0
64.20	221.0
66.90	152.0
68.00	4161.0
69.00	4380.0
70.10	378.0
72.00	268.0
73.00	1877.0
74.00	5645.0
75.10	18032.0
76.10	1509.0
76.90	131.0
78.10	296.0
78.90	2126.0
79.90	656.0
80.90	2118.0
81.80	615.0
83.00	121.0
87.00	1266.0
87.90	1270.0
90.80	294.0
92.00	1214.0
93.00	1732.0
94.00	4469.0
95.00	29776.0
96.10	2022.0
103.90	200.0
104.70	149.0
105.90	226.0
111.00	131.0
112.90	114.0
115.60	128.0
116.90	501.0
117.90	121.0
118.80	276.0
128.00	179.0
130.80	147.0
134.70	102.0
137.00	117.0
140.90	453.0
142.90	688.0
145.90	147.0
154.80	103.0
171.70	183.0
172.40	218.0
173.00	342.0
174.00	24184.0
174.90	2044.0
176.00	23432.0
176.90	1385.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	544.0
37.00	1915.0
38.00	1712.0
39.10	625.0
39.90	9667.0
43.90	704.0
44.90	274.0
46.90	606.0
47.80	331.0
49.00	1688.0
50.10	7025.0
51.00	2118.0
52.10	115.0
55.10	243.0
56.00	976.0
57.00	1574.0
59.90	439.0
61.00	2004.0
62.00	2010.0
63.00	2047.0
64.10	285.0
64.90	134.0
66.80	169.0
68.00	4137.0
69.00	4201.0
70.10	382.0
72.00	228.0
73.00	2031.0
74.00	6155.0
75.10	18664.0
76.10	1488.0
78.10	287.0
78.90	2193.0
79.90	643.0
80.90	2309.0
81.80	586.0
83.00	107.0
86.10	114.0
87.00	1290.0
88.00	1355.0
90.80	256.0
92.10	1259.0
92.90	1842.0
94.00	4450.0
95.00	29688.0
96.10	2054.0
103.90	241.0
104.70	160.0
106.00	325.0
111.00	104.0
115.60	134.0
116.90	501.0
117.80	171.0
118.80	319.0
128.00	249.0
130.80	160.0
137.00	128.0
140.90	518.0
142.90	676.0
145.90	108.0
171.70	258.0
174.00	25472.0
175.00	2125.0
176.00	25360.0
176.90	1428.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

Scan 2794 (10.074 min): VV009789.D
BFB31

m/z	Abundance
35.20	105.0
37.20	125.0
40.00	9478.0
43.90	205.0
52.20	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31