

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030273.D
 Acq On : 21 Mar 2023 13:22
 Operator : SY/MD
 Sample : VV0321WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK316

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	64	rBV5	3804	4829	1.26%	0.148%
2	1.281	68	75	88	rVB	53984	59991	15.72%	1.842%
3	1.535	146	154	168	rVB	54100	63819	16.72%	1.960%
4	2.063	308	318	332	rBV	104359	153575	40.23%	4.716%
5	2.458	430	441	453	rBV2	11583	21043	5.51%	0.646%
6	3.847	860	873	880	rBV2	19120	50877	13.33%	1.562%
7	4.262	985	1002	1026	rBV2	68219	178946	46.88%	5.496%
8	4.966	1204	1221	1248	rBV2	149357	381742	100.00%	11.724%
9	5.542	1388	1400	1423	rBV	140536	293683	76.93%	9.019%
10	5.998	1529	1542	1568	rBV	87905	187853	49.21%	5.769%
11	6.924	1818	1830	1857	rBV2	39152	78247	20.50%	2.403%
12	7.252	1920	1932	1955	rBV	172403	314347	82.35%	9.654%
13	7.564	2019	2029	2049	rBV	24400	46361	12.14%	1.424%
14	8.040	2167	2177	2211	rBV	142446	318243	83.37%	9.773%
15	8.374	2272	2281	2292	rBV6	2776	5339	1.40%	0.164%
16	8.792	2394	2411	2434	rBV	210040	359511	94.18%	11.041%
17	10.162	2827	2837	2850	rBV	66394	105405	27.61%	3.237%
18	11.194	3147	3158	3178	rBV	221851	344274	90.18%	10.573%
19	11.570	3263	3275	3293	rBV	179544	288110	75.47%	8.848%




Sum of corrected areas: 3256195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030273.D
Acq On : 21 Mar 2023 13:22
Operator : SY/MD
Sample : VV0321WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

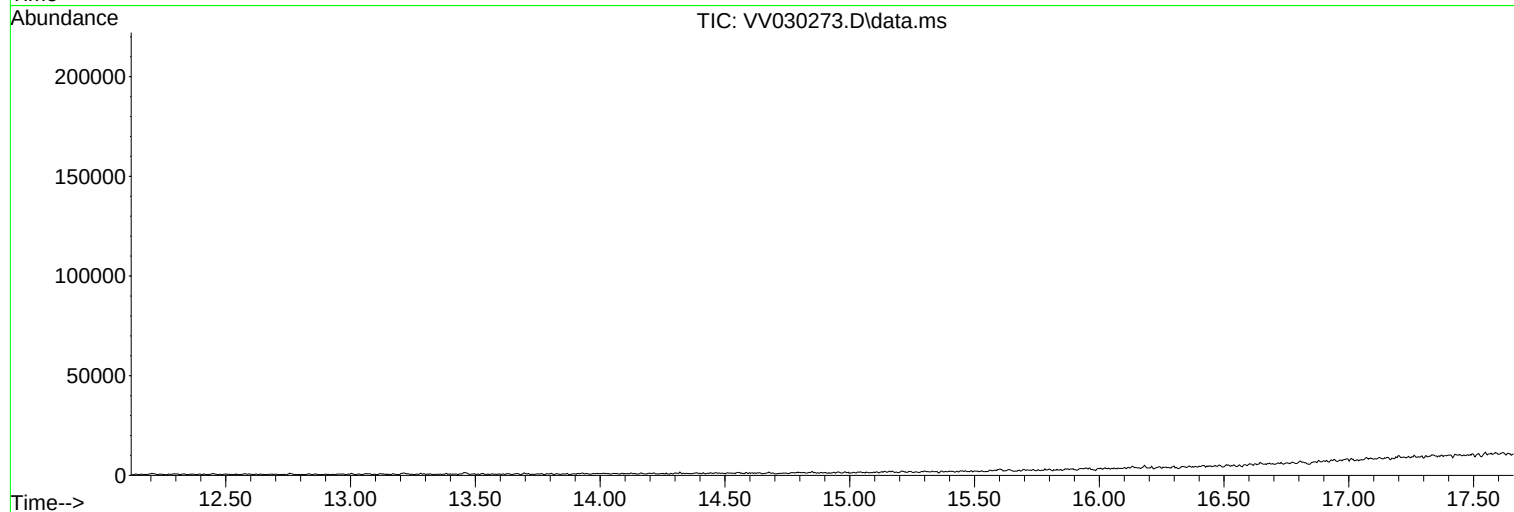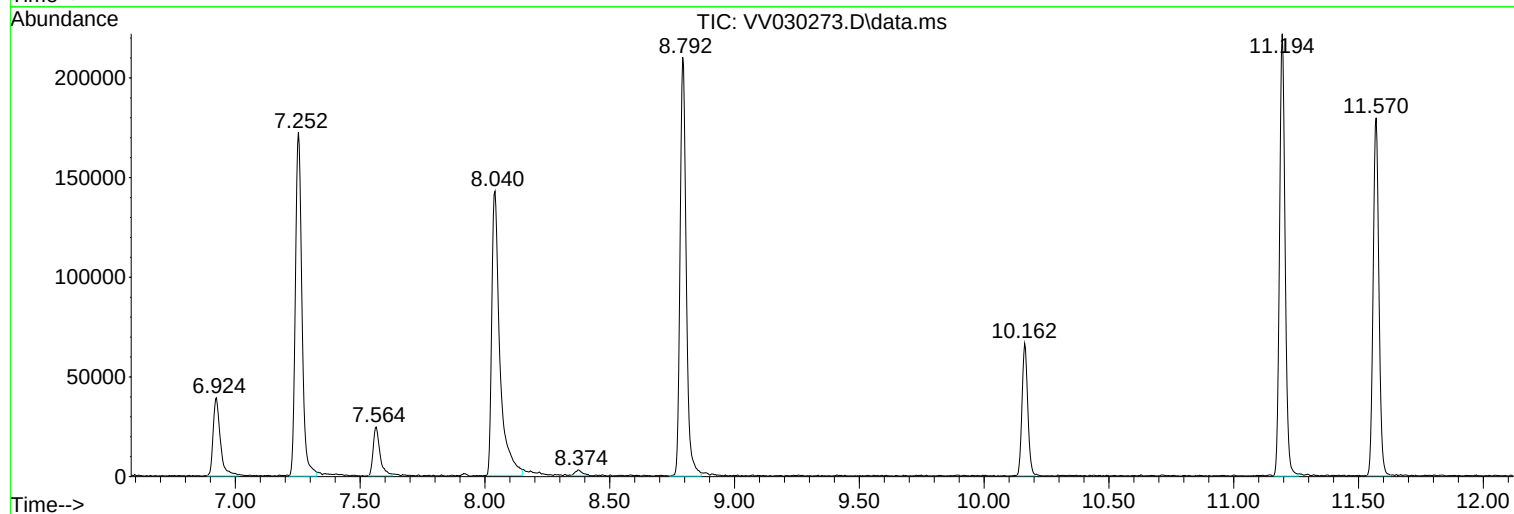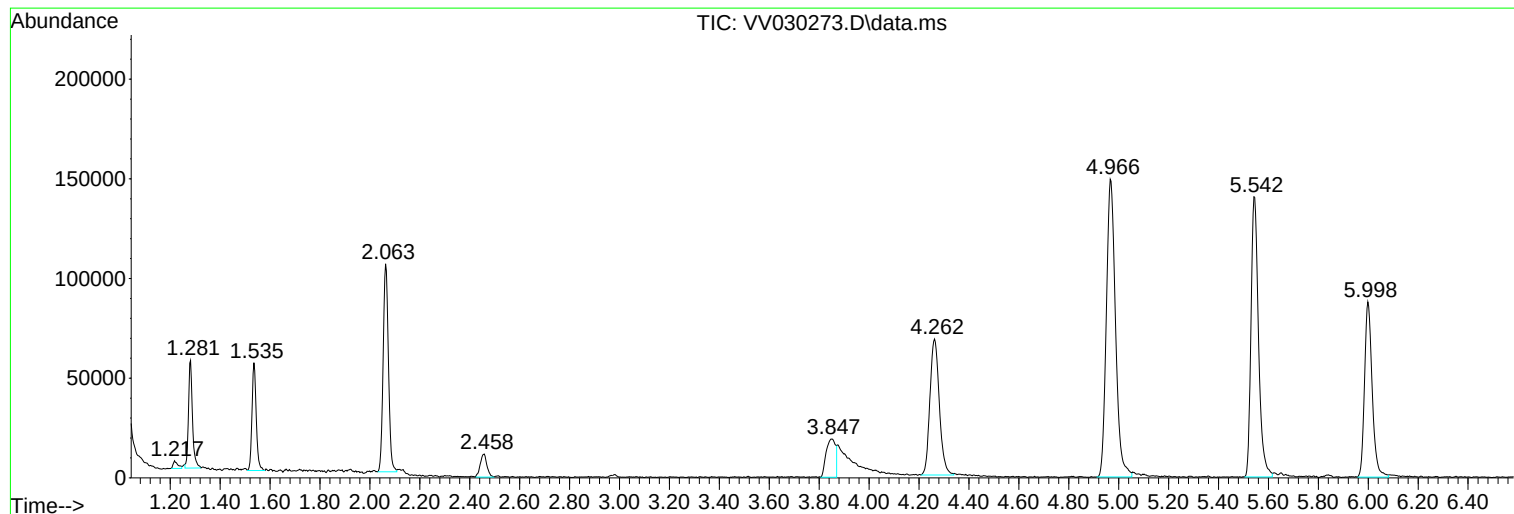

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030273.D
Acq On : 21 Mar 2023 13:22
Operator : SY/MD
Sample : VV0321WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030273.D
Acq On : 21 Mar 2023 13:22
Operator : SY/MD
Sample : VV0321WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc