

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030274.D
 Acq On : 21 Mar 2023 13:46
 Operator : SY/MD
 Sample : 01996-08DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A29DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	46303	52768	13.61%	1.474%
2	1.536	146	154	166	rVB	47413	55498	14.31%	1.551%
3	2.063	306	318	330	rBV2	100611	155465	40.09%	4.344%
4	2.455	428	440	450	rBV2	9250	15561	4.01%	0.435%
5	3.841	859	871	873	rBV	20942	33671	8.68%	0.941%
6	4.259	981	1001	1029	rBV2	68527	177154	45.68%	4.950%
7	4.966	1201	1221	1248	rBV3	140450	362296	93.43%	10.123%
8	5.545	1387	1401	1425	rBV	136106	289714	74.71%	8.095%
9	5.847	1483	1495	1511	rBV4	19653	41664	10.74%	1.164%
10	5.998	1527	1542	1564	rBV	82855	178127	45.94%	4.977%
11	6.921	1818	1829	1848	rBV	40187	76569	19.75%	2.139%
12	7.252	1920	1932	1953	rBV	163804	293331	75.64%	8.196%
13	7.564	2019	2029	2050	rBV2	24230	45787	11.81%	1.279%
14	7.915	2126	2138	2159	rBV	225672	387779	100.00%	10.835%
15	8.040	2166	2177	2210	rBV	145760	319592	82.42%	8.929%
16	8.793	2399	2411	2429	rBV	208924	353887	91.26%	9.888%
17	10.162	2825	2837	2856	rVB	66457	105732	27.27%	2.954%
18	11.194	3145	3158	3176	rBV	223054	350028	90.26%	9.780%
19	11.571	3262	3275	3291	rBV	179393	284481	73.36%	7.948%




Sum of corrected areas: 3579104

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030274.D
Acq On : 21 Mar 2023 13:46
Operator : SY/MD
Sample : 01996-08DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

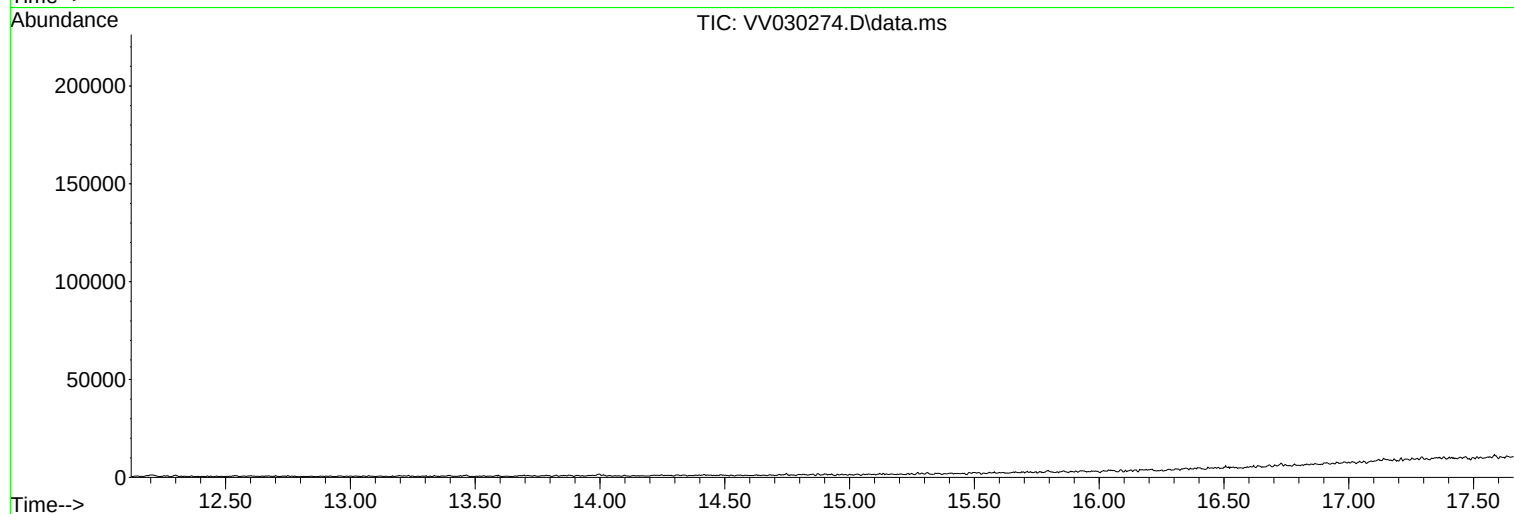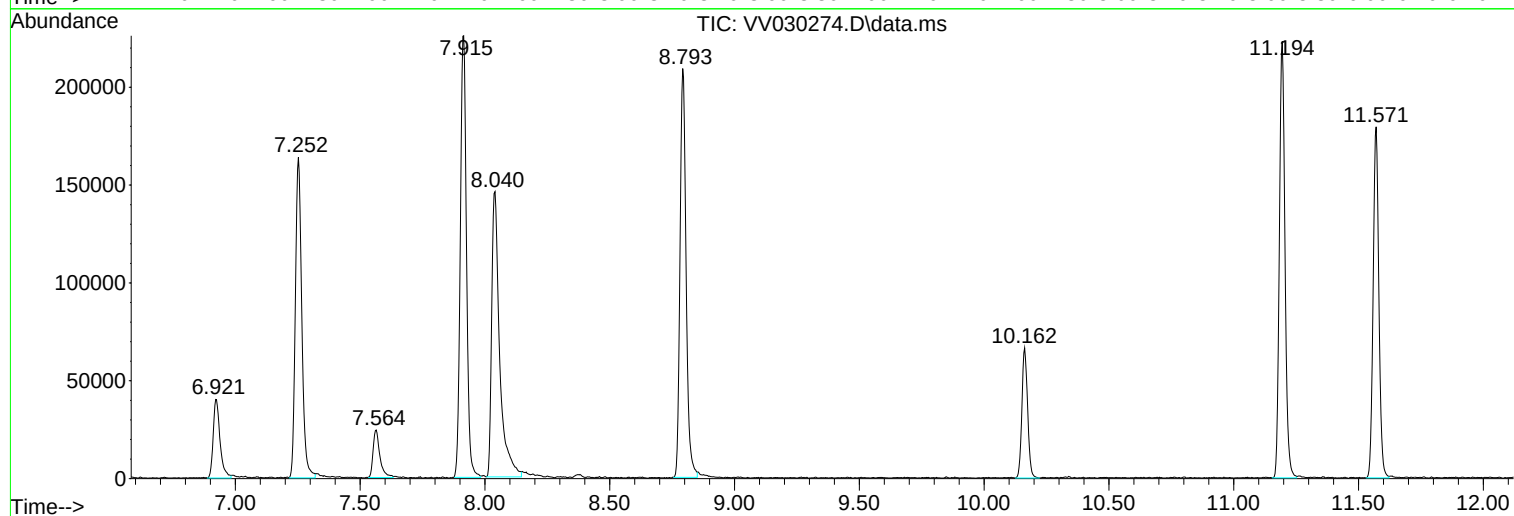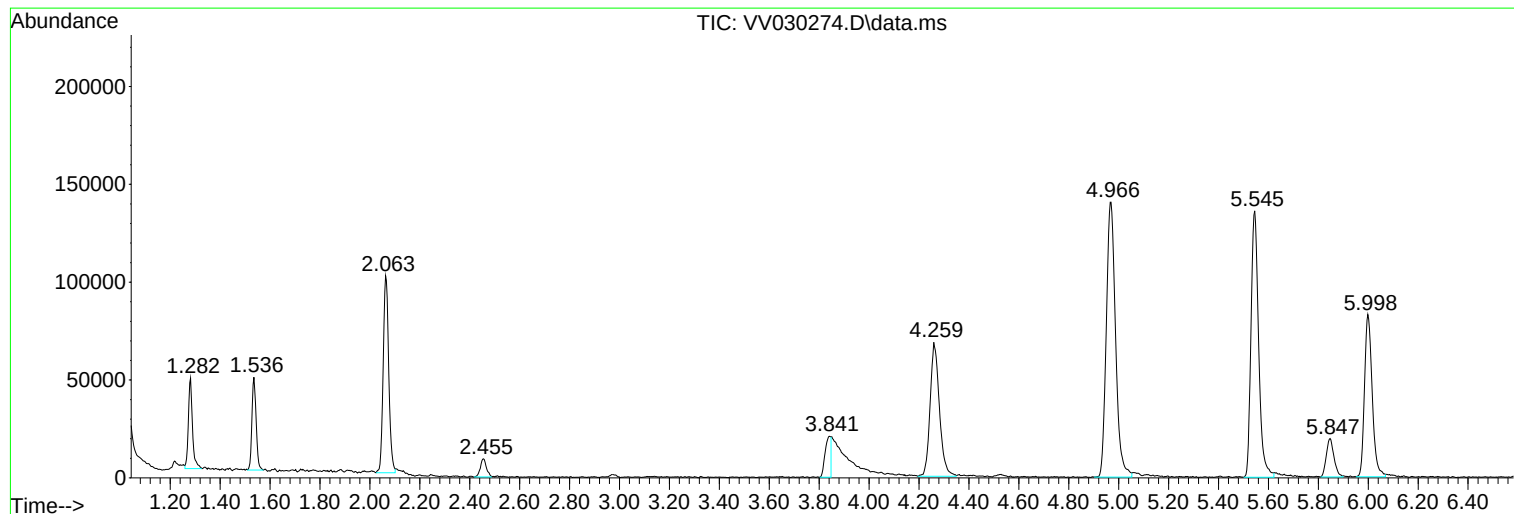

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030274.D
Acq On : 21 Mar 2023 13:46
Operator : SY/MD
Sample : 01996-08DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030274.D
Acq On : 21 Mar 2023 13:46
Operator : SY/MD
Sample : 01996-08DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc