

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030275.D
 Acq On : 21 Mar 2023 14:10
 Operator : SY/MD
 Sample : 01996-01DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A24DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	63628	72868	11.41%	1.755%
2	1.536	146	154	167	rVB	64765	75296	11.79%	1.813%
3	2.063	307	318	332	rBV	134170	199517	31.23%	4.805%
4	2.452	430	439	450	rBV4	4012	6951	1.09%	0.167%
5	3.844	857	872	897	rBV3	22559	100512	15.73%	2.420%
6	4.262	984	1002	1028	rBV2	74524	196562	30.77%	4.733%
7	4.523	1066	1083	1099	rVB3	9853	25564	4.00%	0.616%
8	4.966	1205	1221	1241	rBV2	164485	415646	65.06%	10.009%
9	5.542	1387	1400	1421	rBV2	133425	282277	44.18%	6.798%
10	5.844	1478	1494	1509	rBV4	14584	31278	4.90%	0.753%
11	5.998	1528	1542	1565	rBV2	94599	202812	31.75%	4.884%
12	6.924	1818	1830	1850	rBV	41870	82901	12.98%	1.996%
13	7.252	1915	1932	1956	rBV	194423	352203	55.13%	8.482%
14	7.561	2017	2028	2050	rBV2	26402	51182	8.01%	1.233%
15	7.911	2125	2137	2156	rBV	369586	638877	100.00%	15.385%
16	8.037	2166	2176	2211	rBV	147936	319948	50.08%	7.705%
17	8.792	2400	2411	2436	rBV	206074	350266	54.83%	8.435%
18	10.162	2826	2837	2856	rVB	65638	108415	16.97%	2.611%
19	11.194	3146	3158	3175	rBV	209482	331277	51.85%	7.978%
20	11.570	3263	3275	3297	rBV	192878	308234	48.25%	7.423%




Sum of corrected areas: 4152586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030275.D
Acq On : 21 Mar 2023 14:10
Operator : SY/MD
Sample : 01996-01DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

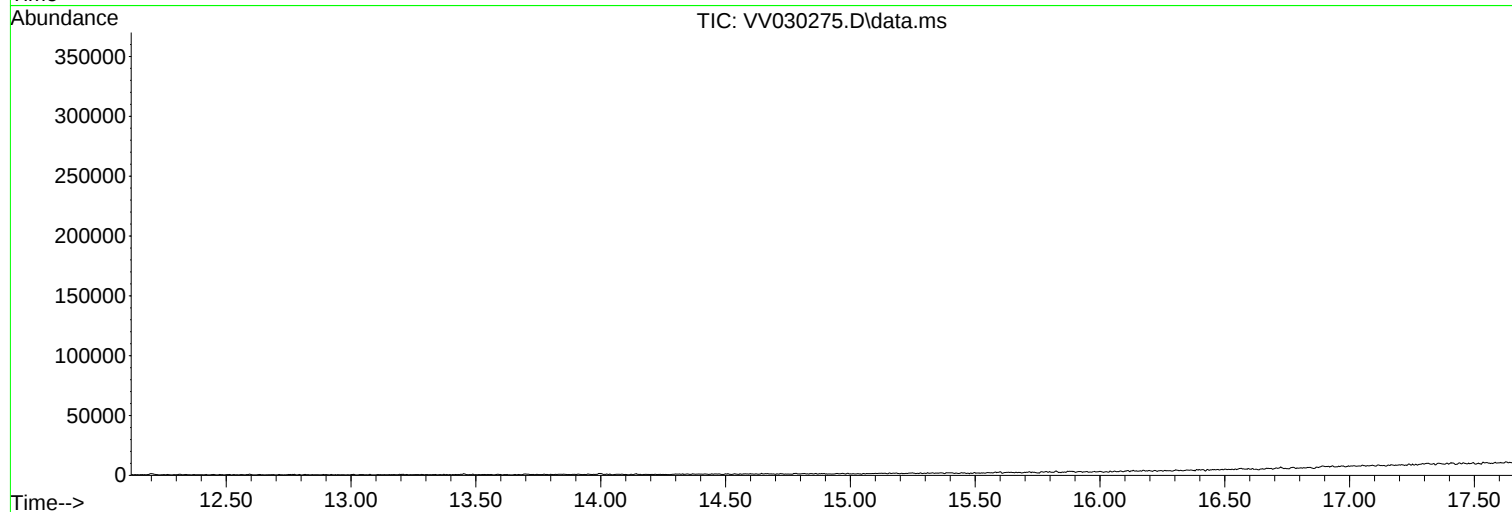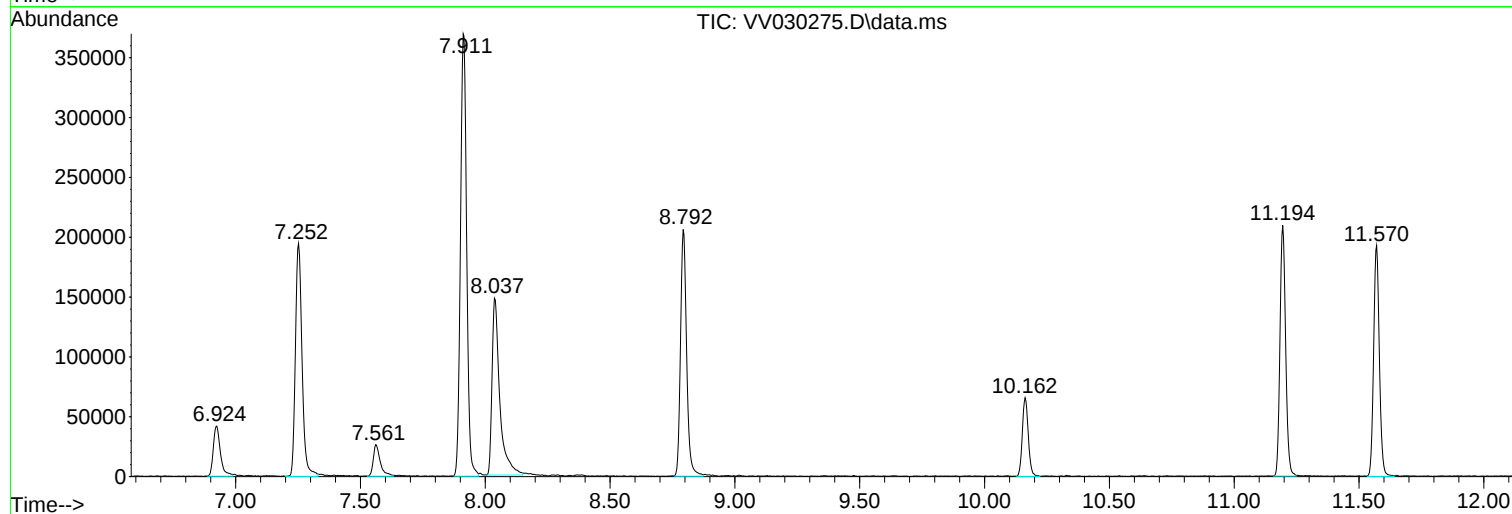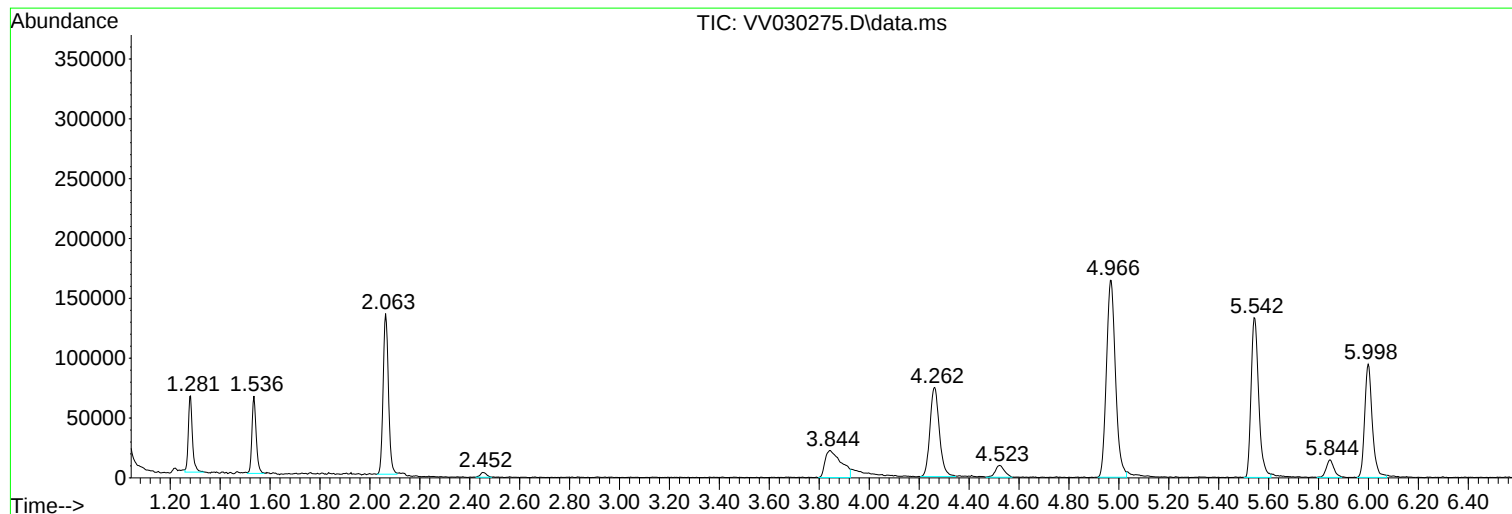

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030275.D
Acq On : 21 Mar 2023 14:10
Operator : SY/MD
Sample : 01996-01DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030275.D
Acq On : 21 Mar 2023 14:10
Operator : SY/MD
Sample : 01996-01DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------