

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030276.D
 Acq On : 21 Mar 2023 14:35
 Operator : SY/MD
 Sample : 01996-07DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A28DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rVB	43645	48155	4.87%	1.137%
2	1.536	147	154	166	rVB	46259	53200	5.38%	1.257%
3	2.063	308	318	335	rVB3	112855	179354	18.14%	4.236%
4	2.455	431	440	451	rBV3	6450	11347	1.15%	0.268%
5	3.847	857	873	884	rBV2	20646	70206	7.10%	1.658%
6	4.262	984	1002	1025	rBV	65980	170565	17.25%	4.029%
7	4.970	1201	1222	1242	rBV3	134416	347960	35.19%	8.218%
8	5.542	1388	1400	1421	rBV2	136523	287600	29.09%	6.793%
9	5.844	1480	1494	1513	rBV3	56044	117045	11.84%	2.764%
10	5.998	1526	1542	1562	rBV2	81379	172826	17.48%	4.082%
11	6.921	1817	1829	1846	rBV2	36989	71949	7.28%	1.699%
12	7.252	1917	1932	1953	rBV	157253	280565	28.38%	6.627%
13	7.564	2019	2029	2046	rBV2	22580	42080	4.26%	0.994%
14	7.912	2123	2137	2165	rBV	577610	988695	100.00%	23.352%
15	8.037	2165	2176	2203	rBV	148356	313814	31.74%	7.412%
16	8.793	2399	2411	2438	rBV	209152	355828	35.99%	8.404%
17	10.162	2826	2837	2849	rBV	65610	104032	10.52%	2.457%
18	11.194	3146	3158	3179	rBV	221149	344458	34.84%	8.136%
19	11.571	3263	3275	3293	rBV	174021	274263	27.74%	6.478%




Sum of corrected areas: 4233942

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030276.D
Acq On : 21 Mar 2023 14:35
Operator : SY/MD
Sample : 01996-07DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

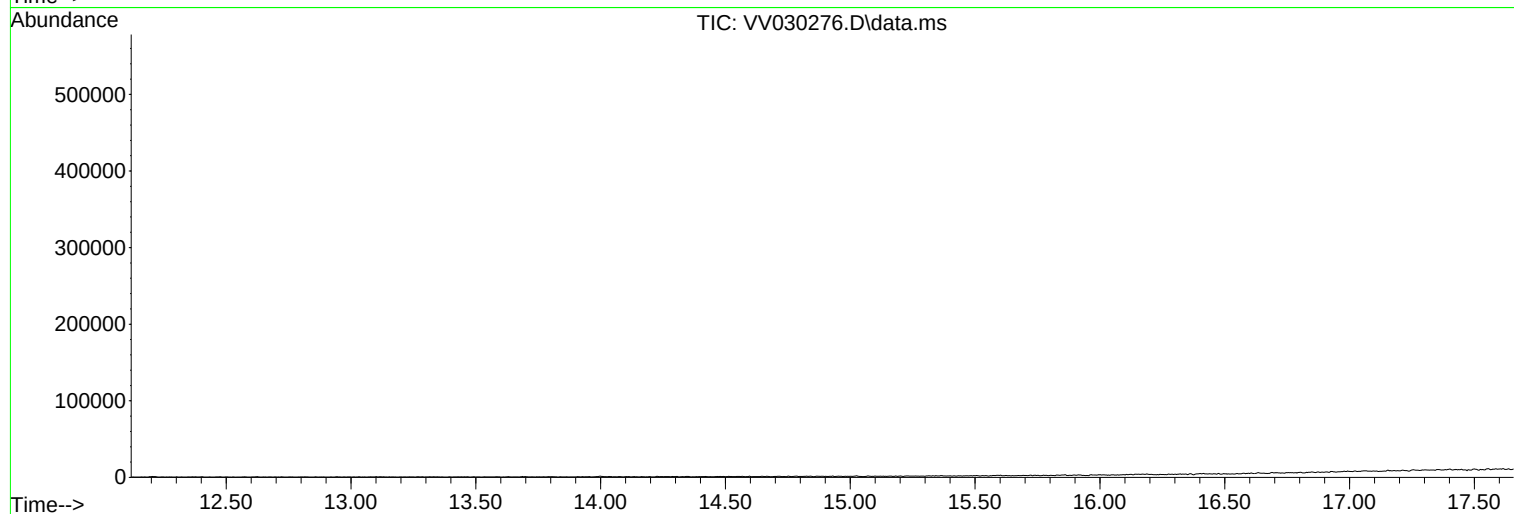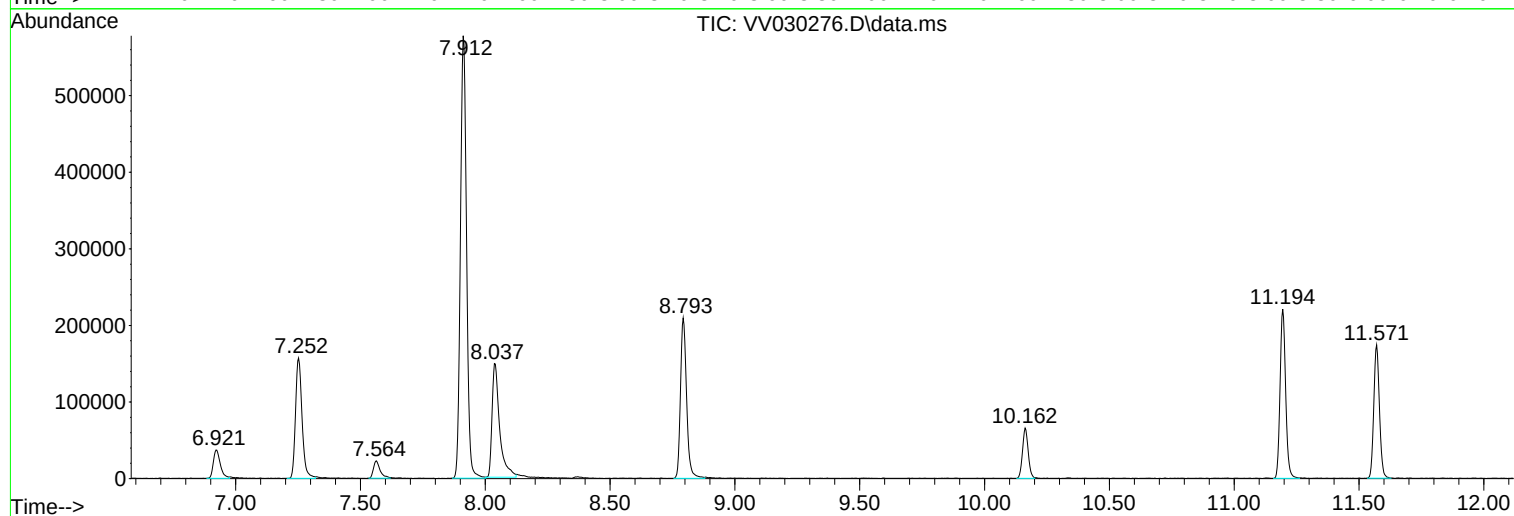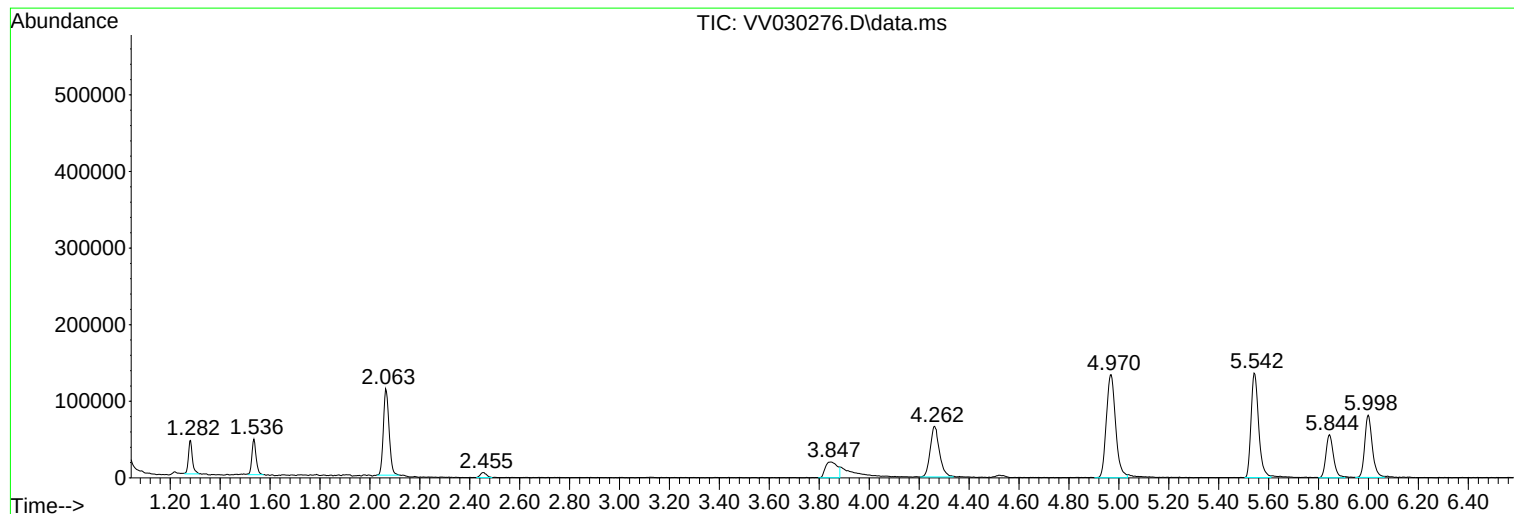

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030276.D
Acq On : 21 Mar 2023 14:35
Operator : SY/MD
Sample : 01996-07DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030276.D
Acq On : 21 Mar 2023 14:35
Operator : SY/MD
Sample : 01996-07DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------