

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030277.D
 Acq On : 21 Mar 2023 14:59
 Operator : SY/MD
 Sample : 01996-09DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A30DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	41706	46178	5.37%	1.128%
2	1.536	147	154	165	rVB	47527	54650	6.35%	1.335%
3	2.063	308	318	334	rBV2	104905	165034	19.19%	4.032%
4	2.452	432	439	453	rVB3	6776	11382	1.32%	0.278%
5	3.838	858	870	897	rBV2	21812	100879	11.73%	2.465%
6	4.259	984	1001	1029	rBV	64519	171816	19.97%	4.198%
7	4.523	1069	1083	1099	rBV7	4274	11000	1.28%	0.269%
8	4.966	1202	1221	1248	rBV2	134232	347218	40.36%	8.483%
9	5.542	1385	1400	1421	rBV	135934	285486	33.19%	6.975%
10	5.844	1482	1494	1516	rBV2	39836	84497	9.82%	2.064%
11	5.998	1528	1542	1564	rBV3	80661	172520	20.06%	4.215%
12	6.921	1816	1829	1847	rBV	36607	71700	8.34%	1.752%
13	7.252	1919	1932	1950	rBV	154499	279949	32.54%	6.839%
14	7.564	2017	2029	2042	rBV2	22969	42966	4.99%	1.050%
15	7.912	2124	2137	2157	rBV	502807	860217	100.00%	21.016%
16	8.037	2163	2176	2210	rBV	149927	317288	36.88%	7.752%
17	8.793	2398	2411	2431	rBV	210336	351908	40.91%	8.597%
18	10.162	2826	2837	2853	rBV	64105	102877	11.96%	2.513%
19	11.194	3145	3158	3175	rBV	217039	339781	39.50%	8.301%
20	11.571	3261	3275	3292	rBV	173526	275879	32.07%	6.740%




Sum of corrected areas: 4093225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030277.D
Acq On : 21 Mar 2023 14:59
Operator : SY/MD
Sample : 01996-09DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

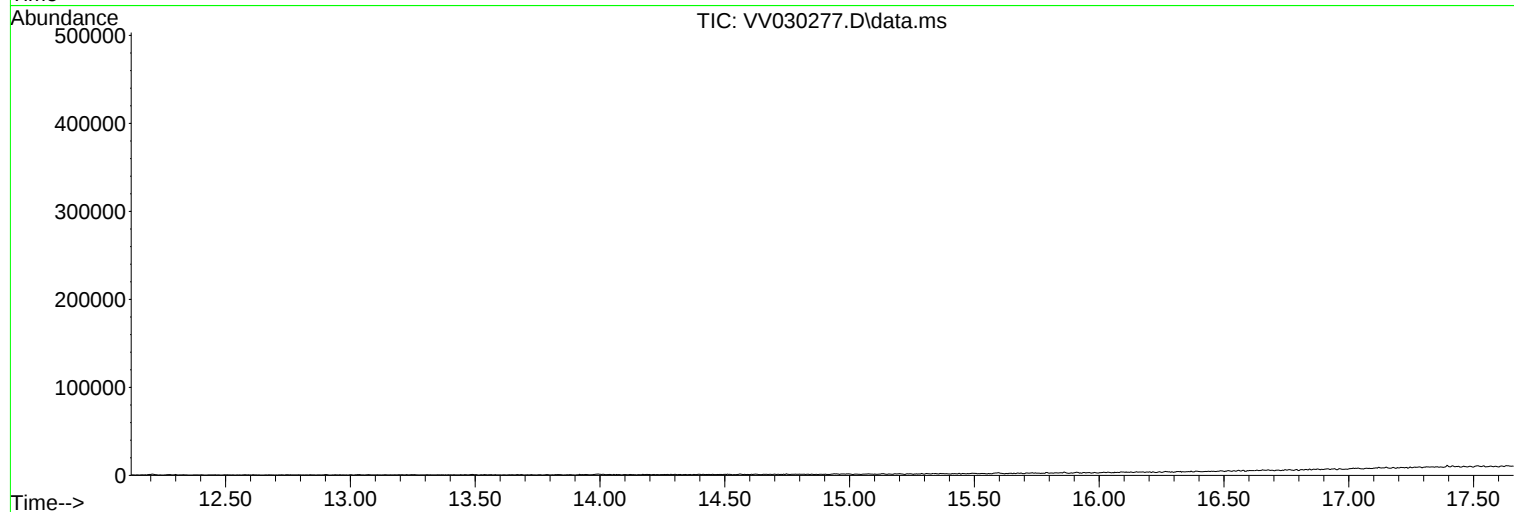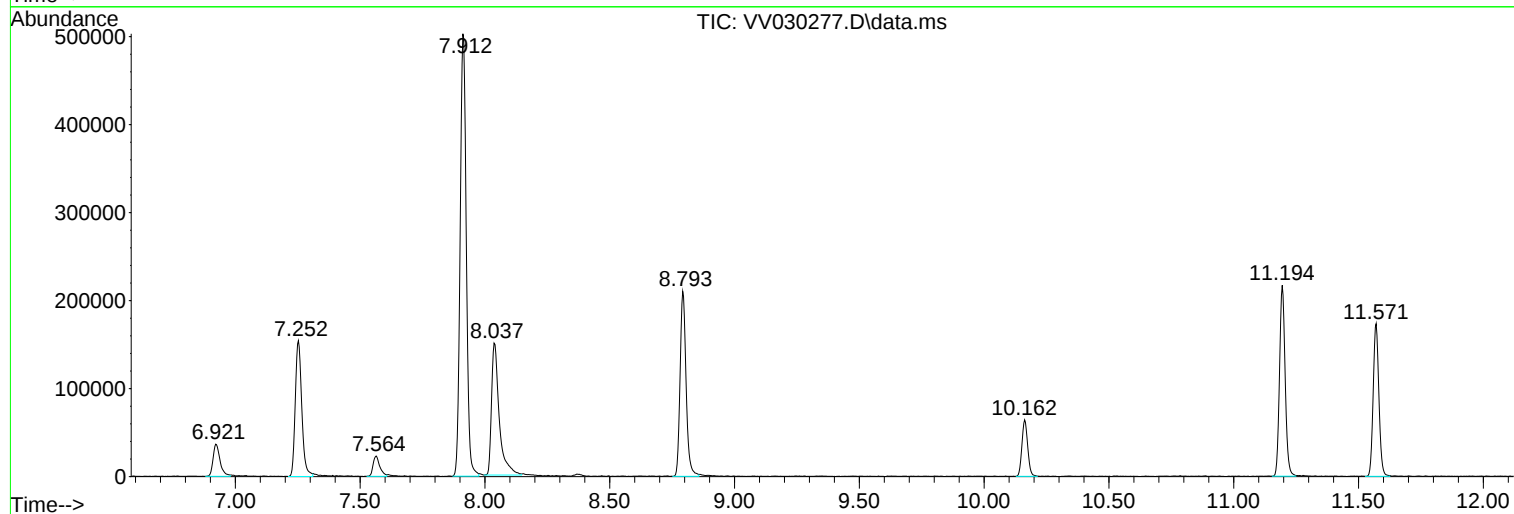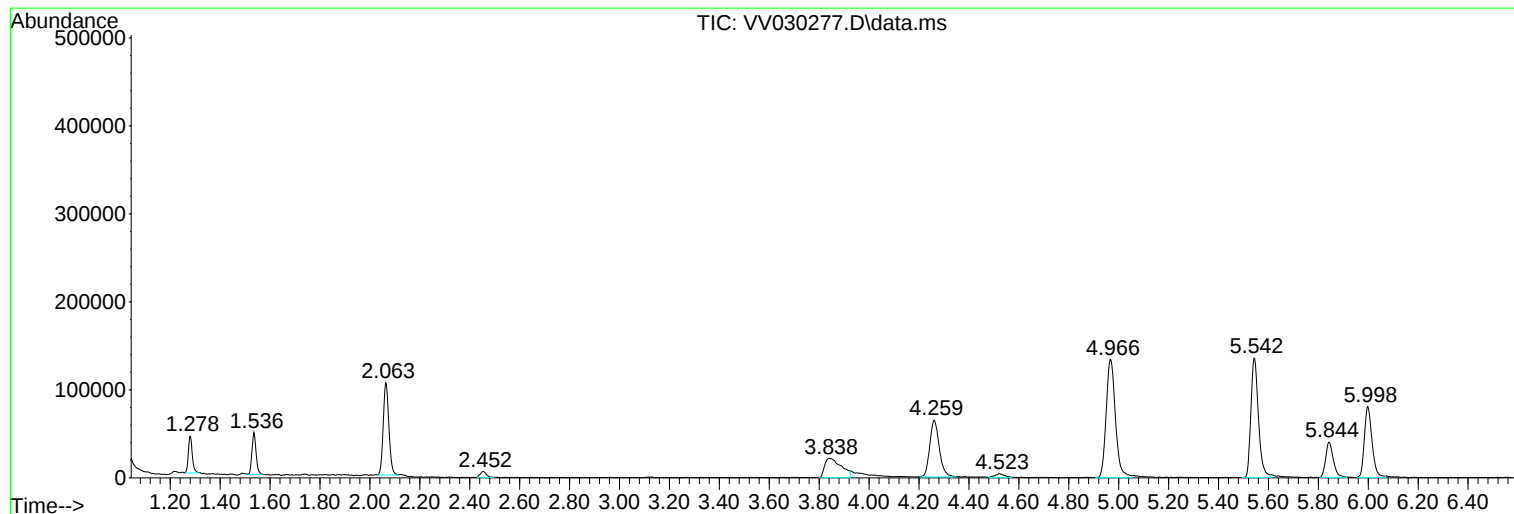

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030277.D
Acq On : 21 Mar 2023 14:59
Operator : SY/MD
Sample : 01996-09DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030277.D
Acq On : 21 Mar 2023 14:59
Operator : SY/MD
Sample : 01996-09DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------