

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030282.D
 Acq On : 21 Mar 2023 17:21
 Operator : SY/MD
 Sample : 02005-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	60	rBV6	3634	4765	1.18%	0.141%
2	1.281	68	75	86	rBV	61061	66095	16.38%	1.957%
3	1.535	147	154	165	rBV	57565	69979	17.34%	2.071%
4	2.063	305	318	333	rBV	128773	189121	46.87%	5.598%
5	2.452	428	439	450	rBV4	4760	8172	2.03%	0.242%
6	3.841	859	871	874	rBV2	21018	41321	10.24%	1.223%
7	4.262	985	1002	1033	rBV2	70484	189156	46.87%	5.599%
8	4.969	1204	1222	1246	rBV3	157447	403537	100.00%	11.945%
9	5.545	1388	1401	1424	rBV2	138371	290805	72.06%	8.608%
10	5.998	1529	1542	1567	rBV	91396	195381	48.42%	5.784%
11	6.921	1819	1829	1846	rBV	41131	78779	19.52%	2.332%
12	7.252	1920	1932	1958	rBV	187933	340104	84.28%	10.068%
13	7.564	2019	2029	2041	rBV2	24382	44685	11.07%	1.323%
14	7.918	2116	2139	2152	rBV5	13315	31005	7.68%	0.918%
15	8.037	2166	2176	2206	rBV	147080	311651	77.23%	9.225%
16	8.792	2398	2411	2436	rBV	215104	361249	89.52%	10.694%
17	10.162	2826	2837	2857	rVB2	64580	102855	25.49%	3.045%
18	10.332	2880	2890	2901	rBV3	7075	11377	2.82%	0.337%
19	11.194	3144	3158	3174	rBV	215722	340009	84.26%	10.065%
20	11.570	3264	3275	3295	rBV	186968	293811	72.81%	8.697%
21	12.204	3463	3472	3482	rVB5	2871	4351	1.08%	0.129%




Sum of corrected areas: 3378208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030282.D
Acq On : 21 Mar 2023 17:21
Operator : SY/MD
Sample : 02005-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

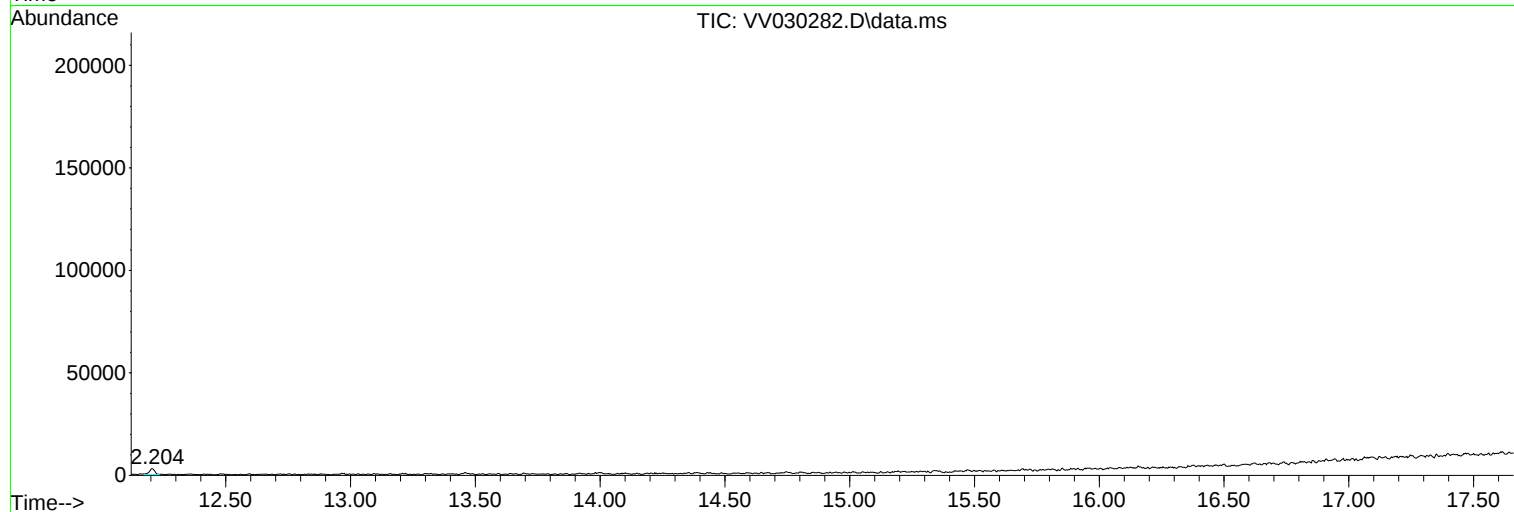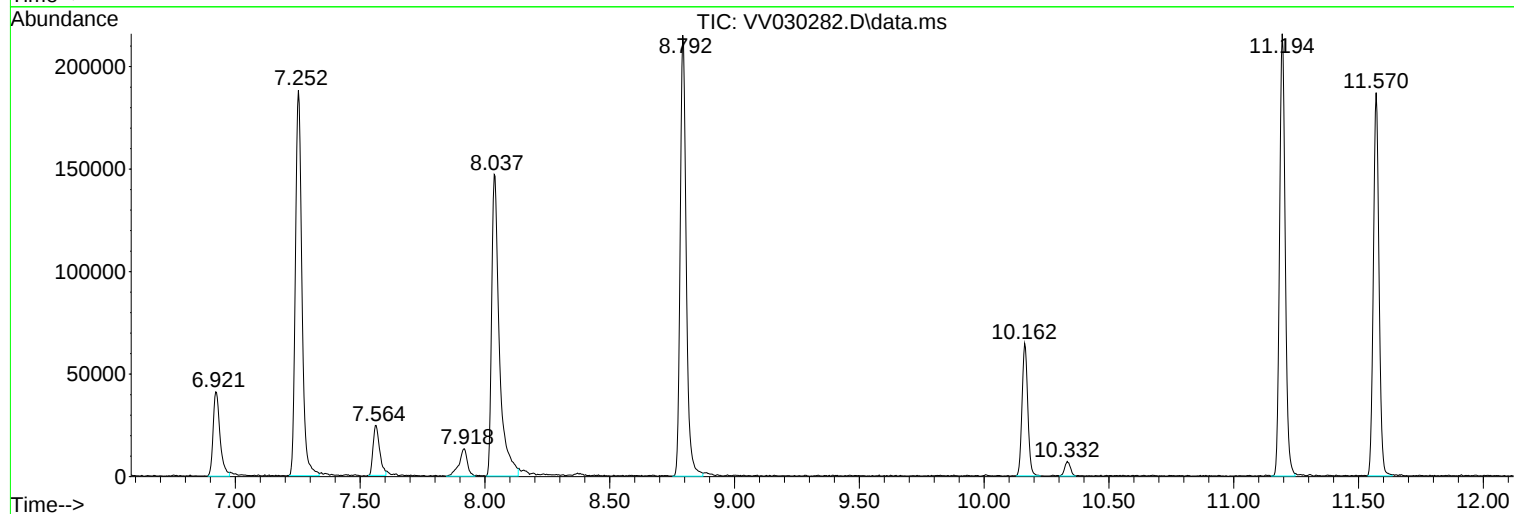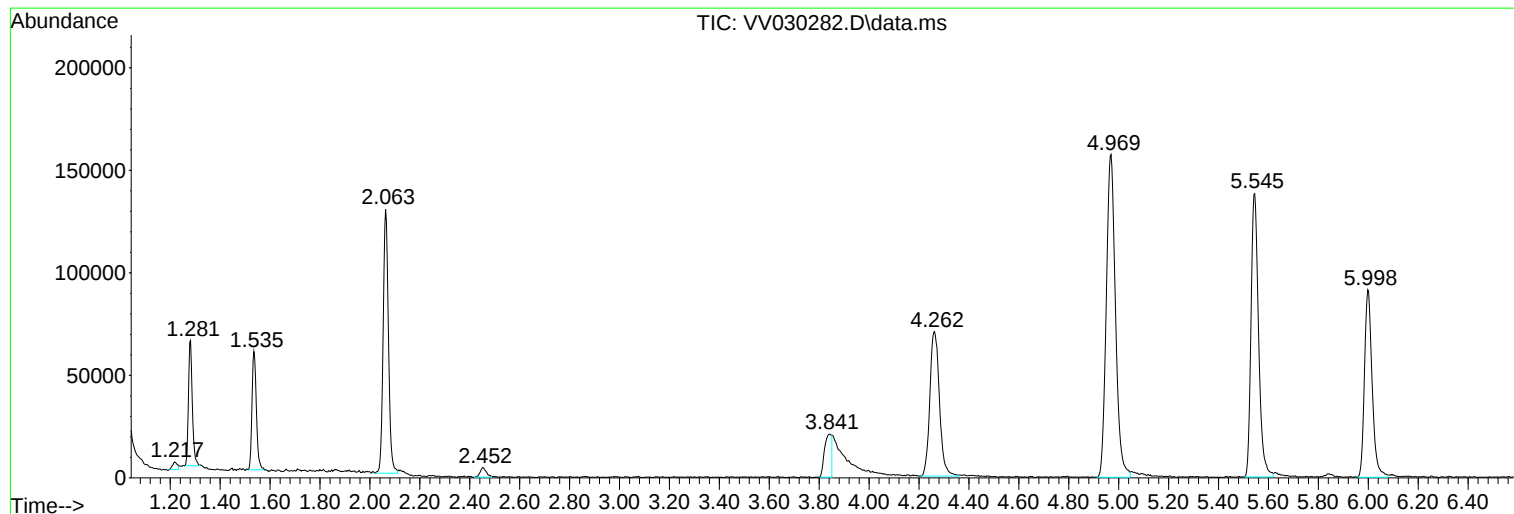

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030282.D
Acq On : 21 Mar 2023 17:21
Operator : SY/MD
Sample : 02005-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030282.D
Acq On : 21 Mar 2023 17:21
Operator : SY/MD
Sample : 02005-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc