

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
 Data File : VV030287.D
 Acq On : 21 Mar 2023 19:24
 Operator : SY/MD
 Sample : 01996-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV4	3746	4520	1.14%	0.133%
2	1.282	68	75	89	rVB	61991	68329	17.22%	2.017%
3	1.536	145	154	171	rVB	59111	72933	18.38%	2.153%
4	2.066	309	319	335	rBV	119899	176609	44.52%	5.214%
5	2.455	433	440	451	rVB3	4141	6901	1.74%	0.204%
6	3.815	851	863	902	rBV	34970	119684	30.17%	3.534%
7	4.262	985	1002	1025	rBV2	71781	185164	46.68%	5.467%
8	4.966	1203	1221	1242	rBV2	155062	396705	100.00%	11.712%
9	5.545	1386	1401	1429	rBV	141784	296894	74.84%	8.765%
10	5.998	1529	1542	1560	rBV3	91366	191147	48.18%	5.643%
11	6.921	1817	1829	1852	rBV	39676	78200	19.71%	2.309%
12	7.252	1919	1932	1960	rBV	189329	338042	85.21%	9.980%
13	7.561	2019	2028	2045	rBV2	25330	47621	12.00%	1.406%
14	7.915	2128	2138	2146	rVB7	5309	8366	2.11%	0.247%
15	8.034	2164	2175	2211	rBV	155345	307441	77.50%	9.077%
16	8.793	2400	2411	2434	rBV	215587	362517	91.38%	10.703%
17	10.162	2825	2837	2851	rBV	64671	102070	25.73%	3.014%
18	11.194	3146	3158	3178	rBV	209757	335958	84.69%	9.919%
19	11.571	3264	3275	3291	rBV	178616	287980	72.59%	8.502%




Sum of corrected areas: 3387081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030287.D
Acq On : 21 Mar 2023 19:24
Operator : SY/MD
Sample : 01996-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

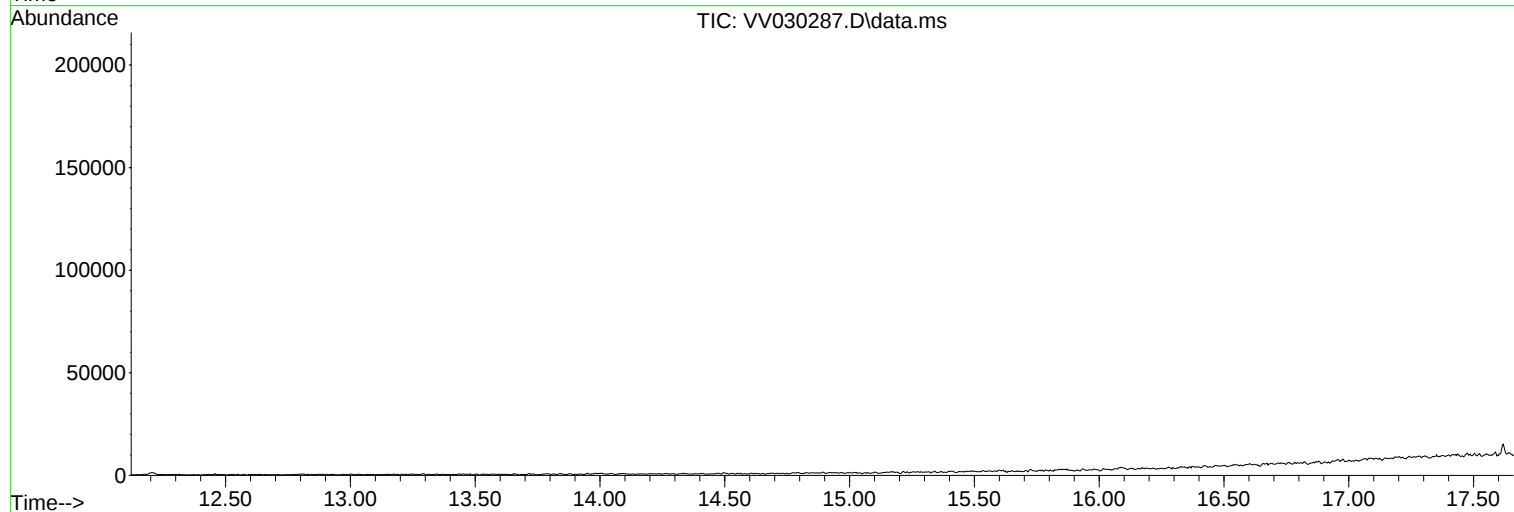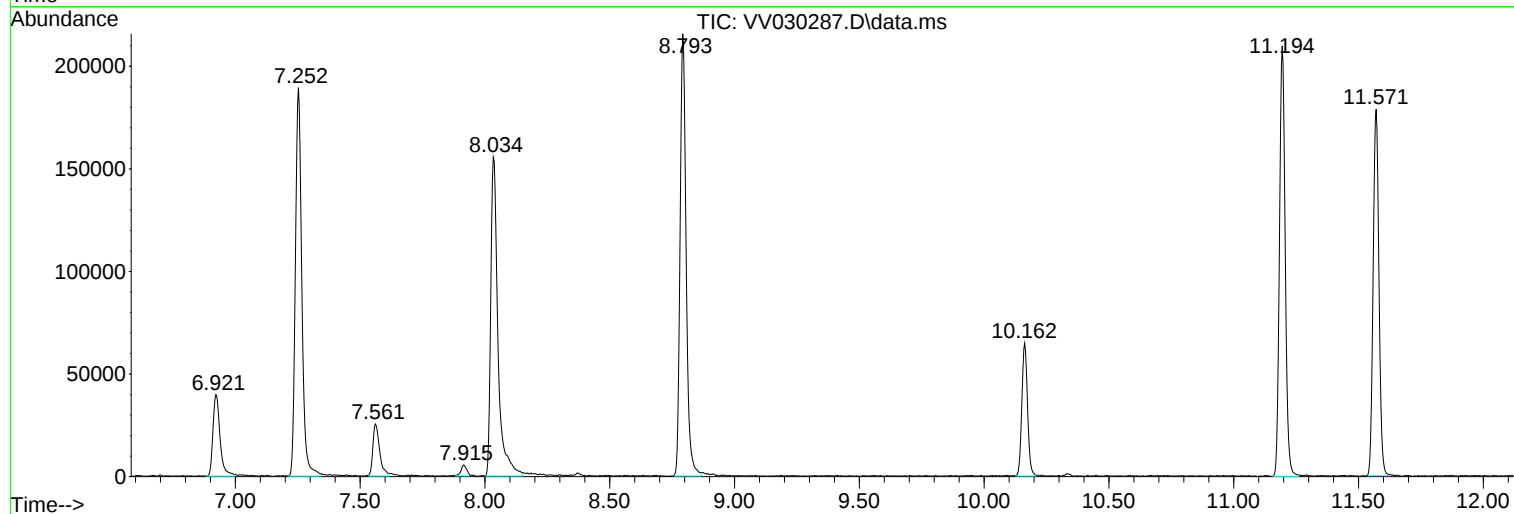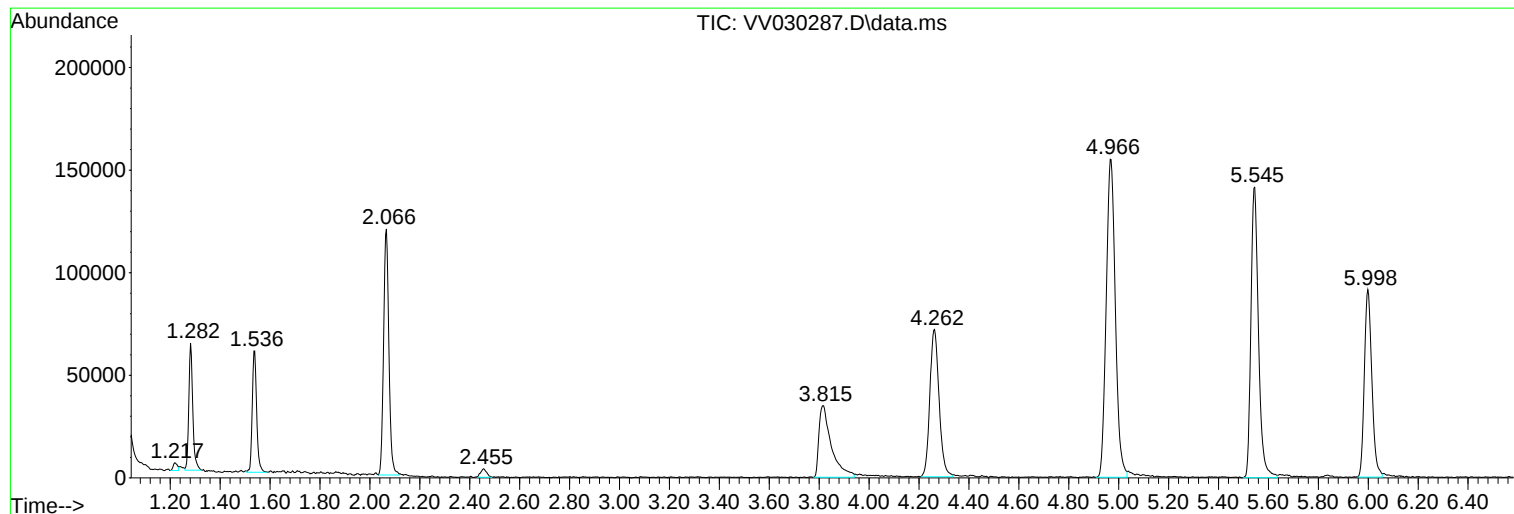

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030287.D
Acq On : 21 Mar 2023 19:24
Operator : SY/MD
Sample : 01996-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030287.D
Acq On : 21 Mar 2023 19:24
Operator : SY/MD
Sample : 01996-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc