


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032123\
Data File : VV030271.D
Acq On : 21 Mar 2023 11:29
Operator : SY/MD
Sample : BFB236
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB236

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 23 01:48:30 2023

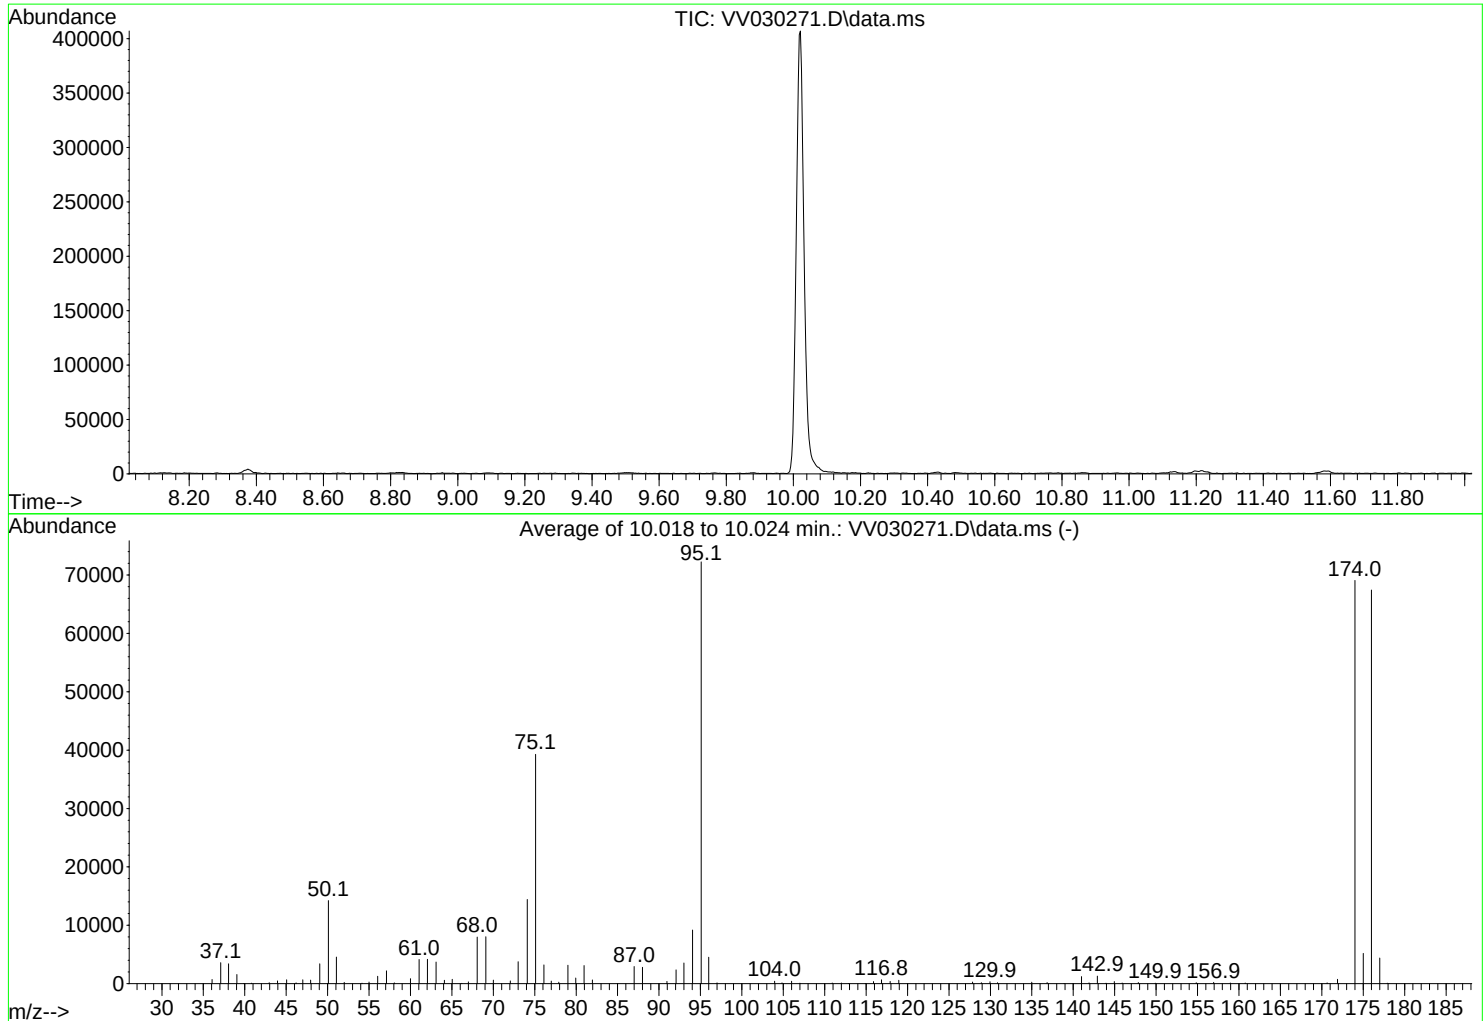

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	14225	PASS
75	95	30	80	54.4	39285	PASS
95	95	100	100	100.0	72259	PASS
96	95	5	9	6.3	4518	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.6	69075	PASS
175	174	5	9	7.5	5189	PASS
176	174	95	105	97.6	67435	PASS
177	176	5	10	6.5	4395	PASS

m/z	Abundance
40.00	186.0
43.90	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.10	770.0
37.10	3670.0
38.10	3461.0
39.00	1731.0
39.90	214.0
40.80	118.0
42.90	155.0
44.00	784.0
45.00	716.0
46.20	115.0
47.00	688.0
48.00	627.0
49.00	3485.0
50.10	14532.0
51.00	4975.0
52.00	245.0
55.00	267.0
56.10	1305.0
57.10	2331.0
58.00	150.0
60.00	873.0
61.10	4215.0
62.00	4330.0
63.10	3779.0
64.10	650.0
65.00	793.0
67.00	296.0
68.10	8302.0
69.10	8232.0
70.00	643.0
72.00	481.0
73.00	3771.0
74.10	14958.0
75.10	41112.0
76.10	3483.0
77.00	440.0
77.90	315.0
79.00	3109.0
80.00	917.0
81.00	3151.0
82.00	642.0
87.00	3245.0
88.00	2854.0
91.00	361.0
92.10	2443.0
93.00	3647.0
94.10	9501.0
95.10	74456.0
96.00	4758.0
97.00	160.0
104.00	451.0
104.90	123.0
106.00	413.0
110.90	140.0
112.00	108.0
112.90	107.0
114.90	111.0
115.90	367.0
116.90	721.0
117.90	377.0
118.90	525.0
127.90	265.0
128.90	151.0
130.00	400.0
130.80	124.0
135.00	250.0
136.80	185.0
141.00	1214.0
141.90	160.0
142.90	1298.0
143.90	121.0
144.90	366.0
145.90	113.0
147.90	197.0
149.90	116.0
155.00	153.0
156.90	175.0
159.00	116.0
160.70	136.0
170.70	153.0
171.90	646.0
174.00	69744.0
175.00	5277.0
176.00	67768.0
177.00	4436.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	720.0
37.10	3635.0
38.00	3464.0
39.00	1585.0
39.90	226.0
40.80	105.0
43.00	170.0
44.00	744.0
45.00	665.0
46.20	139.0
47.00	676.0
47.90	609.0
49.10	3544.0
50.10	14709.0
51.00	4715.0
52.00	234.0
54.20	119.0
55.00	273.0
56.00	1291.0
57.10	2276.0
58.00	149.0
60.00	859.0
61.00	4292.0
62.00	4298.0
63.10	3854.0
64.10	588.0
65.10	772.0
67.00	325.0
68.10	8239.0
69.10	8366.0
70.00	613.0
72.10	478.0
73.00	3898.0
74.10	14891.0
75.10	40576.0
76.10	3284.0
77.00	430.0
77.90	268.0
79.00	3189.0
79.90	1011.0
81.00	3236.0
82.00	634.0
87.00	3042.0
88.00	2946.0
90.90	381.0
92.10	2412.0
93.00	3659.0
94.10	9376.0
95.10	74984.0
96.00	4635.0
97.00	145.0
104.00	451.0
104.80	133.0
106.00	396.0
107.00	129.0
110.90	116.0
112.00	117.0
115.90	370.0
116.90	649.0
117.90	384.0
118.90	569.0
127.90	280.0
128.90	166.0
130.00	332.0
130.80	162.0
135.00	272.0
136.80	197.0
140.00	113.0
141.00	1237.0
141.90	150.0
142.90	1372.0
144.00	126.0
145.00	369.0
145.90	114.0
147.80	199.0
149.90	106.0
154.80	157.0
157.00	225.0
159.00	110.0
160.70	112.0
170.60	130.0
171.90	772.0
174.00	71432.0
175.00	5364.0
176.00	69736.0
177.00	4572.0
177.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	645.0
37.10	3436.0
38.00	3274.0
39.10	1358.0
39.90	194.0
43.00	161.0
44.00	584.0
45.10	591.0
46.20	146.0
47.00	632.0
47.90	552.0
49.10	3182.0
50.10	13434.0
51.10	3978.0
52.00	216.0
54.10	118.0
55.00	277.0
56.00	1200.0
57.10	2001.0
58.10	142.0
60.00	787.0
61.00	3901.0
62.10	3848.0
63.10	3447.0
64.10	495.0
65.10	692.0
66.20	137.0
67.00	295.0
68.00	7423.0
69.10	7535.0
70.00	536.0
72.10	439.0
73.00	3617.0
74.10	13386.0
75.10	36168.0
76.10	2863.0
77.00	422.0
77.90	207.0
79.00	3125.0
79.90	952.0
80.90	2909.0
81.90	584.0
87.00	2533.0
88.00	2604.0
91.00	393.0
92.00	2203.0
93.00	3313.0
94.00	8657.0
95.10	67336.0
96.00	4160.0
97.00	111.0
103.90	356.0
104.90	138.0
106.00	393.0
107.00	133.0
110.90	112.0
112.00	128.0
115.90	331.0
116.80	574.0
117.90	355.0
119.00	604.0
127.80	308.0
128.90	162.0
129.90	248.0
130.90	187.0
135.00	256.0
136.90	186.0
138.90	105.0
141.00	1143.0
141.90	137.0
142.90	1227.0
145.00	340.0
145.90	131.0
147.80	192.0
154.80	174.0
157.00	240.0
158.90	106.0
160.80	106.0
170.60	103.0
171.90	806.0
174.00	66048.0
175.00	4927.0
176.00	64800.0
177.00	4176.0
178.10	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236