

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034780.D
 Acq On : 21 Mar 2024 11:38
 Operator : SY/MD
 Sample : P1743-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 22 02:01:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 22 01:59:49 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	347814	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	331457	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	157751	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	156412	51.875	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	103.740%	
7) Chloroethane-d5	1.532	69	122148	51.999	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	104.000%	
11) 1,1-Dichloroethene-d2	2.060	65	49057	35.976	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.960%	
21) 2-Butanone-d5	3.789	46	161434	80.062	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	80.060%	
24) Chloroform-d	4.246	84	255414	47.910	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.820%	
26) 1,2-Dichloroethane-d4	4.937	65	173574	49.823	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.640%	
32) Benzene-d6	4.957	84	506265	50.609	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.220%	
36) 1,2-Dichloropropane-d6	5.986	67	156949	51.410	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	102.820%	
41) Toluene-d8	7.239	98	457108	50.494	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.980%	
43) trans-1,3-Dichloroprop...	7.551	79	75273	49.100	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	98.200%	
47) 2-Hexanone-d5	8.024	63	99778	65.451	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	65.450%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	190020	47.298	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.558	152	169416	52.541	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.080%	
Target Compounds						
39) cis-1,3-Dichloropropene	6.912	75	4949	1.134	ug/L	Qvalue # 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034780.D
Acq On : 21 Mar 2024 11:38
Operator : SY/MD
Sample : P1743-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 22 02:01:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 01:59:49 2024
Response via : Initial Calibration

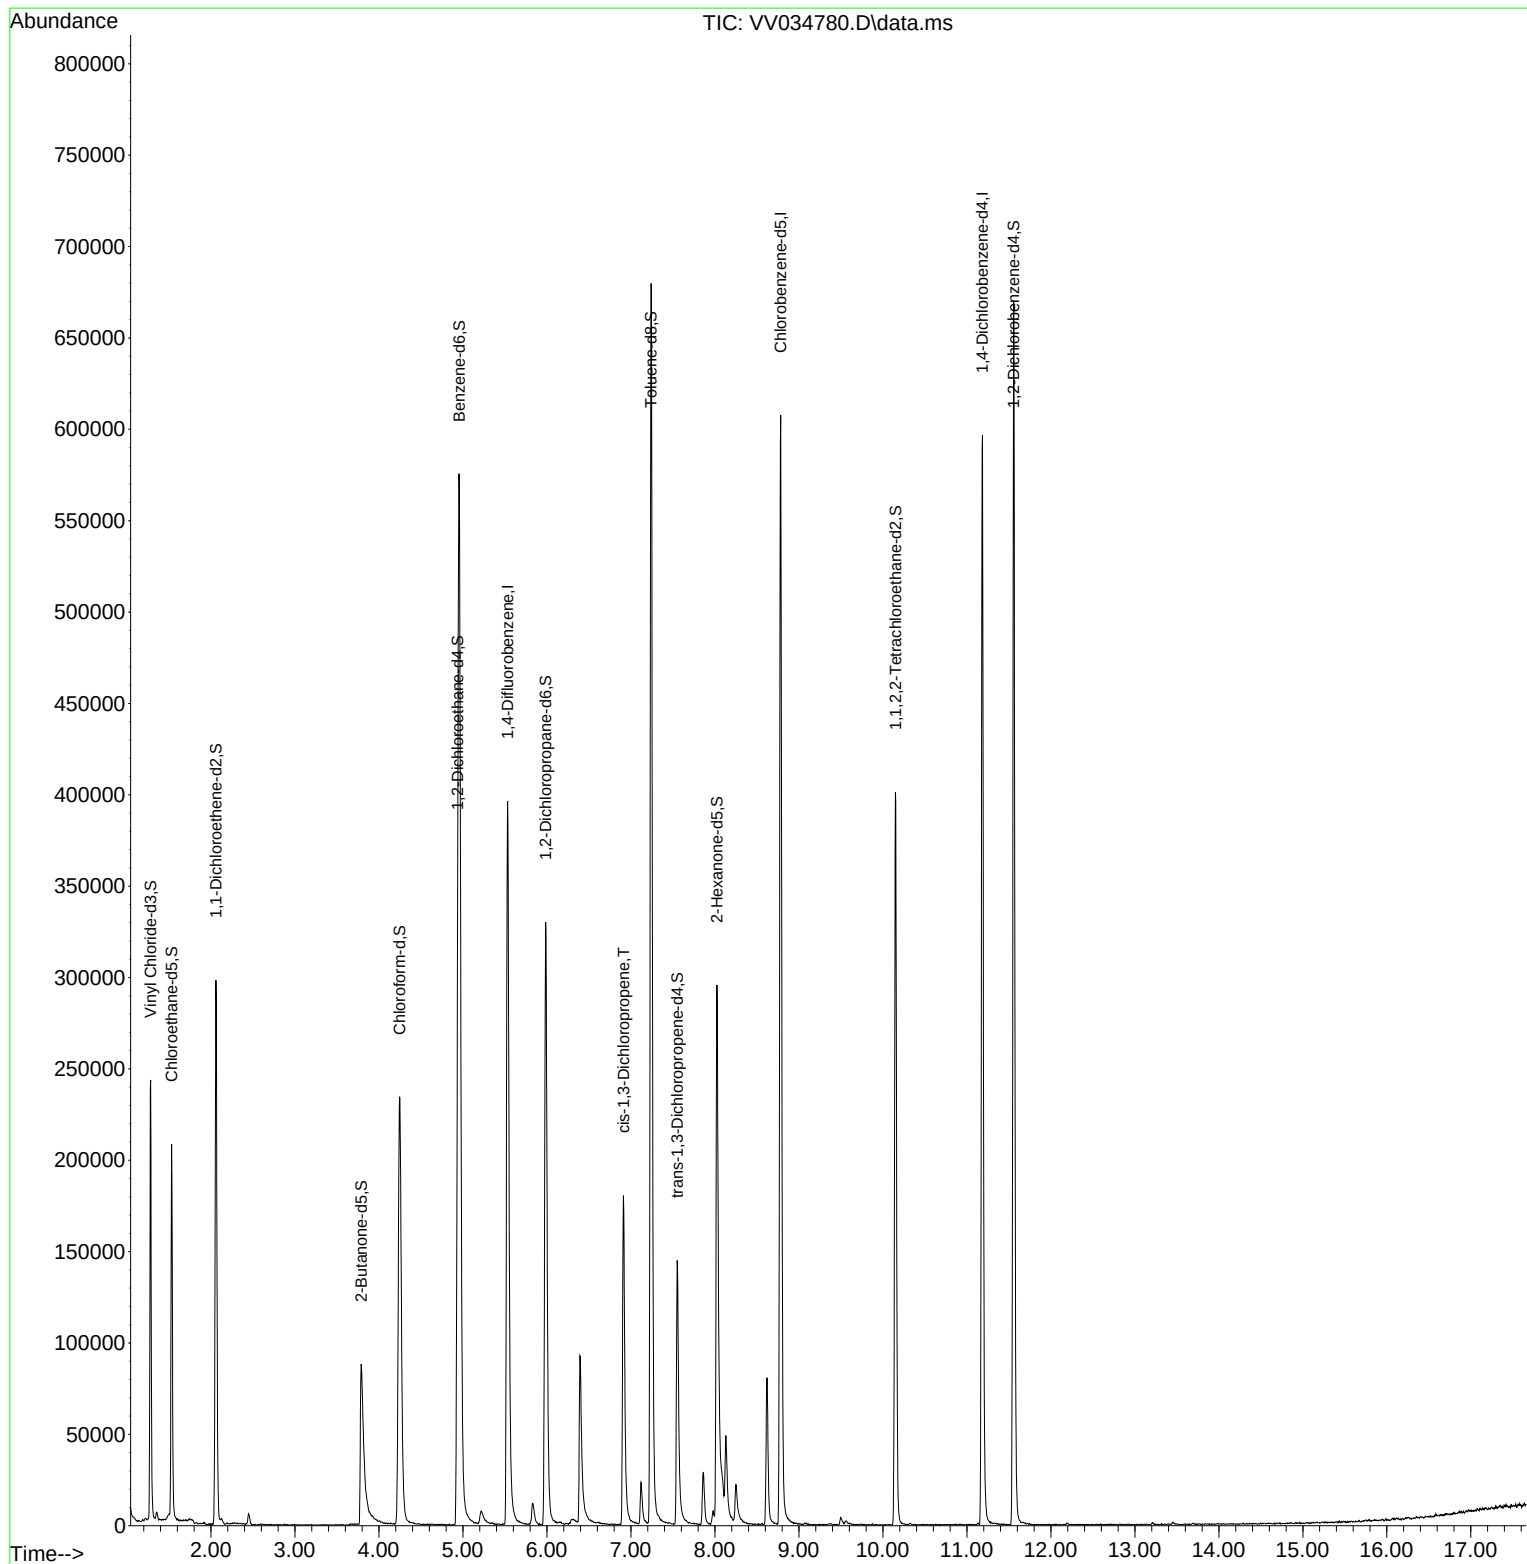

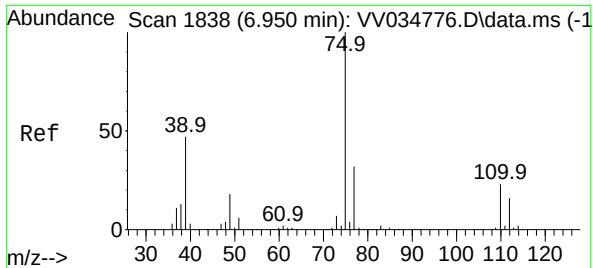

#39
 cis-1,3-Dichloropropene
 Concen: 1.134 ug/L
 RT: 6.912 min Scan# 11
 Delta R.T. -0.038 min
 Lab File: VV034780.D
 Acq: 21 Mar 2024 11:38

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4949
 Ion Ratio Lower Upper
 75 100
 77 57.7 20.9 38.9#

