

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034781.D
 Acq On : 21 Mar 2024 12:02
 Operator : SY/MD
 Sample : P1743-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 22 02:01:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 22 01:59:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	338046	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	323932	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	151701	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	159160	54.311	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 108.620%			
7) Chloroethane-d5	1.532	69	124598	54.575	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 109.140%			
11) 1,1-Dichloroethene-d2	2.060	65	57764	43.585	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 87.180%			
21) 2-Butanone-d5	3.793	46	161015	82.161	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 82.160%			
24) Chloroform-d	4.246	84	258495	49.889	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.780%			
26) 1,2-Dichloroethane-d4	4.937	65	174200	51.448	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.900%			
32) Benzene-d6	4.960	84	513270	52.501	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.000%			
36) 1,2-Dichloropropane-d6	5.985	67	155779	52.213	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 104.420%			
41) Toluene-d8	7.239	98	460036	51.998	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 104.000%			
43) trans-1,3-Dichloroprop...	7.551	79	75386	50.316	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.640%			
47) 2-Hexanone-d5	8.024	63	101181	67.913	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 67.910%			
56) 1,1,2,2-Tetrachloroeth...	10.149	84	192134	48.935	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 97.860%			
66) 1,2-Dichlorobenzene-d4	11.558	152	167808	54.117	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.240%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.911	75	5068	1.188	ug/L #	68
61) 1,2,3-Trichloropropane	11.181	75	17939	6.195	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034781.D
Acq On : 21 Mar 2024 12:02
Operator : SY/MD
Sample : P1743-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 22 02:01:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 01:59:49 2024
Response via : Initial Calibration




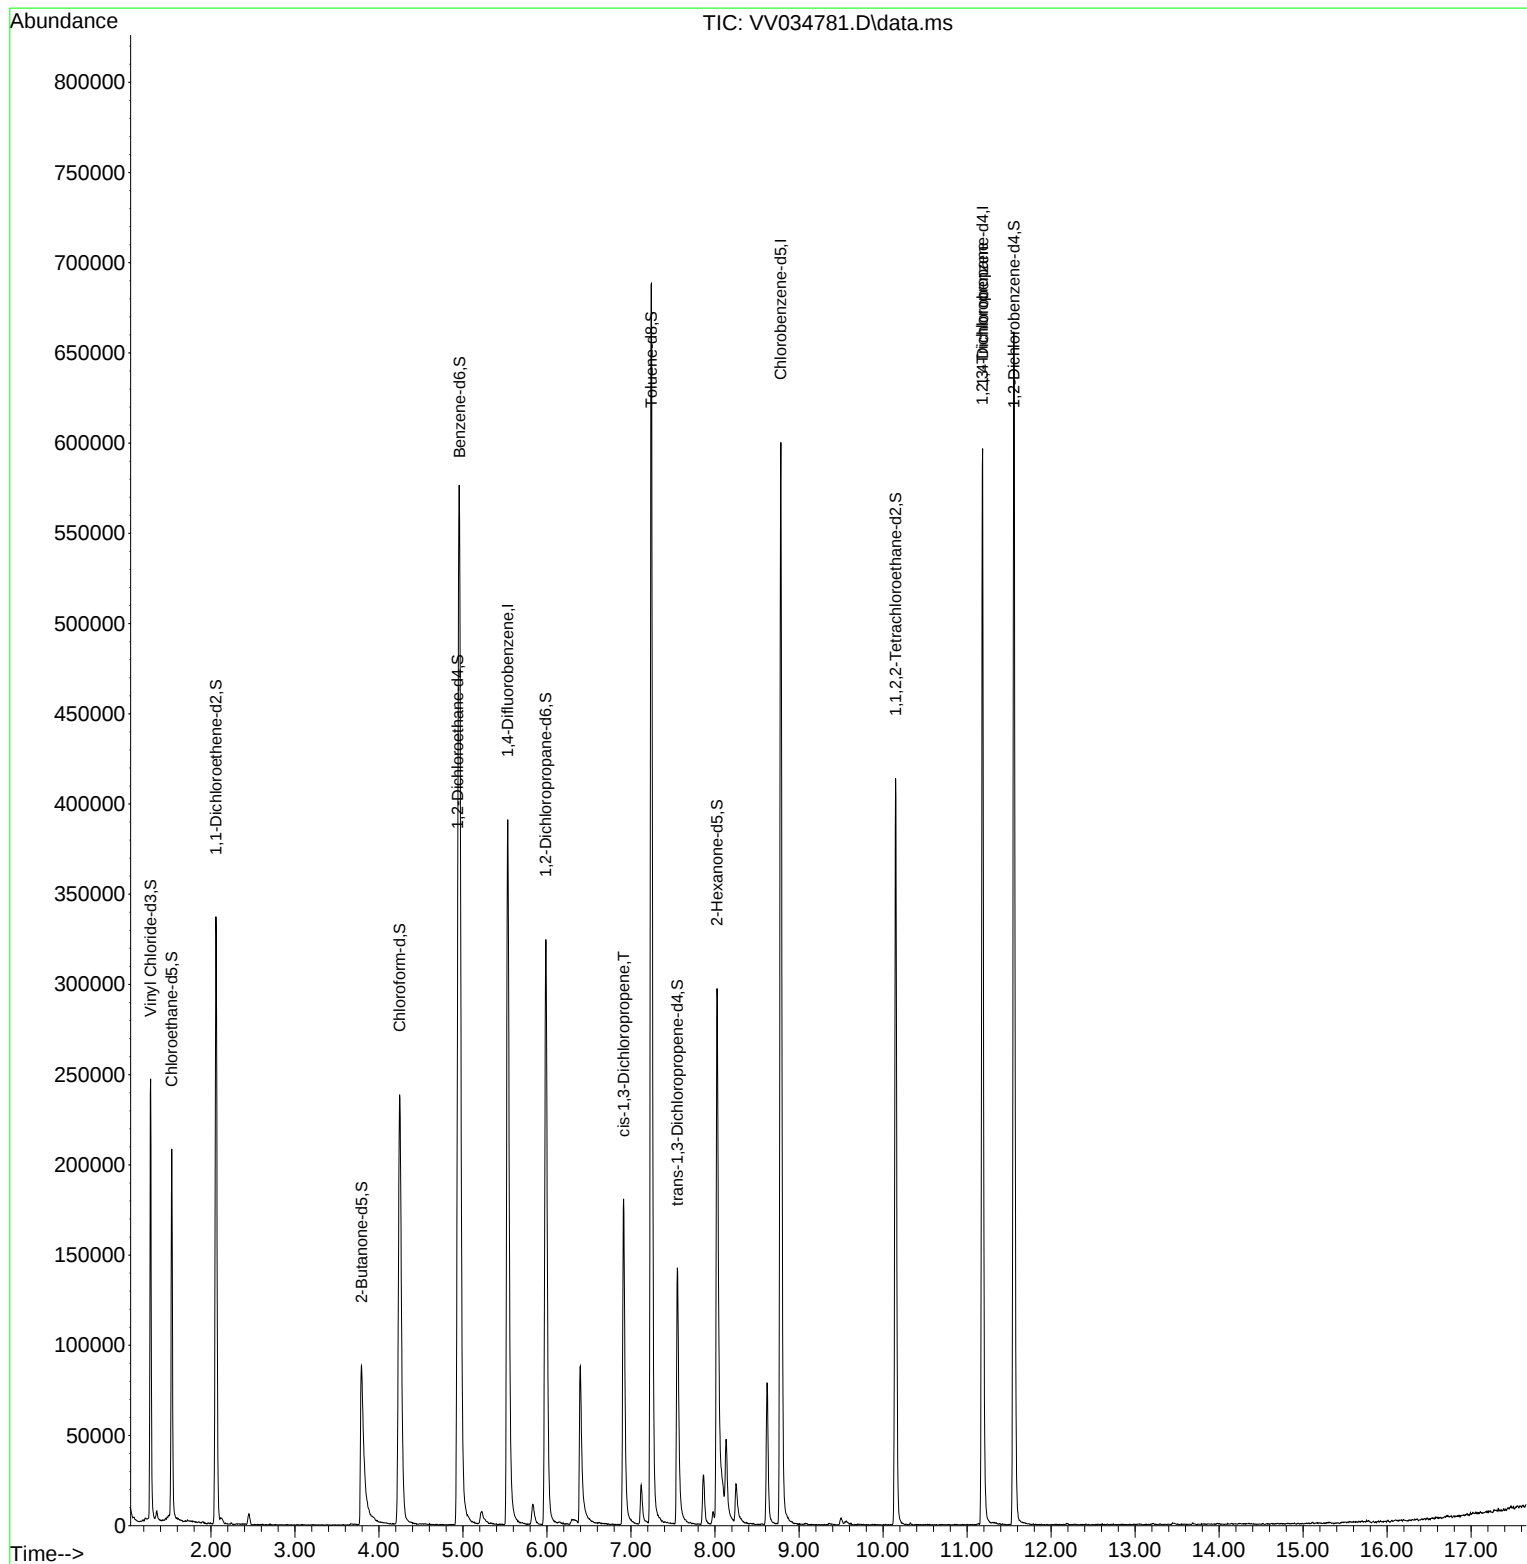


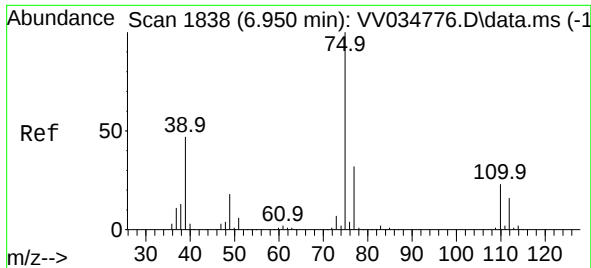

#39
cis-1,3-Dichloropropene
Concen: 1.188 ug/L
RT: 6.911 min Scan# 11
Delta R.T. -0.038 min
Lab File: VV034781.D
Acq: 21 Mar 2024 12:02

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 5068
Ion Ratio Lower Upper
75 100
77 47.3 20.9 38.9#

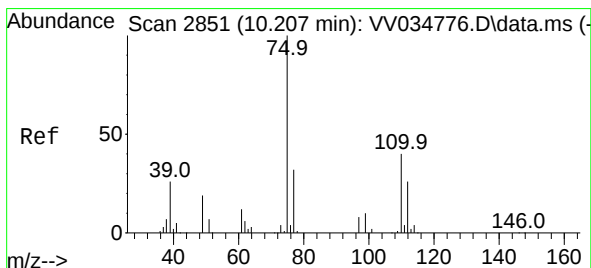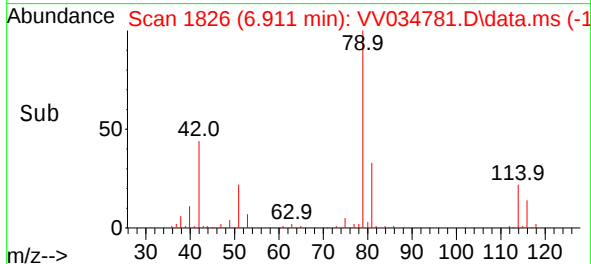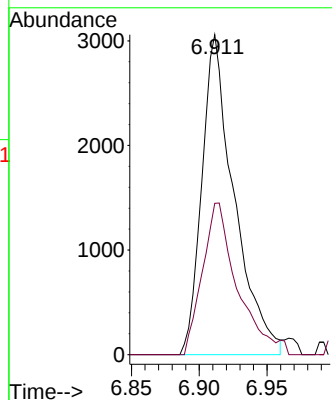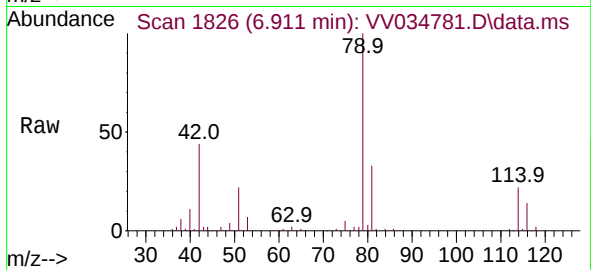

#61
1,2,3-Trichloropropane
Concen: 6.195 ug/L
RT: 11.181 min Scan# 3154
Delta R.T. 0.974 min
Lab File: VV034781.D
Acq: 21 Mar 2024 12:02

Tgt Ion: 75 Resp: 17939
Ion Ratio Lower Upper
75 100
77 35.9 25.9 38.9
110 2.6 33.1 49.7#

