

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034778.D
 Acq On : 21 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1778-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	253368	261223	16.59%	2.337%
2	1.532	146	153	168	rVB	205569	236463	15.02%	2.115%
3	2.060	307	317	334	rBV	347215	505407	32.10%	4.521%
4	2.175	350	353	356	rBV4	570	394	0.03%	0.004%
5	2.452	432	439	451	rVB4	3158	5136	0.33%	0.046%
6	2.629	491	494	496	rBV2	235	118	0.01%	0.001%
7	2.687	509	512	513	rBV2	187	107	0.01%	0.001%
8	2.703	513	517	525	rVV5	688	959	0.06%	0.009%
9	2.735	525	527	529	rVB2	281	112	0.01%	0.001%
10	2.857	563	565	568	rBV	149	91	0.01%	0.001%
11	2.896	574	577	579	rBV2	177	119	0.01%	0.001%
12	2.982	600	604	608	rBV2	296	221	0.01%	0.002%
13	3.011	609	613	616	rBV	231	198	0.01%	0.002%
14	3.163	656	660	663	rBV	140	102	0.01%	0.001%
15	3.208	667	674	679	rVV2	207	228	0.01%	0.002%
16	3.249	684	687	690	rBV2	213	144	0.01%	0.001%
17	3.445	745	748	754	rVB2	155	192	0.01%	0.002%
18	3.548	777	780	786	rBV2	96	87	0.01%	0.001%
19	3.622	800	803	807	rVB2	180	138	0.01%	0.001%
20	3.757	839	845	847	rBV	191	154	0.01%	0.001%
21	3.793	847	856	897	rBV	101885	311353	19.78%	2.785%
22	4.246	981	997	1031	rBV	239198	626458	39.79%	5.603%
23	4.674	1127	1130	1132	rBV2	199	151	0.01%	0.001%
24	4.732	1146	1148	1150	rBV3	377	243	0.02%	0.002%
25	4.834	1178	1180	1186	rVB3	371	278	0.02%	0.002%
26	4.953	1198	1217	1253	rBV2	595626	1574318	100.00%	14.081%
27	5.346	1336	1339	1341	rBV2	231	165	0.01%	0.001%
28	5.465	1371	1376	1378	rBV2	357	223	0.01%	0.002%
29	5.484	1381	1382	1386	rBV	218	169	0.01%	0.002%
30	5.532	1386	1397	1428	rBV	386792	799928	50.81%	7.155%
31	5.834	1479	1491	1515	rVB5	12364	29982	1.90%	0.268%
32	5.986	1525	1538	1570	rBV	330514	694284	44.10%	6.210%
33	6.217	1608	1610	1614	rBV3	405	353	0.02%	0.003%
34	6.246	1618	1619	1622	rVB	436	150	0.01%	0.001%
35	6.269	1622	1626	1630	rBV4	261	281	0.02%	0.003%
36	6.304	1634	1637	1640	rBV2	350	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034778.D
 Acq On : 21 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1778-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.381	1658	1661	1664	rBV2	269	135	0.01%	0.001%
38	6.442	1678	1680	1681	rBV	325	131	0.01%	0.001%
39	6.503	1697	1699	1703	rVB2	255	167	0.01%	0.001%
40	6.539	1703	1710	1713	rBV	199	187	0.01%	0.002%
41	6.555	1713	1715	1718	rVB2	223	153	0.01%	0.001%
42	6.574	1718	1721	1724	rBV2	92	79	0.01%	0.001%
43	6.606	1727	1731	1732	rBV	176	109	0.01%	0.001%
44	6.744	1771	1774	1777	rVB	217	129	0.01%	0.001%
45	6.764	1777	1780	1781	rBV	256	125	0.01%	0.001%
46	6.786	1785	1787	1790	rVV	162	87	0.01%	0.001%
47	6.812	1793	1795	1799	rVB2	345	137	0.01%	0.001%
48	6.834	1799	1802	1805	rBV	228	149	0.01%	0.001%
49	6.912	1815	1826	1850	rBV	181984	343003	21.79%	3.068%
50	7.130	1892	1894	1896	rBV2	271	124	0.01%	0.001%
51	7.240	1918	1928	1957	rBV	689147	1229249	78.08%	10.995%
52	7.551	2016	2025	2058	rBV	122157	227076	14.42%	2.031%
53	7.918	2135	2139	2145	rVB2	647	682	0.04%	0.006%
54	7.947	2145	2148	2150	rBV2	131	94	0.01%	0.001%
55	8.024	2163	2172	2214	rBV2	319427	679704	43.17%	6.080%
56	8.510	2320	2323	2325	rBV2	325	201	0.01%	0.002%
57	8.635	2356	2362	2364	rBV2	223	228	0.01%	0.002%
58	8.651	2364	2367	2370	rBV2	260	169	0.01%	0.002%
59	8.783	2397	2408	2443	rBV	591687	975348	61.95%	8.724%
60	9.024	2479	2483	2488	rVB3	407	420	0.03%	0.004%
61	9.059	2491	2494	2500	rVV3	479	442	0.03%	0.004%
62	9.095	2500	2505	2513	rVV2	618	900	0.06%	0.008%
63	9.140	2516	2519	2525	rVB2	415	230	0.01%	0.002%
64	9.172	2525	2529	2530	rBV2	234	143	0.01%	0.001%
65	9.233	2544	2548	2553	rBV2	277	269	0.02%	0.002%
66	9.294	2565	2567	2571	rBV	265	185	0.01%	0.002%
67	9.548	2639	2646	2647	rBV3	396	405	0.03%	0.004%
68	9.686	2686	2689	2691	rBV	140	87	0.01%	0.001%
69	9.767	2711	2714	2719	rVB2	186	153	0.01%	0.001%
70	9.796	2719	2723	2724	rBV	173	116	0.01%	0.001%
71	9.873	2743	2747	2750	rBV2	475	457	0.03%	0.004%
72	10.021	2789	2793	2797	rBV2	271	192	0.01%	0.002%
73	10.072	2805	2809	2813	rBV	265	248	0.02%	0.002%
74	10.149	2819	2833	2861	rBV	427996	683736	43.43%	6.116%
75	10.297	2876	2879	2881	rBV2	271	141	0.01%	0.001%
76	10.323	2881	2887	2888	rBV3	454	452	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034778.D
 Acq On : 21 Mar 2024 10:49
 Operator : SY/MD
 Sample : P1778-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.355	2894	2897	2902	rBV2	286	199	0.01%	0.002%
78	10.416	2914	2916	2920	rBV2	230	106	0.01%	0.001%
79	10.484	2931	2937	2941	rVV3	741	910	0.06%	0.008%
80	10.635	2982	2984	2987	rBV	180	82	0.01%	0.001%
81	10.654	2987	2990	2991	rBV	216	103	0.01%	0.001%
82	10.792	3030	3033	3036	rBV3	433	320	0.02%	0.003%
83	10.837	3045	3047	3049	rBV2	209	87	0.01%	0.001%
84	10.866	3051	3056	3063	rVB4	810	974	0.06%	0.009%
85	11.034	3105	3108	3112	rBV	232	152	0.01%	0.001%
86	11.130	3133	3138	3144	rBV4	1174	1610	0.10%	0.014%
87	11.185	3144	3155	3180	rVV	568709	903186	57.37%	8.079%
88	11.423	3225	3229	3233	rBV4	464	449	0.03%	0.004%
89	11.558	3259	3271	3299	rBV	656923	1061104	67.40%	9.491%
90	12.017	3413	3414	3416	rBV2	334	95	0.01%	0.001%
91	12.403	3529	3534	3536	rBV2	357	286	0.02%	0.003%
92	12.593	3588	3593	3597	rBV2	617	655	0.04%	0.006%
93	12.644	3607	3609	3613	rBV2	242	212	0.01%	0.002%
94	12.915	3690	3693	3701	rBV	386	407	0.03%	0.004%
95	13.027	3725	3728	3731	rBV2	278	170	0.01%	0.002%
96	13.210	3778	3785	3791	rBV7	2249	3484	0.22%	0.031%
97	13.451	3853	3860	3871	rBV4	3853	5967	0.38%	0.053%
98	13.641	3918	3919	3920	rBV4	234	85	0.01%	0.001%
99	13.686	3929	3933	3941	rVB7	1956	2704	0.17%	0.024%
100	14.731	4252	4258	4260	rBV5	600	560	0.04%	0.005%




Sum of corrected areas: 11180090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034778.D
Acq On : 21 Mar 2024 10:49
Operator : SY/MD
Sample : P1778-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

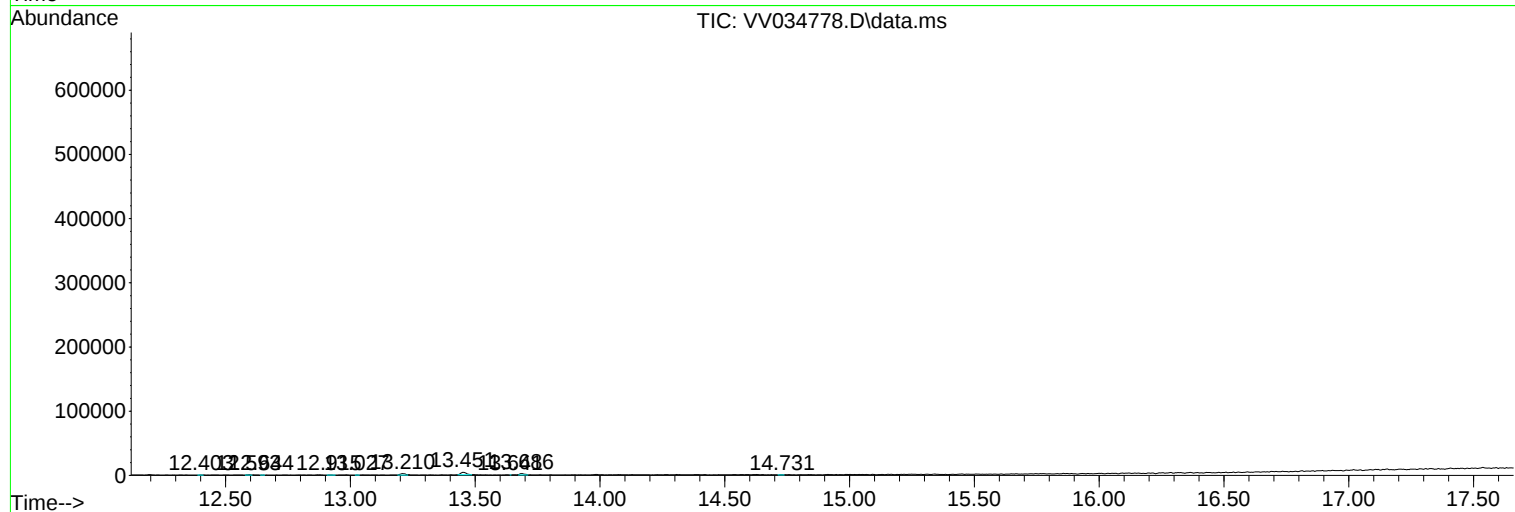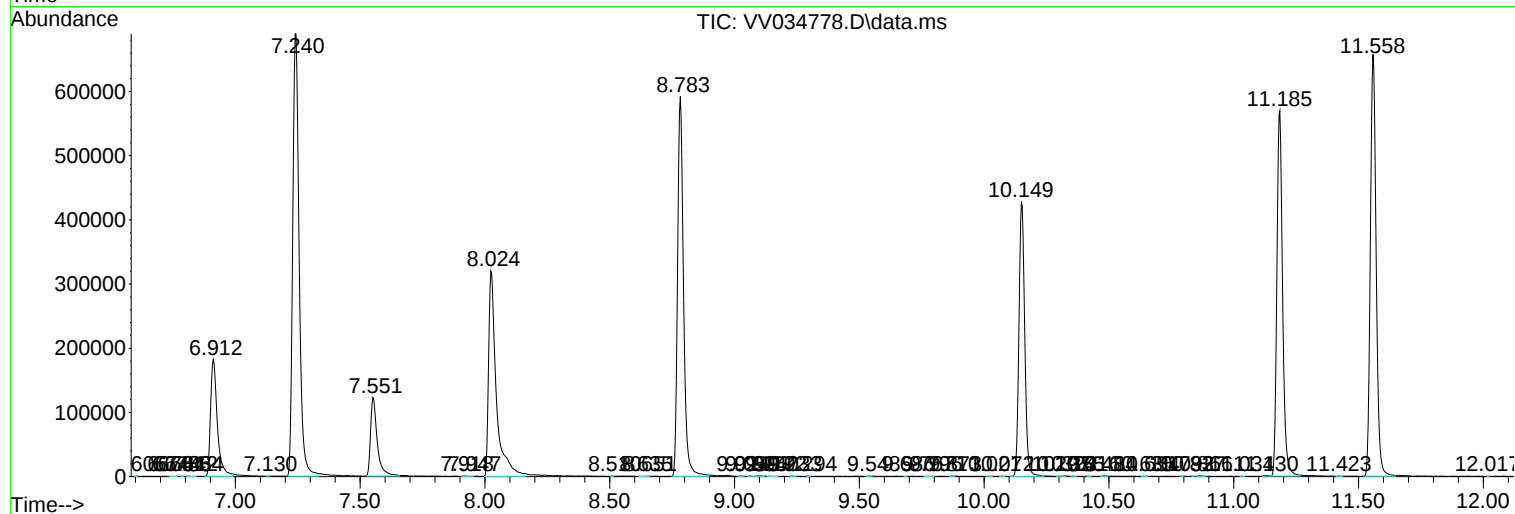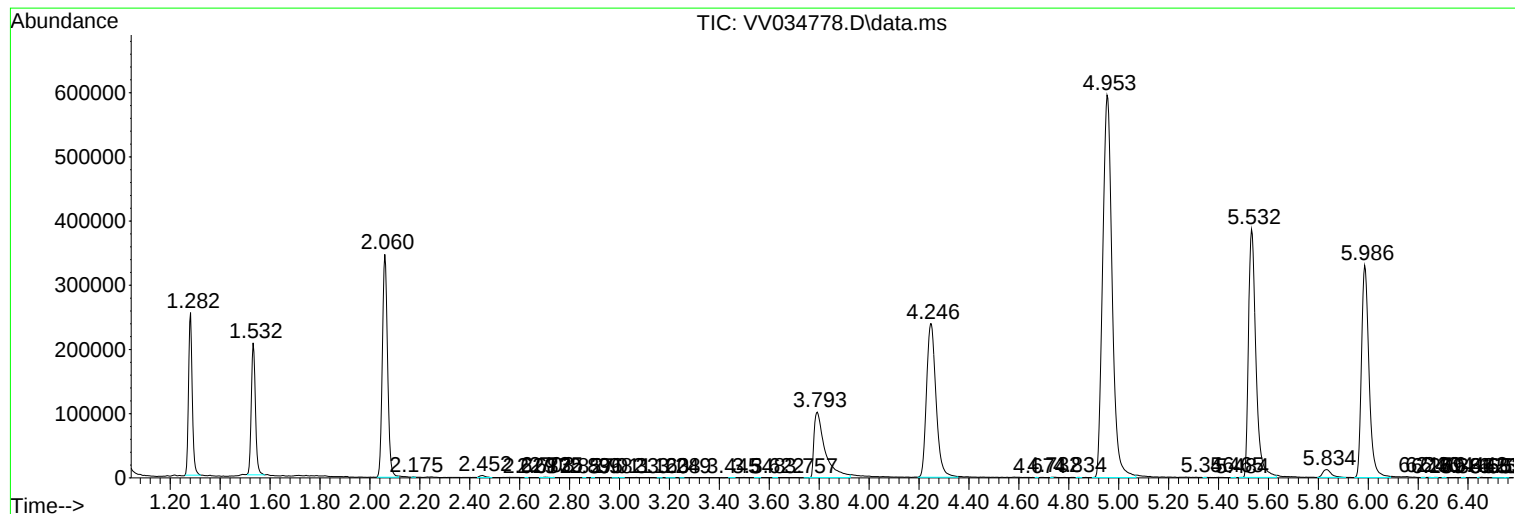

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034778.D
Acq On : 21 Mar 2024 10:49
Operator : SY/MD
Sample : P1778-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034778.D
Acq On : 21 Mar 2024 10:49
Operator : SY/MD
Sample : P1778-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc