

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034783.D
 Acq On : 21 Mar 2024 12:50
 Operator : SY/MD
 Sample : P1755-15DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rVB	235210	249341	16.50%	2.251%
2	1.532	146	153	176	rVB	200336	234615	15.53%	2.118%
3	2.060	306	317	328	rBV	312142	457501	30.28%	4.130%
4	2.121	329	336	362	rVB	147051	297345	19.68%	2.684%
5	2.738	524	528	529	rBV	331	206	0.01%	0.002%
6	2.860	564	566	571	rVB3	272	138	0.01%	0.001%
7	2.892	572	576	578	rBV2	184	163	0.01%	0.001%
8	2.931	585	588	591	rBV2	130	128	0.01%	0.001%
9	2.982	601	604	607	rVB	320	138	0.01%	0.001%
10	3.050	619	625	631	rBV	270	367	0.02%	0.003%
11	3.114	636	645	646	rBV2	2119	2453	0.16%	0.022%
12	3.230	676	681	683	rBV	119	126	0.01%	0.001%
13	3.320	706	709	713	rVB2	248	177	0.01%	0.002%
14	3.362	719	722	725	rBV2	237	150	0.01%	0.001%
15	3.568	783	786	787	rBV2	334	119	0.01%	0.001%
16	3.616	797	801	805	rBV2	288	147	0.01%	0.001%
17	3.671	816	818	820	rBV2	180	109	0.01%	0.001%
18	3.793	847	856	895	rBV	96565	297427	19.68%	2.685%
19	4.246	982	997	1030	rBV	235617	607033	40.17%	5.480%
20	4.670	1125	1129	1133	rBV2	288	271	0.02%	0.002%
21	4.693	1133	1136	1138	rBV	177	118	0.01%	0.001%
22	4.828	1174	1178	1179	rBV	273	166	0.01%	0.001%
23	4.953	1201	1217	1259	rBV2	565740	1511119	100.00%	13.643%
24	5.381	1347	1350	1352	rBV2	241	161	0.01%	0.001%
25	5.452	1367	1372	1375	rBV3	403	372	0.02%	0.003%
26	5.481	1379	1381	1384	rBV3	223	150	0.01%	0.001%
27	5.532	1386	1397	1429	rBV	384970	796005	52.68%	7.186%
28	5.834	1481	1491	1507	rBV4	11203	23740	1.57%	0.214%
29	5.986	1526	1538	1567	rBV	319191	658597	43.58%	5.946%
30	6.297	1633	1635	1637	rBV2	284	147	0.01%	0.001%
31	6.339	1644	1648	1651	rBV3	368	354	0.02%	0.003%
32	6.381	1658	1661	1663	rBV2	206	163	0.01%	0.001%
33	6.397	1663	1666	1672	rVB2	354	280	0.02%	0.003%
34	6.439	1677	1679	1681	rVB	336	151	0.01%	0.001%
35	6.465	1681	1687	1691	rVB2	407	347	0.02%	0.003%
36	6.497	1691	1697	1699	rBV3	431	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034783.D
 Acq On : 21 Mar 2024 12:50
 Operator : SY/MD
 Sample : P1755-15DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.510	1699	1701	1705	rVB2	347	200	0.01%	0.002%
38	6.532	1705	1708	1713	rVB2	416	231	0.02%	0.002%
39	6.568	1716	1719	1724	rBV3	249	278	0.02%	0.003%
40	6.693	1756	1758	1761	rBV3	280	146	0.01%	0.001%
41	6.754	1773	1777	1778	rBV	194	116	0.01%	0.001%
42	6.863	1807	1811	1814	rBV2	208	157	0.01%	0.001%
43	6.912	1815	1826	1863	rBV	173506	337620	22.34%	3.048%
44	7.146	1896	1899	1903	rVB3	498	358	0.02%	0.003%
45	7.169	1903	1906	1909	rBV2	387	218	0.01%	0.002%
46	7.240	1917	1928	1967	rBV	660796	1189971	78.75%	10.743%
47	7.551	2016	2025	2055	rBV	117836	218862	14.48%	1.976%
48	7.764	2088	2091	2094	rBV3	311	247	0.02%	0.002%
49	7.821	2107	2109	2111	rBV2	262	169	0.01%	0.002%
50	7.873	2116	2125	2134	rVB3	1482	2034	0.13%	0.018%
51	8.024	2163	2172	2211	rBV	310479	646046	42.75%	5.833%
52	8.420	2293	2295	2298	rBV3	334	142	0.01%	0.001%
53	8.551	2334	2336	2344	rVV4	714	624	0.04%	0.006%
54	8.584	2344	2346	2349	rVB2	306	147	0.01%	0.001%
55	8.635	2356	2362	2364	rBV4	651	568	0.04%	0.005%
56	8.783	2397	2408	2444	rBV	577939	969061	64.13%	8.749%
57	9.043	2487	2489	2493	rBV3	513	374	0.02%	0.003%
58	9.063	2493	2495	2498	rVV	362	232	0.02%	0.002%
59	9.137	2516	2518	2527	rVB3	526	610	0.04%	0.006%
60	9.175	2527	2530	2535	rBV2	347	286	0.02%	0.003%
61	9.233	2546	2548	2554	rBV	227	242	0.02%	0.002%
62	9.326	2575	2577	2580	rVB2	393	146	0.01%	0.001%
63	9.368	2586	2590	2592	rVB2	261	150	0.01%	0.001%
64	9.436	2608	2611	2613	rBV2	235	173	0.01%	0.002%
65	9.477	2619	2624	2627	rBV2	392	412	0.03%	0.004%
66	9.519	2633	2637	2641	rVB2	371	353	0.02%	0.003%
67	9.609	2663	2665	2668	rVB	493	252	0.02%	0.002%
68	9.641	2672	2675	2680	rBV	220	149	0.01%	0.001%
69	9.693	2688	2691	2692	rBV	276	126	0.01%	0.001%
70	9.728	2700	2702	2705	rVB3	285	127	0.01%	0.001%
71	9.802	2723	2725	2729	rVB2	212	109	0.01%	0.001%
72	9.841	2734	2737	2738	rBV	208	114	0.01%	0.001%
73	9.886	2747	2751	2754	rVB2	287	255	0.02%	0.002%
74	10.008	2784	2789	2792	rBV2	268	217	0.01%	0.002%
75	10.104	2817	2819	2821	rBV	169	105	0.01%	0.001%
76	10.149	2821	2833	2861	rVV	416558	653799	43.27%	5.903%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034783.D
 Acq On : 21 Mar 2024 12:50
 Operator : SY/MD
 Sample : P1755-15DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.371	2900	2902	2906	rVB	428	234	0.02%	0.002%
78	10.413	2912	2915	2918	rVV2	294	176	0.01%	0.002%
79	10.628	2977	2982	2989	rBV2	280	316	0.02%	0.003%
80	10.702	3003	3005	3010	rVB2	295	206	0.01%	0.002%
81	10.767	3023	3025	3027	rVB2	246	117	0.01%	0.001%
82	10.837	3043	3047	3048	rBV2	280	152	0.01%	0.001%
83	10.908	3065	3069	3071	rBV	163	123	0.01%	0.001%
84	11.082	3118	3123	3125	rBV2	280	237	0.02%	0.002%
85	11.185	3143	3155	3184	rBV	558997	894284	59.18%	8.074%
86	11.558	3259	3271	3297	rBV	633999	1012142	66.98%	9.138%
87	11.763	3331	3335	3338	rVB2	387	324	0.02%	0.003%
88	11.860	3359	3365	3366	rBV3	367	290	0.02%	0.003%
89	11.870	3366	3368	3372	rVV2	364	256	0.02%	0.002%
90	12.516	3566	3569	3570	rBV	352	154	0.01%	0.001%
91	12.587	3588	3591	3595	rVB	253	143	0.01%	0.001%
92	12.741	3637	3639	3643	rBV	297	195	0.01%	0.002%
93	12.760	3643	3645	3647	rBV	174	105	0.01%	0.001%
94	13.181	3774	3776	3778	rBV	353	199	0.01%	0.002%
95	13.252	3795	3798	3800	rBV3	253	150	0.01%	0.001%
96	13.297	3809	3812	3814	rBV2	296	169	0.01%	0.002%
97	13.378	3835	3837	3841	rVB2	434	218	0.01%	0.002%
98	13.503	3873	3876	3879	rVB3	438	253	0.02%	0.002%
99	13.522	3879	3882	3883	rBV2	298	191	0.01%	0.002%
100	13.693	3933	3935	3939	rBV3	354	163	0.01%	0.001%




Sum of corrected areas: 11076398

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034783.D
Acq On : 21 Mar 2024 12:50
Operator : SY/MD
Sample : P1755-15DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

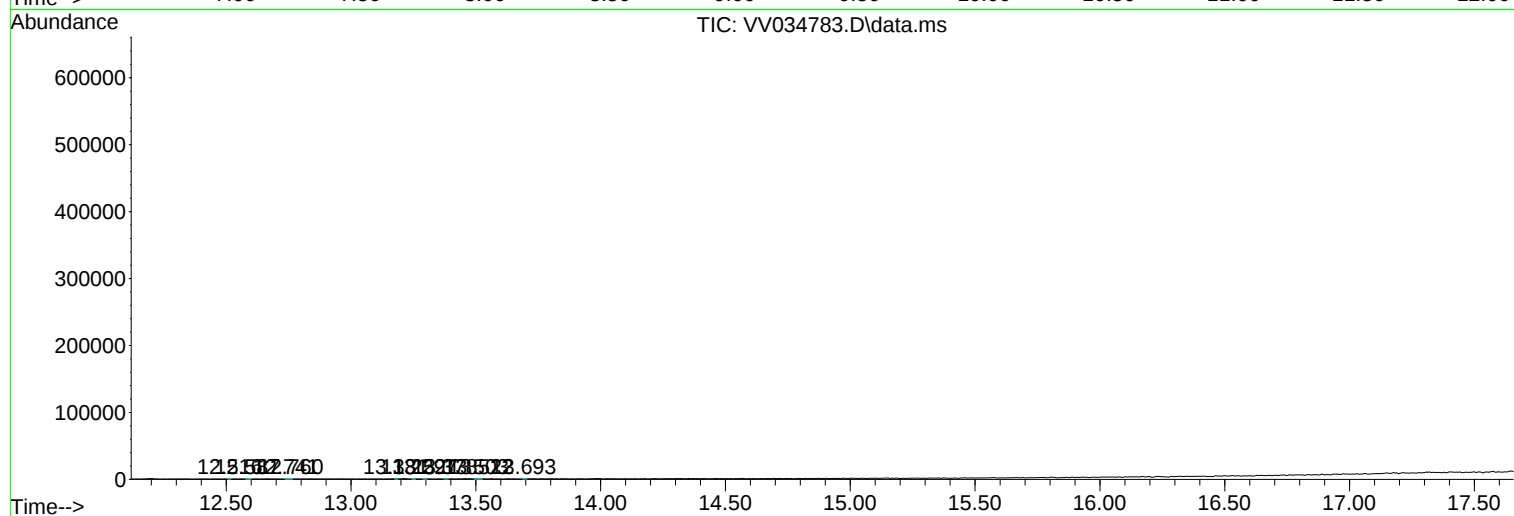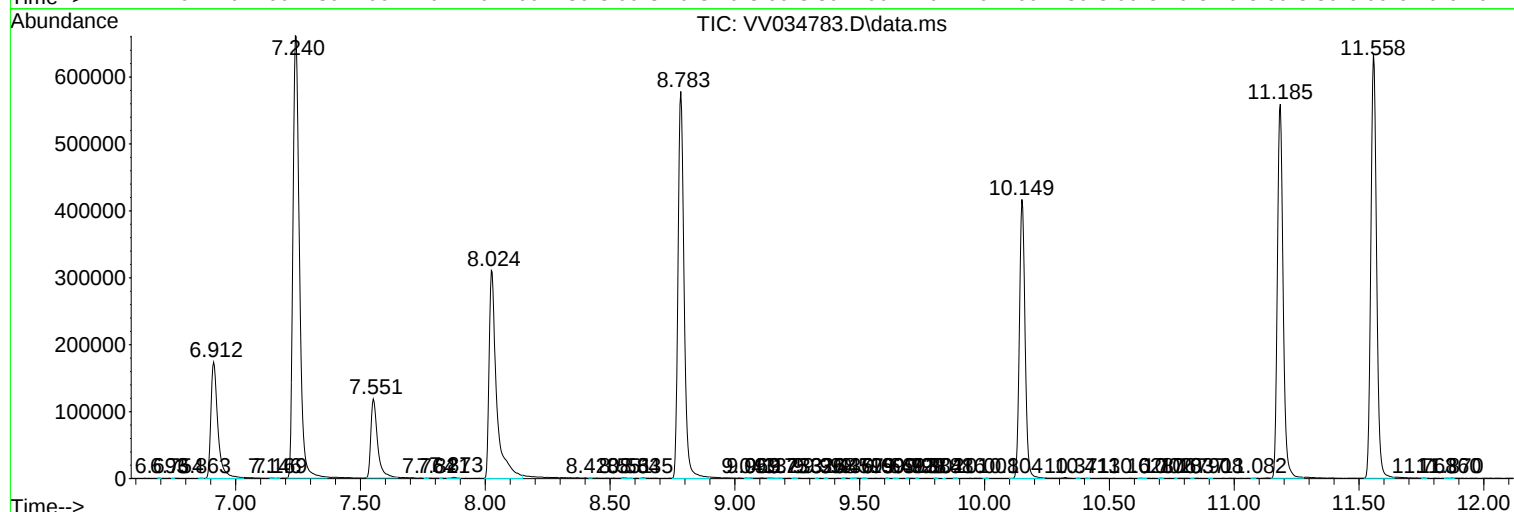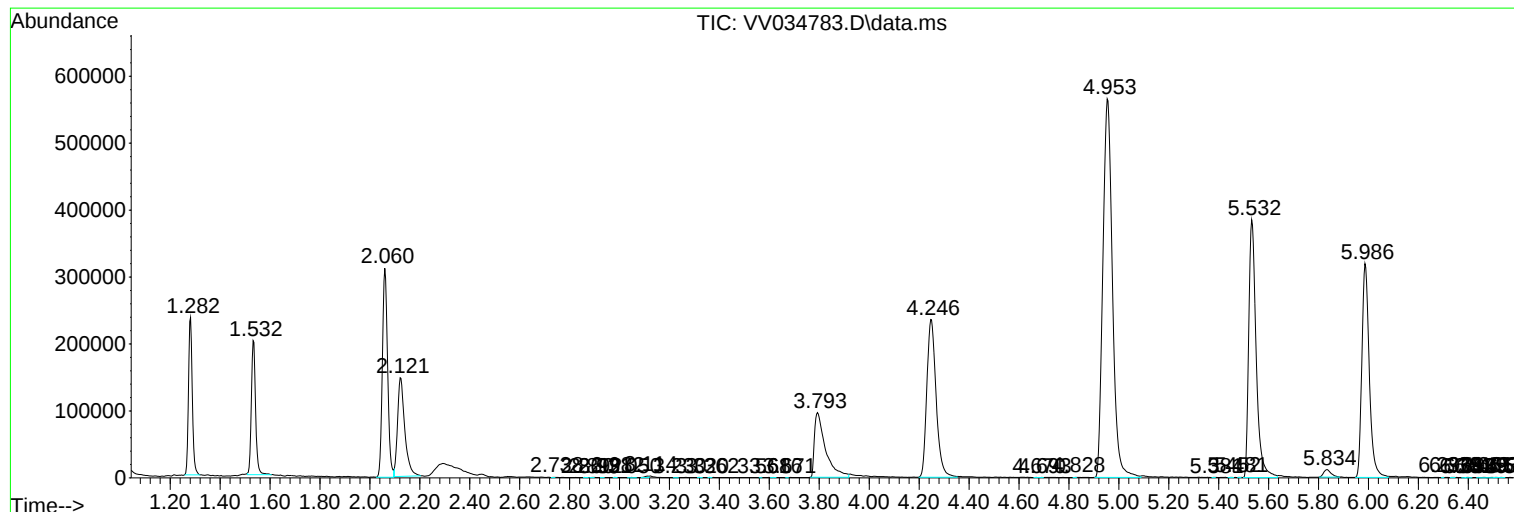

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034783.D
Acq On : 21 Mar 2024 12:50
Operator : SY/MD
Sample : P1755-15DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034783.D
Acq On : 21 Mar 2024 12:50
Operator : SY/MD
Sample : P1755-15DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
