

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034791.D
 Acq On : 21 Mar 2024 15:59
 Operator : SY/MD
 Sample : P1757-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	238109	250813	16.46%	2.293%
2	1.532	146	153	168	rVB	200871	235594	15.46%	2.154%
3	2.018	302	304	306	rBV	527	244	0.02%	0.002%
4	2.060	306	317	346	rVV	312242	457688	30.03%	4.184%
5	2.452	433	439	448	rVB6	1964	3001	0.20%	0.027%
6	2.809	547	550	553	rBV2	186	127	0.01%	0.001%
7	2.873	568	570	571	rBV	188	43	0.00%	0.000%
8	3.034	617	620	621	rBV	206	100	0.01%	0.001%
9	3.359	719	721	722	rBV	150	34	0.00%	0.000%
10	3.542	774	778	781	rBV2	231	181	0.01%	0.002%
11	3.687	820	823	827	rVB	309	216	0.01%	0.002%
12	3.789	847	855	908	rBV	98806	309099	20.28%	2.826%
13	4.249	982	998	1027	rBV	236184	603020	39.57%	5.513%
14	4.693	1134	1136	1139	rVB	351	135	0.01%	0.001%
15	4.744	1148	1152	1159	rBV3	273	398	0.03%	0.004%
16	4.812	1170	1173	1178	rVB4	393	305	0.02%	0.003%
17	4.838	1178	1181	1184	rBV2	290	214	0.01%	0.002%
18	4.883	1192	1195	1198	rBV3	276	198	0.01%	0.002%
19	4.957	1198	1218	1263	rBV2	572181	1524121	100.00%	13.934%
20	5.310	1327	1328	1330	rBV	295	146	0.01%	0.001%
21	5.346	1337	1339	1342	rVB2	665	349	0.02%	0.003%
22	5.394	1351	1354	1355	rBV2	435	235	0.02%	0.002%
23	5.532	1386	1397	1426	rBV	386784	813013	53.34%	7.433%
24	5.831	1481	1490	1507	rBV3	11403	26776	1.76%	0.245%
25	5.986	1526	1538	1565	rBV	323527	670015	43.96%	6.125%
26	6.384	1660	1662	1665	rVB2	179	77	0.01%	0.001%
27	6.410	1665	1670	1671	rBV	171	141	0.01%	0.001%
28	6.500	1694	1698	1699	rBV	262	156	0.01%	0.001%
29	6.548	1712	1713	1717	rVB2	188	100	0.01%	0.001%
30	6.593	1725	1727	1729	rBV	259	68	0.00%	0.001%
31	6.625	1735	1737	1740	rBV2	224	160	0.01%	0.001%
32	6.661	1746	1748	1750	rVB2	301	141	0.01%	0.001%
33	6.674	1750	1752	1753	rBV	215	67	0.00%	0.001%
34	6.735	1768	1771	1774	rBV2	323	180	0.01%	0.002%
35	6.780	1782	1785	1786	rBV	205	104	0.01%	0.001%
36	6.838	1802	1803	1806	rBV	185	66	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034791.D
 Acq On : 21 Mar 2024 15:59
 Operator : SY/MD
 Sample : P1757-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1859	rBV	175508	339320	22.26%	3.102%
38	7.243	1918	1929	1957	rBV	667434	1176953	77.22%	10.760%
39	7.551	2016	2025	2050	rBV	119529	222154	14.58%	2.031%
40	7.738	2079	2083	2084	rBV	424	309	0.02%	0.003%
41	7.850	2115	2118	2119	rBV	248	126	0.01%	0.001%
42	7.944	2144	2147	2149	rBV	178	116	0.01%	0.001%
43	7.969	2153	2155	2156	rBV	131	41	0.00%	0.000%
44	8.027	2163	2173	2221	rBV	312340	652452	42.81%	5.965%
45	8.358	2275	2276	2279	rBV2	564	245	0.02%	0.002%
46	8.542	2331	2333	2336	rBV	345	159	0.01%	0.001%
47	8.619	2353	2357	2358	rBV	240	152	0.01%	0.001%
48	8.719	2386	2388	2391	rBV2	238	155	0.01%	0.001%
49	8.783	2397	2408	2441	rBV	597925	998363	65.50%	9.127%
50	9.066	2492	2496	2498	rVB3	482	329	0.02%	0.003%
51	9.082	2498	2501	2503	rBV	214	140	0.01%	0.001%
52	9.143	2518	2520	2523	rVB	266	142	0.01%	0.001%
53	9.243	2547	2551	2553	rBV	246	192	0.01%	0.002%
54	9.336	2577	2580	2583	rBV	200	132	0.01%	0.001%
55	9.358	2585	2587	2590	rVV	198	88	0.01%	0.001%
56	9.506	2631	2633	2635	rVB2	242	77	0.01%	0.001%
57	9.551	2645	2647	2649	rVB	217	69	0.00%	0.001%
58	9.802	2722	2725	2728	rBV2	127	82	0.01%	0.001%
59	9.821	2728	2731	2733	rBV2	262	185	0.01%	0.002%
60	10.075	2808	2810	2811	rBV2	166	52	0.00%	0.000%
61	10.149	2822	2833	2861	rBV	406673	653663	42.89%	5.976%
62	10.307	2878	2882	2884	rBV2	322	269	0.02%	0.002%
63	10.323	2884	2887	2893	rVV2	674	643	0.04%	0.006%
64	10.805	3031	3037	3039	rBV	375	354	0.02%	0.003%
65	10.863	3053	3055	3060	rVB3	330	231	0.02%	0.002%
66	10.895	3060	3065	3068	rBV2	311	274	0.02%	0.003%
67	11.130	3130	3138	3144	rBV3	1609	2668	0.18%	0.024%
68	11.181	3144	3154	3186	rVV	578338	936443	61.44%	8.561%
69	11.487	3245	3249	3251	rBV	350	276	0.02%	0.003%
70	11.558	3259	3271	3301	rBV	641459	1045922	68.62%	9.562%
71	12.188	3462	3467	3469	rBV	861	683	0.04%	0.006%
72	12.371	3521	3524	3528	rBV2	469	336	0.02%	0.003%
73	12.796	3654	3656	3665	rBV2	385	388	0.03%	0.004%
74	12.866	3674	3678	3681	rBV2	553	447	0.03%	0.004%
75	13.152	3765	3767	3772	rBV	269	152	0.01%	0.001%
76	13.210	3779	3785	3793	rVB6	2402	3137	0.21%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034791.D
Acq On : 21 Mar 2024 15:59
Operator : SY/MD
Sample : P1757-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	13.275	3802	3805	3807	rBV2	384	218	0.01%	0.002%
78	13.516	3877	3880	3885	rBV3	286	285	0.02%	0.003%
79	13.680	3926	3931	3932	rBV2	746	574	0.04%	0.005%
80	13.976	4016	4023	4026	rBV2	856	1122	0.07%	0.010%
81	14.046	4044	4045	4047	rVB	398	101	0.01%	0.001%
82	14.169	4080	4083	4089	rBV4	740	795	0.05%	0.007%




Sum of corrected areas: 10938339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034791.D
Acq On : 21 Mar 2024 15:59
Operator : SY/MD
Sample : P1757-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

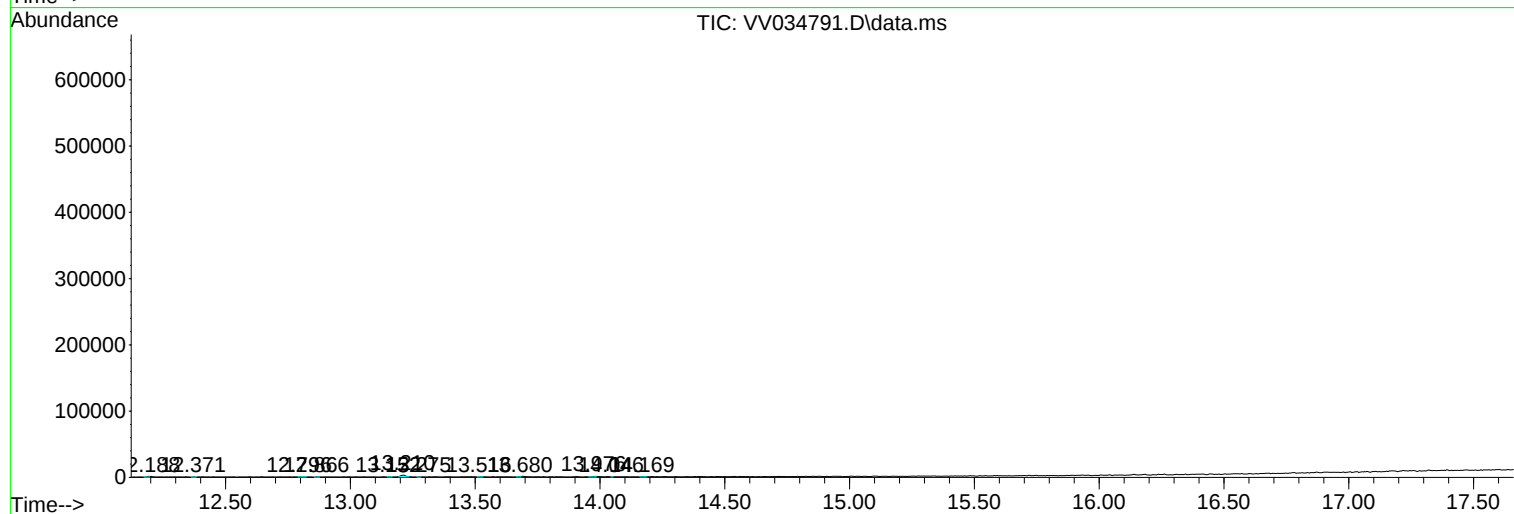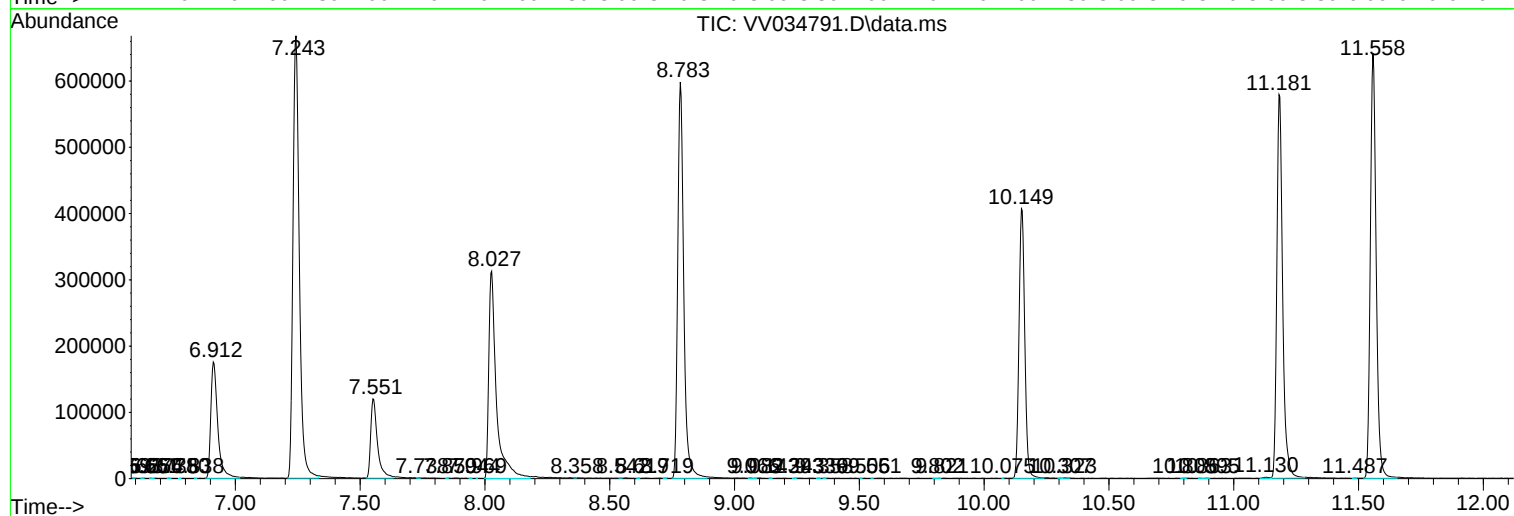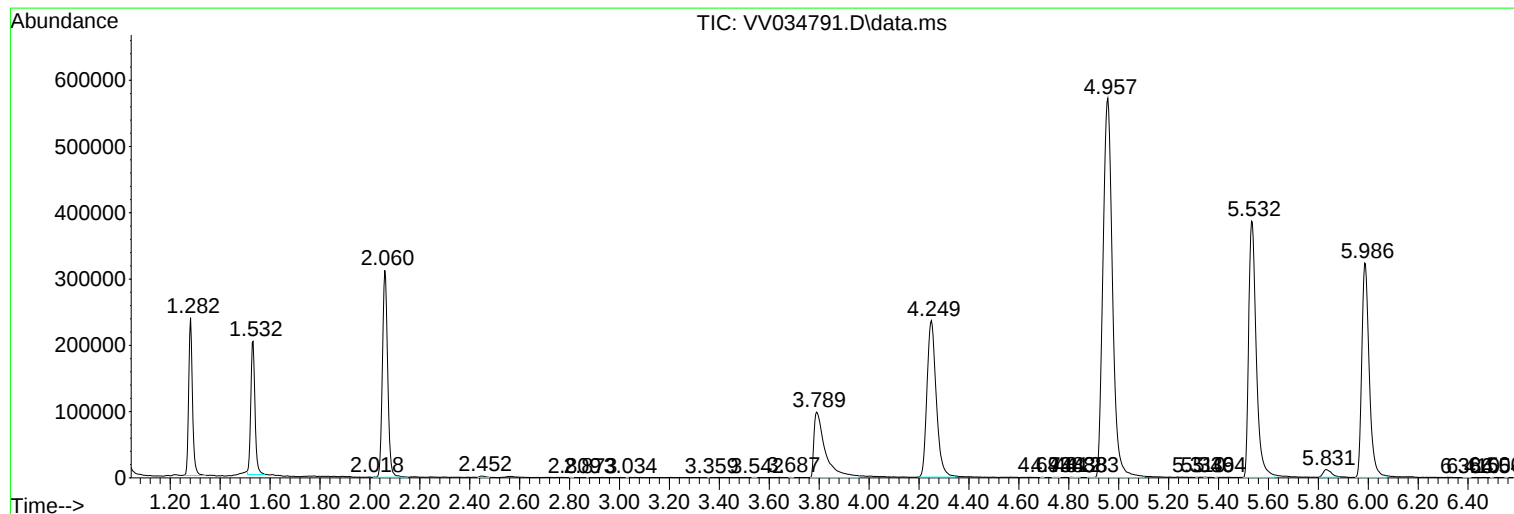

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034791.D
Acq On : 21 Mar 2024 15:59
Operator : SY/MD
Sample : P1757-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034791.D
Acq On : 21 Mar 2024 15:59
Operator : SY/MD
Sample : P1757-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------