

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034796.D
 Acq On : 21 Mar 2024 18:21
 Operator : SY/MD
 Sample : P1757-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	210409	224701	8.90%	2.156%
2	1.529	146	152	172	rVB	184469	217504	8.61%	2.087%
3	2.060	306	317	332	rBV	238345	347454	13.76%	3.334%
4	2.185	353	356	364	rBV2	329	345	0.01%	0.003%
5	2.384	415	418	419	rBV2	282	144	0.01%	0.001%
6	2.452	431	439	446	rVB2	2120	2870	0.11%	0.028%
7	2.651	498	501	505	rBV2	182	183	0.01%	0.002%
8	2.699	508	516	519	rBV2	420	576	0.02%	0.006%
9	2.741	524	529	533	rBV2	237	267	0.01%	0.003%
10	2.777	533	540	543	rVB2	186	195	0.01%	0.002%
11	2.802	543	548	551	rBV2	150	185	0.01%	0.002%
12	2.847	559	562	565	rVB2	191	130	0.01%	0.001%
13	2.973	596	601	609	rBV2	365	500	0.02%	0.005%
14	3.043	619	623	627	rBV2	230	237	0.01%	0.002%
15	3.066	627	630	632	rBV2	186	129	0.01%	0.001%
16	3.127	647	649	656	rVB2	289	232	0.01%	0.002%
17	3.162	656	660	664	rBV2	196	191	0.01%	0.002%
18	3.320	704	709	711	rBV2	146	121	0.00%	0.001%
19	3.352	715	719	721	rBV2	184	122	0.00%	0.001%
20	3.388	725	730	733	rBV2	177	172	0.01%	0.002%
21	3.468	749	755	758	rBV	225	141	0.01%	0.001%
22	3.490	758	762	770	rVV2	180	178	0.01%	0.002%
23	3.580	786	790	796	rVB2	238	304	0.01%	0.003%
24	3.642	806	809	812	rBV	289	176	0.01%	0.002%
25	3.664	813	816	819	rBV2	153	119	0.00%	0.001%
26	3.738	836	839	843	rBV2	132	136	0.01%	0.001%
27	3.789	847	855	886	rBV	64030	181023	7.17%	1.737%
28	4.246	981	997	1029	rBV	158237	402654	15.94%	3.863%
29	4.587	1100	1103	1105	rBV	264	211	0.01%	0.002%
30	4.622	1112	1114	1117	rVB2	266	123	0.00%	0.001%
31	4.645	1117	1121	1124	rVB3	407	294	0.01%	0.003%
32	4.677	1124	1131	1133	rBV	113	113	0.00%	0.001%
33	4.709	1136	1141	1142	rBV	297	217	0.01%	0.002%
34	4.757	1153	1156	1161	rBV2	121	124	0.00%	0.001%
35	4.850	1182	1185	1189	rVB	215	128	0.01%	0.001%
36	4.895	1194	1199	1202	rBV3	314	312	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034796.D
 Acq On : 21 Mar 2024 18:21
 Operator : SY/MD
 Sample : P1757-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1228	rBV2	370592	964261	38.18%	9.251%
38	5.313	1326	1329	1331	rBV2	304	218	0.01%	0.002%
39	5.358	1340	1343	1346	rBV2	352	264	0.01%	0.003%
40	5.449	1364	1371	1375	rVB2	264	233	0.01%	0.002%
41	5.481	1377	1381	1383	rBV2	371	246	0.01%	0.002%
42	5.532	1387	1397	1428	rBV	266102	550669	21.80%	5.283%
43	5.834	1481	1491	1504	rBV4	7532	16656	0.66%	0.160%
44	5.985	1526	1538	1568	rBV2	200306	416890	16.51%	4.000%
45	6.278	1626	1629	1634	rVB	223	148	0.01%	0.001%
46	6.320	1639	1642	1644	rBV	198	124	0.00%	0.001%
47	6.403	1665	1668	1671	rBV	195	134	0.01%	0.001%
48	6.616	1729	1734	1737	rVB	202	196	0.01%	0.002%
49	6.757	1775	1778	1779	rBV2	232	111	0.00%	0.001%
50	6.911	1816	1826	1853	rBV	117579	222735	8.82%	2.137%
51	7.185	1907	1911	1913	rBV4	483	460	0.02%	0.004%
52	7.243	1918	1929	1972	rVV	444121	785217	31.09%	7.534%
53	7.555	2014	2026	2054	rBV	80042	149756	5.93%	1.437%
54	7.754	2085	2088	2090	rBV2	472	235	0.01%	0.002%
55	7.821	2105	2109	2112	rVB2	213	188	0.01%	0.002%
56	7.847	2112	2117	2119	rBV	251	182	0.01%	0.002%
57	7.918	2134	2139	2141	rBV	581	403	0.02%	0.004%
58	8.024	2163	2172	2211	rBV	211506	418254	16.56%	4.013%
59	8.284	2252	2253	2255	rBV	253	126	0.00%	0.001%
60	8.436	2296	2300	2303	rVB2	297	211	0.01%	0.002%
61	8.458	2303	2307	2309	rBV2	208	153	0.01%	0.001%
62	8.487	2314	2316	2318	rBV	393	196	0.01%	0.002%
63	8.577	2343	2344	2348	rVB	325	129	0.01%	0.001%
64	8.600	2348	2351	2354	rVB2	175	126	0.00%	0.001%
65	8.616	2354	2356	2359	rBV2	187	143	0.01%	0.001%
66	8.651	2364	2367	2368	rBV	275	113	0.00%	0.001%
67	8.718	2386	2388	2389	rBV	222	109	0.00%	0.001%
68	8.812	2398	2417	2440	rBV2	1160799	2525501	100.00%	24.230%
69	9.101	2500	2507	2509	rBV4	669	804	0.03%	0.008%
70	9.294	2564	2567	2568	rBV	288	128	0.01%	0.001%
71	9.481	2622	2625	2626	rBV2	465	236	0.01%	0.002%
72	9.532	2638	2641	2647	rVV5	484	440	0.02%	0.004%
73	9.583	2654	2657	2662	rVB2	386	254	0.01%	0.002%
74	9.628	2669	2671	2672	rBV2	260	109	0.00%	0.001%
75	9.741	2703	2706	2709	rBV	279	177	0.01%	0.002%
76	9.799	2721	2724	2726	rBV	173	135	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034796.D
 Acq On : 21 Mar 2024 18:21
 Operator : SY/MD
 Sample : P1757-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.873	2742	2747	2750	rBV3	494	570	0.02%	0.005%
78	9.908	2756	2758	2760	rBV	218	126	0.00%	0.001%
79	9.950	2766	2771	2774	rBV	274	278	0.01%	0.003%
80	10.001	2781	2787	2789	rBV2	214	216	0.01%	0.002%
81	10.149	2822	2833	2852	rBV	287202	457862	18.13%	4.393%
82	10.316	2882	2885	2887	rBV2	528	389	0.02%	0.004%
83	10.455	2925	2928	2930	rBV	187	132	0.01%	0.001%
84	10.667	2990	2994	2996	rBV	176	141	0.01%	0.001%
85	10.734	3012	3015	3017	rBV2	229	124	0.00%	0.001%
86	10.802	3034	3036	3038	rBV2	209	145	0.01%	0.001%
87	10.860	3049	3054	3055	rBV	719	605	0.02%	0.006%
88	11.014	3100	3102	3105	rBV2	187	144	0.01%	0.001%
89	11.072	3113	3120	3122	rBV	260	373	0.01%	0.004%
90	11.120	3126	3135	3145	rBV2	42794	67253	2.66%	0.645%
91	11.185	3145	3155	3185	rVB2	477544	1165855	46.16%	11.185%
92	11.561	3259	3272	3297	rBV3	554213	1200394	47.53%	11.517%
93	11.767	3334	3336	3337	rBV	237	116	0.00%	0.001%
94	12.046	3419	3423	3425	rBV	221	192	0.01%	0.002%
95	12.114	3435	3444	3446	rBV2	253	330	0.01%	0.003%
96	12.130	3447	3449	3453	rBV2	229	169	0.01%	0.002%
97	12.587	3585	3591	3603	rVB5	2288	3679	0.15%	0.035%
98	13.204	3774	3783	3796	rBV2	15376	23770	0.94%	0.228%
99	13.445	3850	3858	3873	rBV	23067	38966	1.54%	0.374%
100	13.683	3923	3932	3946	rBV3	14244	21953	0.87%	0.211%




Sum of corrected areas: 10422963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034796.D
Acq On : 21 Mar 2024 18:21
Operator : SY/MD
Sample : P1757-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

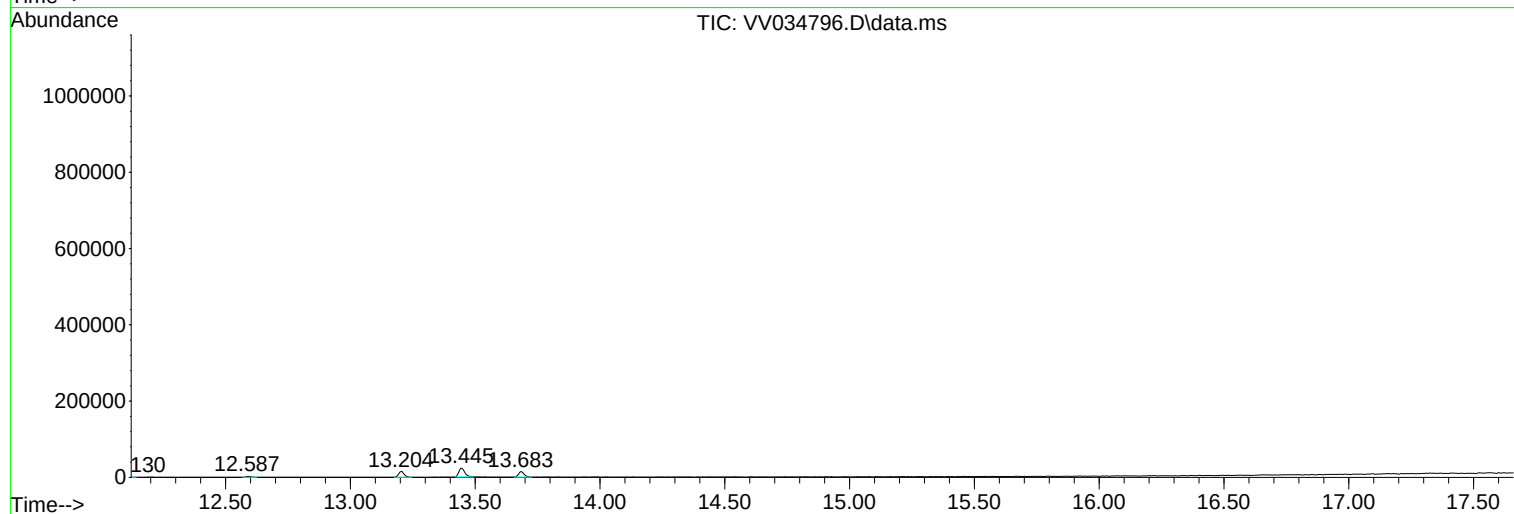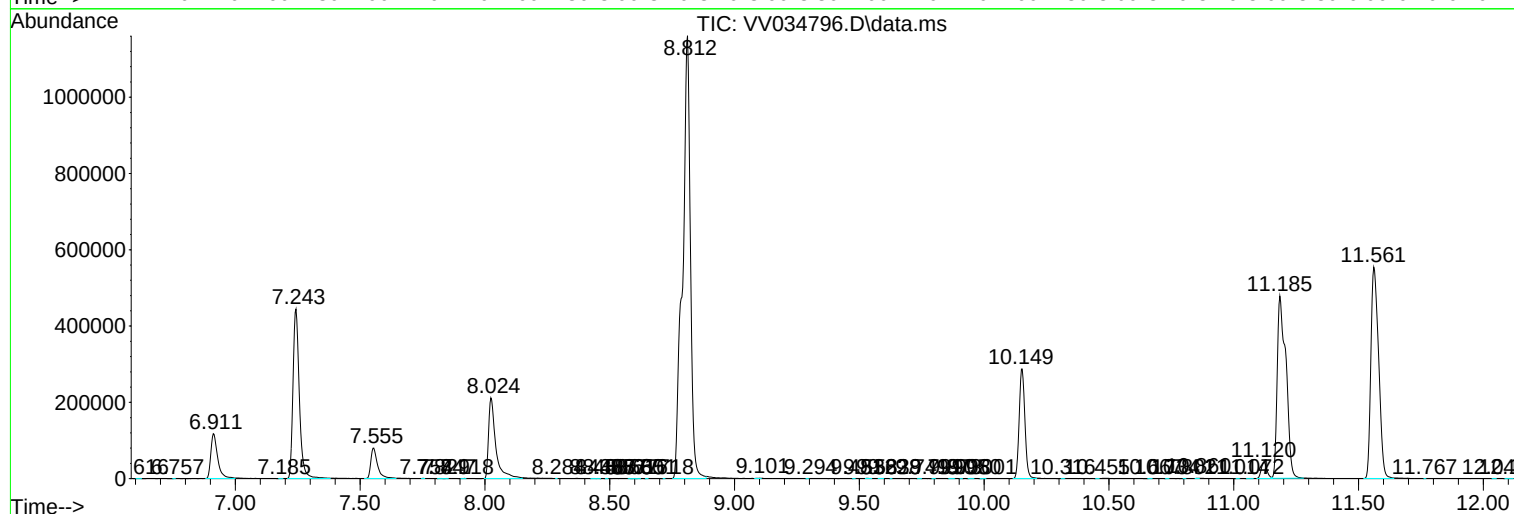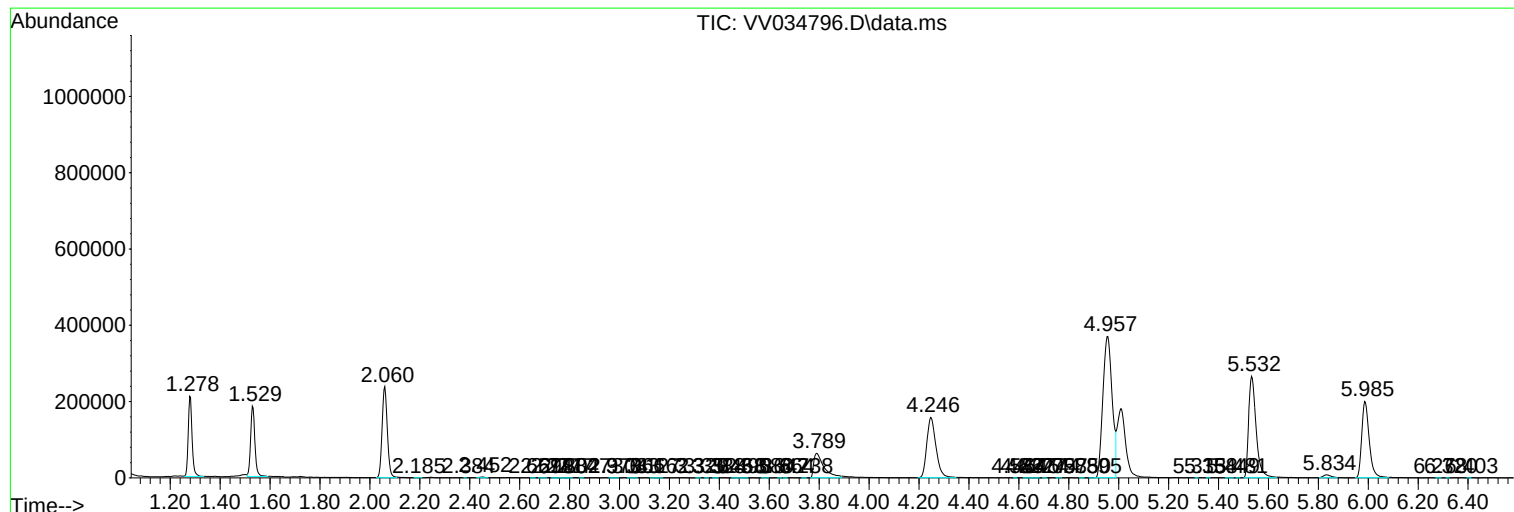

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034796.D
Acq On : 21 Mar 2024 18:21
Operator : SY/MD
Sample : P1757-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034796.D
Acq On : 21 Mar 2024 18:21
Operator : SY/MD
Sample : P1757-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------