

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034797.D
 Acq On : 21 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1757-04DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	208963	222258	14.22%	1.926%
2	1.532	146	153	170	rVB	190383	220819	14.13%	1.914%
3	2.060	306	317	335	rBV	282569	411328	26.32%	3.565%
4	2.381	414	417	420	rBV	441	315	0.02%	0.003%
5	2.449	431	438	451	rVB3	2725	4972	0.32%	0.043%
6	2.552	465	470	471	rBV	689	495	0.03%	0.004%
7	2.693	512	514	516	rVB	340	109	0.01%	0.001%
8	2.709	516	519	521	rBV2	486	316	0.02%	0.003%
9	2.780	539	541	543	rBV2	312	142	0.01%	0.001%
10	2.844	558	561	563	rBV	175	100	0.01%	0.001%
11	2.873	567	570	571	rBV	180	106	0.01%	0.001%
12	2.928	584	587	589	rBV2	317	175	0.01%	0.002%
13	3.002	607	610	612	rBV2	153	96	0.01%	0.001%
14	3.047	619	624	628	rVB2	257	277	0.02%	0.002%
15	3.095	637	639	640	rBV	253	73	0.00%	0.001%
16	3.147	651	655	659	rBV2	221	195	0.01%	0.002%
17	3.211	671	675	680	rBV2	186	125	0.01%	0.001%
18	3.285	696	698	701	rBV	219	136	0.01%	0.001%
19	3.304	701	704	706	rBV	156	107	0.01%	0.001%
20	3.368	721	724	726	rBV	156	111	0.01%	0.001%
21	3.449	746	749	753	rBV	144	126	0.01%	0.001%
22	3.648	808	811	815	rVB3	269	183	0.01%	0.002%
23	3.667	815	817	818	rBV3	167	82	0.01%	0.001%
24	3.674	818	819	825	rVB	374	223	0.01%	0.002%
25	3.712	829	831	834	rVB	234	111	0.01%	0.001%
26	3.732	834	837	841	rBV	282	263	0.02%	0.002%
27	3.790	846	855	910	rBV	103496	317372	20.31%	2.751%
28	4.246	982	997	1025	rBV	221521	570944	36.54%	4.948%
29	4.561	1093	1095	1098	rBV	340	222	0.01%	0.002%
30	4.674	1127	1130	1132	rBV2	305	242	0.02%	0.002%
31	4.728	1144	1147	1148	rBV	405	200	0.01%	0.002%
32	4.764	1155	1158	1159	rBV	271	131	0.01%	0.001%
33	4.854	1180	1186	1191	rVB3	314	427	0.03%	0.004%
34	4.954	1201	1217	1263	rBV2	536315	1562600	100.00%	13.543%
35	5.265	1312	1314	1320	rVB4	494	367	0.02%	0.003%
36	5.333	1333	1335	1336	rBV2	290	145	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034797.D
 Acq On : 21 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1757-04DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.465	1374	1376	1377	rBV2	404	147	0.01%	0.001%
38	5.532	1386	1397	1433	rBV	372471	768110	49.16%	6.657%
39	5.831	1480	1490	1505	rBV5	10407	25020	1.60%	0.217%
40	5.986	1525	1538	1565	rBV	298244	624737	39.98%	5.415%
41	6.236	1615	1616	1618	rBV	300	125	0.01%	0.001%
42	6.256	1618	1622	1626	rVB3	366	371	0.02%	0.003%
43	6.285	1626	1631	1637	rBV4	350	435	0.03%	0.004%
44	6.368	1655	1657	1661	rVB2	361	179	0.01%	0.002%
45	6.388	1661	1663	1665	rBV	144	83	0.01%	0.001%
46	6.449	1680	1682	1686	rVB	357	172	0.01%	0.001%
47	6.500	1696	1698	1702	rVB	267	153	0.01%	0.001%
48	6.568	1718	1719	1721	rVB	225	83	0.01%	0.001%
49	6.632	1736	1739	1741	rVB2	175	97	0.01%	0.001%
50	6.651	1741	1745	1747	rBV	106	86	0.01%	0.001%
51	6.735	1769	1771	1774	rBV2	151	101	0.01%	0.001%
52	6.912	1814	1826	1856	rBV	166334	319358	20.44%	2.768%
53	7.243	1917	1929	1955	rBV	612446	1085536	69.47%	9.409%
54	7.551	2016	2025	2054	rBV	113497	210971	13.50%	1.829%
55	7.863	2118	2122	2123	rBV2	277	169	0.01%	0.001%
56	7.908	2133	2136	2138	rBV2	316	190	0.01%	0.002%
57	7.941	2143	2146	2148	rVB	206	87	0.01%	0.001%
58	7.982	2156	2159	2161	rBV2	302	186	0.01%	0.002%
59	8.024	2163	2172	2214	rBV	325048	650708	41.64%	5.640%
60	8.545	2331	2334	2337	rBV2	434	400	0.03%	0.003%
61	8.584	2344	2346	2347	rBV	288	140	0.01%	0.001%
62	8.625	2355	2359	2361	rBV3	191	113	0.01%	0.001%
63	8.786	2396	2409	2411	rBV	623510	830304	53.14%	7.196%
64	9.085	2498	2502	2504	rBV3	685	494	0.03%	0.004%
65	9.265	2555	2558	2560	rBV	242	143	0.01%	0.001%
66	9.320	2573	2575	2577	rVB	270	92	0.01%	0.001%
67	9.413	2601	2604	2607	rBV	214	98	0.01%	0.001%
68	9.474	2619	2623	2624	rBV2	170	125	0.01%	0.001%
69	9.487	2624	2627	2632	rBV2	461	504	0.03%	0.004%
70	9.574	2652	2654	2658	rVB	369	148	0.01%	0.001%
71	9.850	2736	2740	2742	rBV	222	159	0.01%	0.001%
72	10.111	2816	2821	2822	rBV	238	165	0.01%	0.001%
73	10.153	2822	2834	2858	rVV	404246	641636	41.06%	5.561%
74	10.310	2881	2883	2885	rBV	363	190	0.01%	0.002%
75	10.323	2885	2887	2895	rVB3	887	759	0.05%	0.007%
76	10.423	2915	2918	2921	rVB2	349	206	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034797.D
 Acq On : 21 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1757-04DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.445	2922	2925	2927	rBV	204	134	0.01%	0.001%
78	10.484	2931	2937	2944	rVV4	926	1135	0.07%	0.010%
79	10.538	2951	2954	2957	rBV	232	177	0.01%	0.002%
80	10.574	2962	2965	2967	rBV	160	89	0.01%	0.001%
81	10.648	2987	2988	2993	rBV2	168	102	0.01%	0.001%
82	10.715	3005	3009	3011	rBV2	224	179	0.01%	0.002%
83	10.741	3015	3017	3020	rBV	216	152	0.01%	0.001%
84	10.854	3050	3052	3053	rBV	381	115	0.01%	0.001%
85	11.124	3127	3136	3145	rBV4	24505	40697	2.60%	0.353%
86	11.185	3145	3155	3185	rVB2	612388	1411532	90.33%	12.234%
87	11.561	3259	3272	3298	rBV2	713404	1557124	99.65%	13.496%
88	11.792	3342	3344	3347	rVB	350	108	0.01%	0.001%
89	12.085	3434	3435	3444	rVB2	198	181	0.01%	0.002%
90	12.413	3534	3537	3539	rBV2	219	138	0.01%	0.001%
91	12.715	3628	3631	3638	rBV2	317	338	0.02%	0.003%
92	12.786	3649	3653	3656	rBV	265	236	0.02%	0.002%
93	13.143	3762	3764	3769	rBV	236	207	0.01%	0.002%
94	13.204	3774	3783	3794	rBV3	12289	19282	1.23%	0.167%
95	13.333	3821	3823	3826	rBV3	357	218	0.01%	0.002%
96	13.374	3835	3836	3838	rBV2	305	126	0.01%	0.001%
97	13.448	3852	3859	3871	rBV2	9769	15125	0.97%	0.131%
98	13.532	3884	3885	3888	rBV2	285	191	0.01%	0.002%
99	13.577	3895	3899	3901	rBV	360	292	0.02%	0.003%
100	13.686	3924	3933	3944	rBV3	6641	11188	0.72%	0.097%




Sum of corrected areas: 11537739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034797.D
Acq On : 21 Mar 2024 18:45
Operator : SY/MD
Sample : P1757-04DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

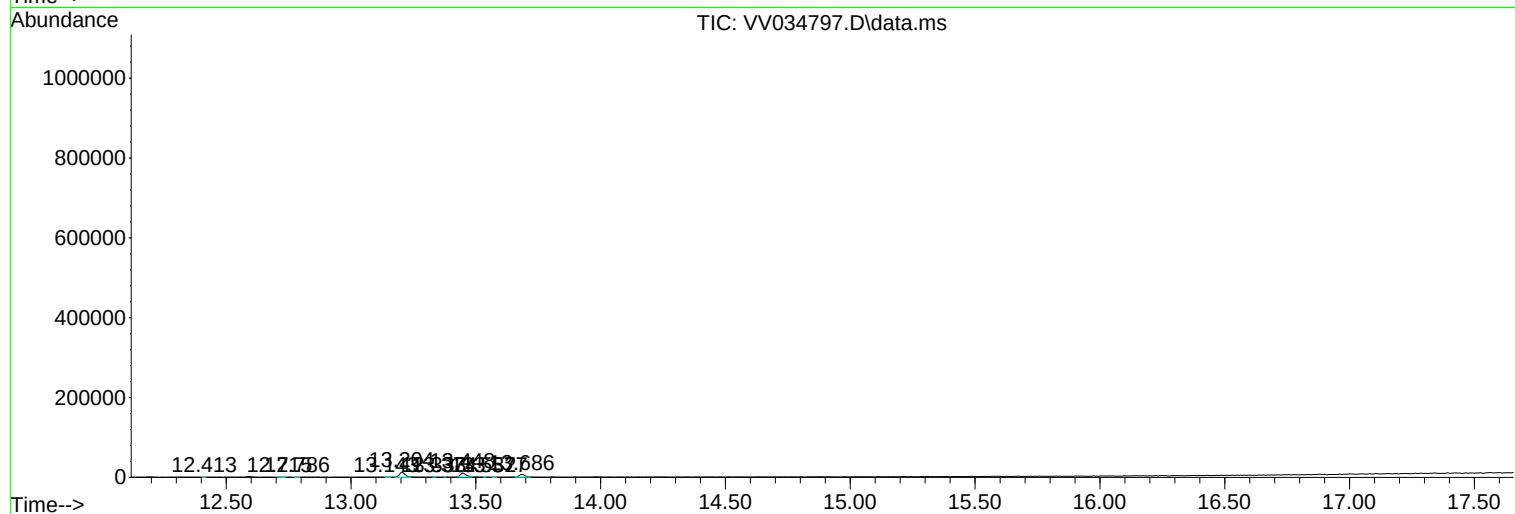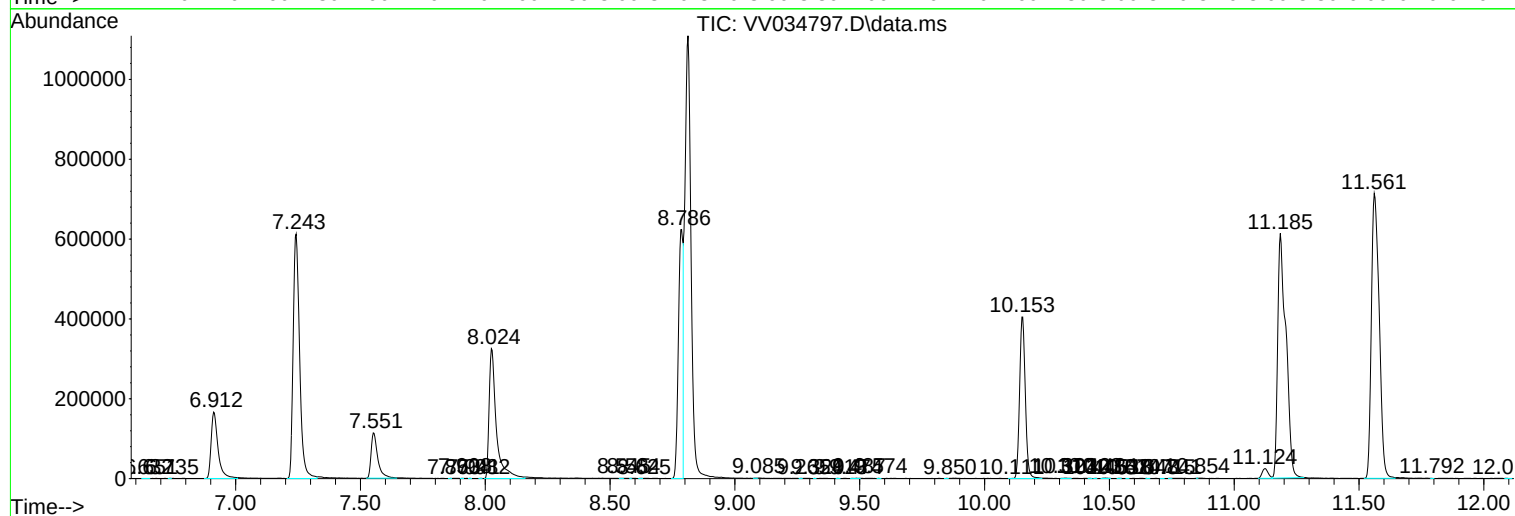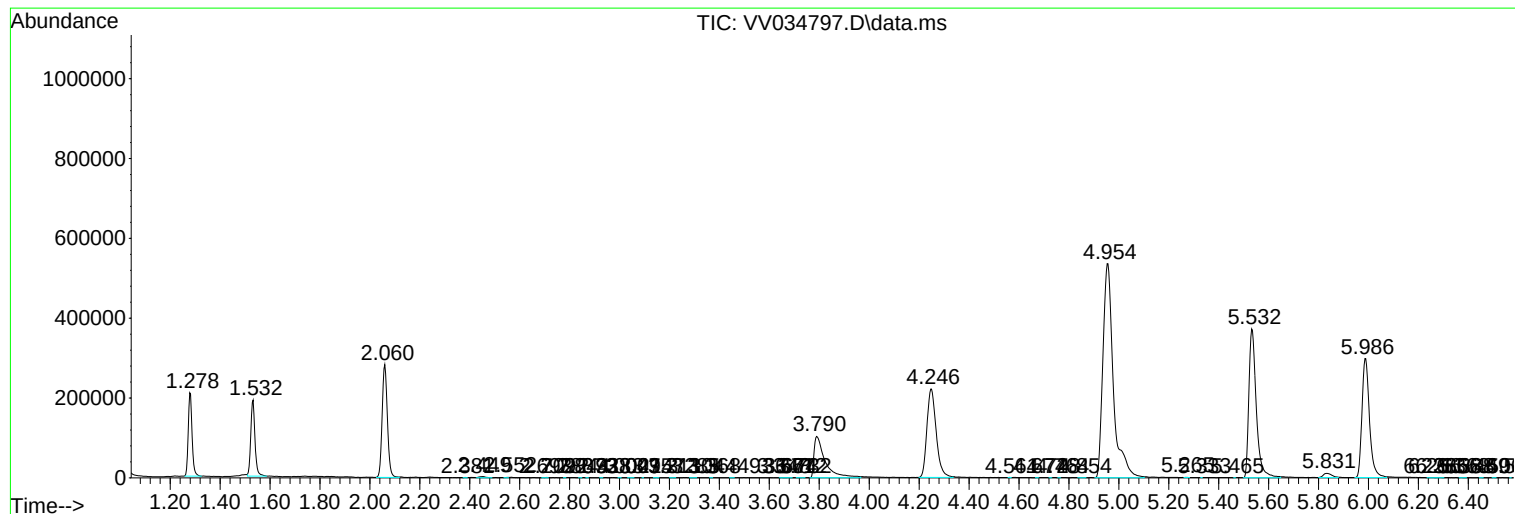

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034797.D
Acq On : 21 Mar 2024 18:45
Operator : SY/MD
Sample : P1757-04DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034797.D
Acq On : 21 Mar 2024 18:45
Operator : SY/MD
Sample : P1757-04DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc