

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034798.D
 Acq On : 21 Mar 2024 19:09
 Operator : SY/MD
 Sample : P1757-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	165124	175088	7.52%	1.492%
2	1.529	146	152	184	rVB	163239	203766	8.76%	1.737%
3	2.056	306	316	331	rBV	226828	335003	14.40%	2.855%
4	2.445	429	437	447	rVB4	4074	6572	0.28%	0.056%
5	2.552	462	470	472	rBV4	2011	2129	0.09%	0.018%
6	2.600	483	485	488	rVB	295	98	0.00%	0.001%
7	2.703	511	517	519	rBV4	1232	1272	0.05%	0.011%
8	2.838	557	559	560	rBV4	203	74	0.00%	0.001%
9	2.944	590	592	597	rVB2	246	123	0.01%	0.001%
10	2.976	600	602	604	rVB2	217	79	0.00%	0.001%
11	3.011	611	613	619	rBV2	155	112	0.00%	0.001%
12	3.114	639	645	650	rBV2	357	405	0.02%	0.003%
13	3.140	650	653	656	rBV2	270	215	0.01%	0.002%
14	3.204	670	673	677	rBV2	169	151	0.01%	0.001%
15	3.227	677	680	685	rVV	224	195	0.01%	0.002%
16	3.246	685	686	691	rVB	275	150	0.01%	0.001%
17	3.278	691	696	698	rBV	143	144	0.01%	0.001%
18	3.442	746	747	750	rVB	238	73	0.00%	0.001%
19	3.474	750	757	763	rBV	229	344	0.01%	0.003%
20	3.529	771	774	777	rVB2	270	140	0.01%	0.001%
21	3.670	813	818	822	rVB3	358	366	0.02%	0.003%
22	3.706	822	829	831	rBV2	130	149	0.01%	0.001%
23	3.754	840	844	847	rBV	198	140	0.01%	0.001%
24	3.789	847	855	904	rBV	100470	305144	13.11%	2.601%
25	4.249	983	998	1022	rBV	189791	488498	20.99%	4.164%
26	4.683	1130	1133	1138	rVB	345	268	0.01%	0.002%
27	4.780	1160	1163	1166	rBV2	250	157	0.01%	0.001%
28	4.867	1187	1190	1194	rBV3	259	236	0.01%	0.002%
29	4.953	1201	1217	1267	rBV2	466383	1294284	55.62%	11.032%
30	5.336	1332	1336	1340	rBV2	503	385	0.02%	0.003%
31	5.410	1355	1359	1360	rBV	308	227	0.01%	0.002%
32	5.445	1366	1370	1374	rBV3	324	258	0.01%	0.002%
33	5.477	1378	1380	1381	rVV3	186	74	0.00%	0.001%
34	5.532	1386	1397	1428	rBV	305493	636736	27.36%	5.427%
35	5.834	1480	1491	1511	rBV3	10742	23717	1.02%	0.202%
36	5.985	1525	1538	1568	rBV	266355	556012	23.89%	4.739%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034798.D
 Acq On : 21 Mar 2024 19:09
 Operator : SY/MD
 Sample : P1757-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COB80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.217	1605	1610	1611	rBV3	459	362	0.02%	0.003%
38	6.323	1640	1643	1646	rBV	142	95	0.00%	0.001%
39	6.339	1646	1648	1650	rBV	272	133	0.01%	0.001%
40	6.638	1734	1741	1744	rBV	315	319	0.01%	0.003%
41	6.657	1745	1747	1752	rVB2	165	84	0.00%	0.001%
42	6.683	1752	1755	1757	rBV2	234	169	0.01%	0.001%
43	6.754	1774	1777	1779	rVB2	270	131	0.01%	0.001%
44	6.773	1780	1783	1789	rVB2	323	232	0.01%	0.002%
45	6.802	1789	1792	1796	rBV2	146	135	0.01%	0.001%
46	6.911	1811	1826	1851	rBV	144453	279006	11.99%	2.378%
47	7.149	1895	1900	1902	rBV	247	251	0.01%	0.002%
48	7.178	1905	1909	1910	rBV2	669	432	0.02%	0.004%
49	7.243	1917	1929	1971	rBV	537467	950950	40.87%	8.105%
50	7.555	2017	2026	2047	rBV	100727	183768	7.90%	1.566%
51	7.776	2092	2095	2099	rBV6	453	382	0.02%	0.003%
52	7.844	2112	2116	2119	rVB3	316	246	0.01%	0.002%
53	7.860	2119	2121	2123	rBV	359	171	0.01%	0.001%
54	7.918	2132	2139	2144	rBV4	1174	1600	0.07%	0.014%
55	7.950	2146	2149	2150	rBV2	218	116	0.00%	0.001%
56	8.027	2164	2173	2215	rBV	305764	618464	26.58%	5.271%
57	8.362	2275	2277	2278	rBV	761	308	0.01%	0.003%
58	8.535	2330	2331	2333	rBV	322	102	0.00%	0.001%
59	8.606	2350	2353	2355	rBV2	172	98	0.00%	0.001%
60	8.677	2371	2375	2376	rBV2	283	214	0.01%	0.002%
61	8.712	2384	2386	2389	rBV	342	253	0.01%	0.002%
62	8.786	2397	2409	2410	rBV	547783	616079	26.48%	5.251%
63	9.162	2523	2526	2533	rBV2	399	405	0.02%	0.003%
64	9.294	2564	2567	2570	rBV2	380	221	0.01%	0.002%
65	9.336	2578	2580	2584	rVB2	268	141	0.01%	0.001%
66	9.355	2584	2586	2589	rBV	218	162	0.01%	0.001%
67	9.590	2656	2659	2664	rBV3	339	274	0.01%	0.002%
68	9.661	2678	2681	2685	rVB3	323	213	0.01%	0.002%
69	9.699	2690	2693	2698	rBV	216	232	0.01%	0.002%
70	9.741	2703	2706	2709	rBV2	214	210	0.01%	0.002%
71	9.789	2717	2721	2724	rBV	268	215	0.01%	0.002%
72	9.879	2740	2749	2759	rBV2	1143	1986	0.09%	0.017%
73	10.027	2792	2795	2798	rVB2	265	125	0.01%	0.001%
74	10.152	2821	2834	2858	rBV	372687	590562	25.38%	5.034%
75	10.297	2877	2879	2881	rBV	338	113	0.00%	0.001%
76	10.355	2894	2897	2898	rBV2	221	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034798.D
 Acq On : 21 Mar 2024 19:09
 Operator : SY/MD
 Sample : P1757-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.699	3002	3004	3005	rBV	316	128	0.01%	0.001%
78	10.754	3019	3021	3024	rVB	233	94	0.00%	0.001%
79	10.995	3094	3096	3099	rBV2	233	95	0.00%	0.001%
80	11.062	3113	3117	3118	rBV	262	145	0.01%	0.001%
81	11.120	3125	3135	3145	rBV	69727	110424	4.75%	0.941%
82	11.207	3145	3162	3185	rVB2	743999	1848694	79.45%	15.757%
83	11.574	3256	3276	3303	rBV2	1072403	2327002	100.00%	19.834%
84	11.963	3395	3397	3399	rVB	269	110	0.00%	0.001%
85	12.111	3438	3443	3444	rBV	361	255	0.01%	0.002%
86	12.146	3451	3454	3457	rBV2	217	149	0.01%	0.001%
87	12.464	3550	3553	3557	rBV2	257	154	0.01%	0.001%
88	12.590	3585	3592	3602	rBV6	1859	2998	0.13%	0.026%
89	12.686	3618	3622	3625	rBV2	402	325	0.01%	0.003%
90	12.731	3633	3636	3638	rBV2	311	158	0.01%	0.001%
91	12.828	3664	3666	3667	rBV	289	105	0.00%	0.001%
92	12.892	3684	3686	3688	rBV	291	177	0.01%	0.002%
93	12.956	3703	3706	3707	rBV2	297	156	0.01%	0.001%
94	12.985	3711	3715	3716	rBV	229	173	0.01%	0.001%
95	13.201	3772	3782	3799	rBV	76044	120580	5.18%	1.028%
96	13.448	3853	3859	3873	rVB2	5919	9095	0.39%	0.078%
97	13.603	3905	3907	3915	rBV2	420	374	0.02%	0.003%
98	13.683	3924	3932	3944	rVB3	18499	28442	1.22%	0.242%
99	13.966	4017	4020	4021	rBV2	563	320	0.01%	0.003%
100	15.107	4373	4375	4378	rBV3	875	332	0.01%	0.003%




Sum of corrected areas: 11732367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034798.D
Acq On : 21 Mar 2024 19:09
Operator : SY/MD
Sample : P1757-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

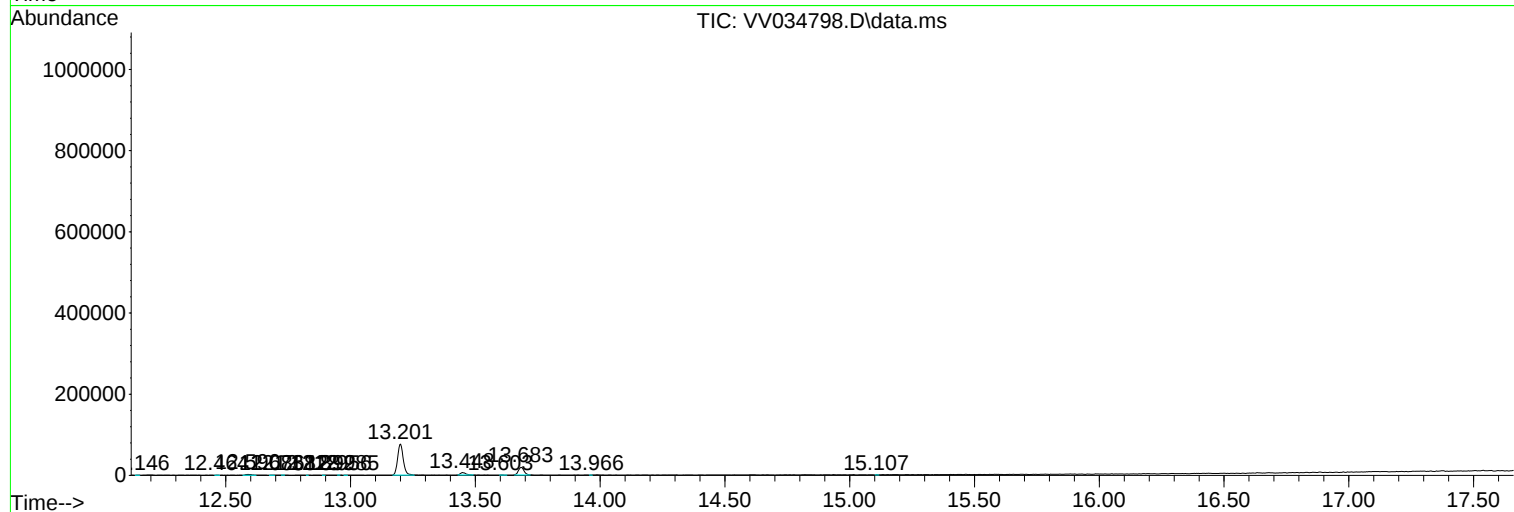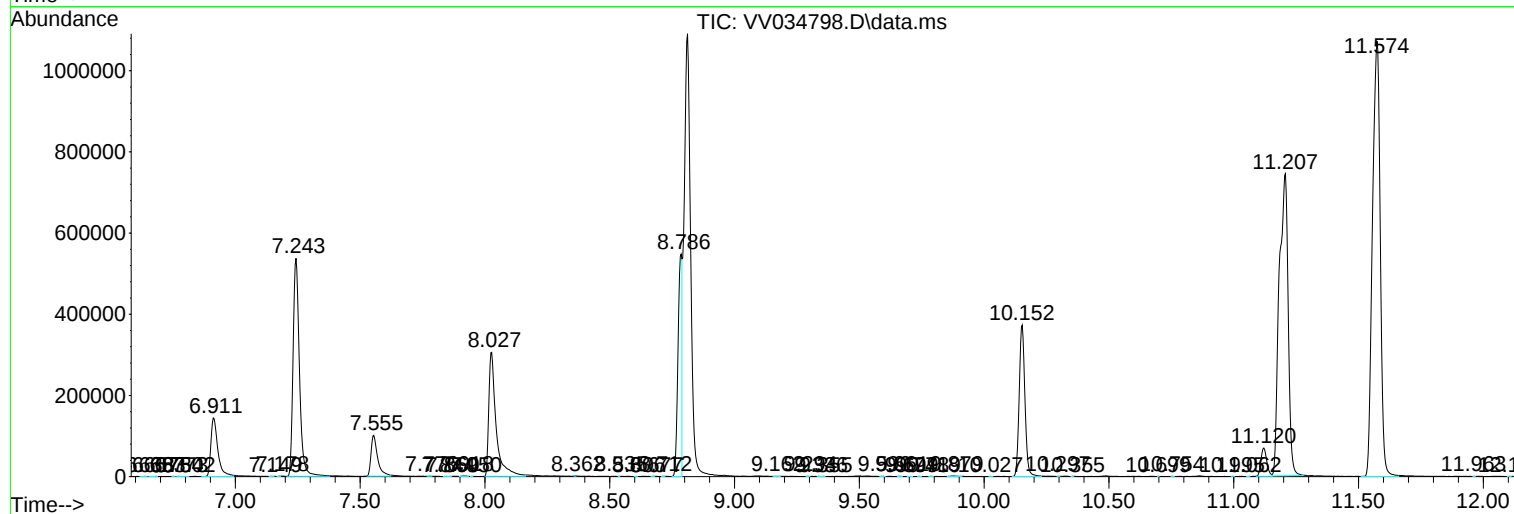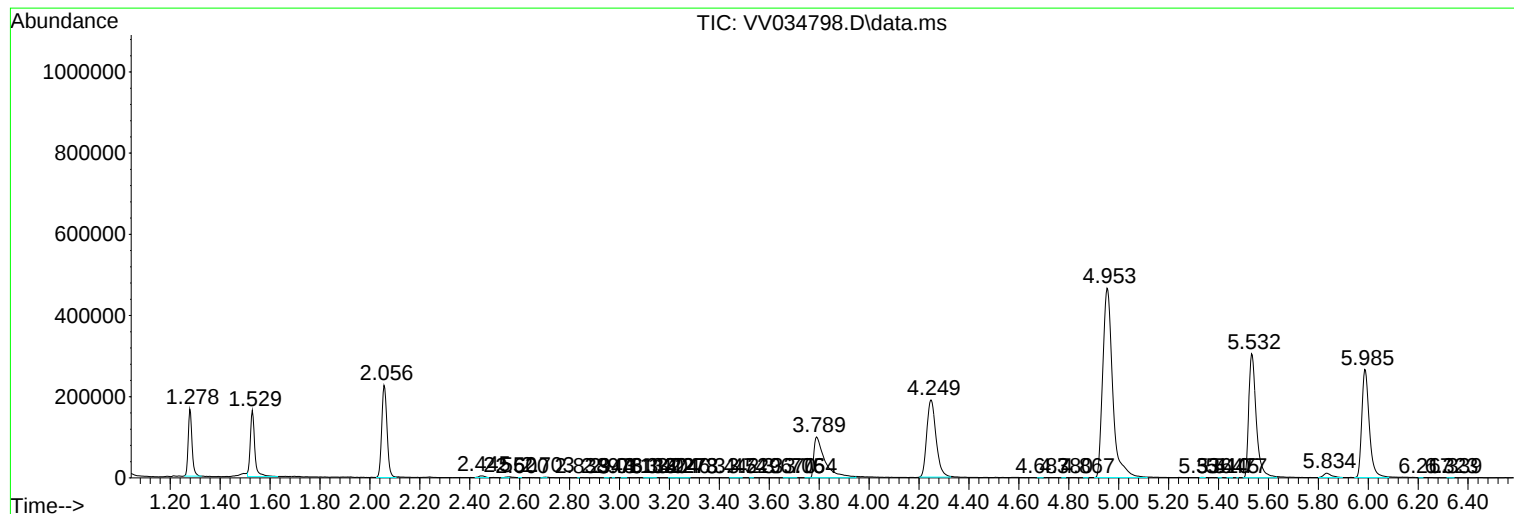

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034798.D
Acq On : 21 Mar 2024 19:09
Operator : SY/MD
Sample : P1757-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034798.D
Acq On : 21 Mar 2024 19:09
Operator : SY/MD
Sample : P1757-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc