

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034799.D
 Acq On : 21 Mar 2024 19:33
 Operator : SY/MD
 Sample : P1757-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034799.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	196333	212352	7.16%	1.457%
2	1.529	145	152	167	rVB	182377	210390	7.10%	1.444%
3	2.060	305	317	333	rBV	255915	376833	12.71%	2.586%
4	2.117	333	335	338	rVB3	1180	715	0.02%	0.005%
5	2.162	347	349	353	rBV3	491	275	0.01%	0.002%
6	2.243	369	374	376	rBV3	668	622	0.02%	0.004%
7	2.449	432	438	446	rVB3	2569	3840	0.13%	0.026%
8	2.494	449	452	454	rBV	361	202	0.01%	0.001%
9	2.558	463	472	484	rBV3	1487	2537	0.09%	0.017%
10	2.709	514	519	522	rBV3	655	671	0.02%	0.005%
11	2.931	584	588	591	rBV2	317	252	0.01%	0.002%
12	3.008	607	612	617	rBV2	303	407	0.01%	0.003%
13	3.098	636	640	644	rBV2	325	313	0.01%	0.002%
14	3.301	699	703	710	rVB2	187	226	0.01%	0.002%
15	3.793	847	856	892	rBV	102571	300687	10.14%	2.063%
16	4.246	981	997	1032	rBV	218042	568127	19.17%	3.899%
17	4.535	1084	1087	1090	rBV3	274	212	0.01%	0.001%
18	4.664	1123	1127	1131	rBV2	372	359	0.01%	0.002%
19	4.744	1148	1152	1153	rBV2	302	219	0.01%	0.002%
20	4.780	1156	1163	1165	rBV2	291	338	0.01%	0.002%
21	4.953	1201	1217	1262	rBV2	536934	1450932	48.95%	9.956%
22	5.240	1303	1306	1309	rVB2	333	198	0.01%	0.001%
23	5.262	1309	1313	1315	rBV2	341	236	0.01%	0.002%
24	5.339	1334	1337	1340	rVB3	467	287	0.01%	0.002%
25	5.358	1340	1343	1350	rVB3	646	595	0.02%	0.004%
26	5.532	1385	1397	1433	rBV	353493	739904	24.96%	5.077%
27	5.831	1479	1490	1491	rBV2	10327	11274	0.38%	0.077%
28	5.908	1511	1514	1519	rVB4	448	318	0.01%	0.002%
29	5.985	1525	1538	1573	rBV	306909	638366	21.54%	4.381%
30	6.137	1581	1585	1586	rBV3	577	411	0.01%	0.003%
31	6.204	1604	1606	1609	rBV3	364	287	0.01%	0.002%
32	6.239	1614	1617	1620	rVB2	372	208	0.01%	0.001%
33	6.256	1620	1622	1626	rVB2	354	232	0.01%	0.002%
34	6.281	1626	1630	1634	rBV3	460	340	0.01%	0.002%
35	6.304	1634	1637	1642	rVB3	214	187	0.01%	0.001%
36	6.394	1660	1665	1666	rBV2	311	212	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034799.D
 Acq On : 21 Mar 2024 19:33
 Operator : SY/MD
 Sample : P1757-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.497	1692	1697	1701	rBV2	429	567	0.02%	0.004%
38	6.641	1739	1742	1745	rBV2	290	208	0.01%	0.001%
39	6.667	1747	1750	1755	rVB2	395	269	0.01%	0.002%
40	6.911	1816	1826	1868	rBV	169965	324915	10.96%	2.230%
41	7.127	1891	1893	1898	rVB3	314	220	0.01%	0.002%
42	7.153	1898	1901	1903	rBV3	335	235	0.01%	0.002%
43	7.194	1911	1914	1917	rBV	290	226	0.01%	0.002%
44	7.243	1917	1929	1957	rBV	615106	1095896	36.97%	7.520%
45	7.555	2016	2026	2050	rBV	117101	212563	7.17%	1.459%
46	7.780	2094	2096	2104	rVB3	496	544	0.02%	0.004%
47	7.815	2104	2107	2112	rBV2	461	372	0.01%	0.003%
48	8.024	2164	2172	2205	rBV	324234	644035	21.73%	4.419%
49	8.278	2249	2251	2256	rVB2	755	485	0.02%	0.003%
50	8.371	2277	2280	2284	rVB3	707	538	0.02%	0.004%
51	8.487	2312	2316	2321	rVB3	314	364	0.01%	0.002%
52	8.606	2349	2353	2356	rVB3	306	226	0.01%	0.002%
53	8.625	2356	2359	2364	rVB2	303	253	0.01%	0.002%
54	8.783	2397	2408	2413	rBV	578803	929592	31.36%	6.379%
55	9.098	2501	2506	2509	rBV4	754	655	0.02%	0.004%
56	9.185	2530	2533	2538	rVB2	212	204	0.01%	0.001%
57	9.435	2602	2611	2613	rBV2	248	320	0.01%	0.002%
58	9.490	2624	2628	2629	rBV	316	210	0.01%	0.001%
59	9.612	2663	2666	2669	rVB	307	214	0.01%	0.001%
60	9.873	2744	2747	2750	rBV	335	252	0.01%	0.002%
61	9.889	2750	2752	2760	rVB2	452	411	0.01%	0.003%
62	10.153	2822	2834	2866	rVV	407861	647629	21.85%	4.444%
63	10.265	2866	2869	2871	rBV4	434	220	0.01%	0.002%
64	10.316	2882	2885	2894	rVB4	636	825	0.03%	0.006%
65	10.484	2934	2937	2940	rBV2	553	384	0.01%	0.003%
66	10.734	3013	3015	3021	rVB2	270	246	0.01%	0.002%
67	10.821	3037	3042	3044	rBV2	264	236	0.01%	0.002%
68	10.857	3050	3053	3054	rBV2	408	242	0.01%	0.002%
69	11.117	3123	3134	3145	rBV	270715	424717	14.33%	2.914%
70	11.204	3145	3161	3183	rVB2	1136595	2594545	87.53%	17.804%
71	11.516	3255	3258	3260	rBV2	305	200	0.01%	0.001%
72	11.574	3260	3276	3305	rBV2	1394589	2964108	100.00%	20.340%
73	11.763	3329	3335	3340	rBV5	349	462	0.02%	0.003%
74	11.947	3388	3392	3398	rBV5	453	476	0.02%	0.003%
75	12.191	3462	3468	3469	rBV2	671	565	0.02%	0.004%
76	12.201	3469	3471	3478	rVB2	884	627	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034799.D
 Acq On : 21 Mar 2024 19:33
 Operator : SY/MD
 Sample : P1757-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.358	3517	3520	3523	rVB2	629	377	0.01%	0.003%
78	12.455	3545	3550	3552	rBV	243	203	0.01%	0.001%
79	12.519	3566	3570	3573	rBV2	507	361	0.01%	0.002%
80	12.586	3588	3591	3593	rBV2	412	332	0.01%	0.002%
81	12.763	3641	3646	3649	rBV	256	229	0.01%	0.002%
82	13.085	3742	3746	3748	rBV2	498	326	0.01%	0.002%
83	13.201	3772	3782	3798	rBV	83366	132548	4.47%	0.910%
84	13.307	3812	3815	3817	rBV	363	213	0.01%	0.001%
85	13.451	3853	3860	3874	rVB	3853	6176	0.21%	0.042%
86	13.683	3921	3932	3951	rVB3	33320	54378	1.83%	0.373%
87	13.757	3952	3955	3958	rBV3	312	207	0.01%	0.001%
88	13.834	3976	3979	3983	rVV2	434	366	0.01%	0.003%
89	13.988	4021	4027	4029	rBV	799	781	0.03%	0.005%
90	14.030	4036	4040	4042	rBV2	368	299	0.01%	0.002%
91	14.207	4092	4095	4097	rBV2	369	245	0.01%	0.002%
92	14.377	4147	4148	4154	rVB3	586	406	0.01%	0.003%
93	14.403	4154	4156	4159	rBV	345	263	0.01%	0.002%
94	14.435	4164	4166	4169	rVB2	335	197	0.01%	0.001%
95	14.738	4259	4260	4263	rBV3	386	227	0.01%	0.002%
96	14.866	4298	4300	4304	rBV3	408	220	0.01%	0.002%
97	15.159	4389	4391	4392	rBV	578	270	0.01%	0.002%
98	15.303	4434	4436	4439	rBV2	547	440	0.01%	0.003%
99	15.348	4448	4450	4456	rBV3	764	560	0.02%	0.004%
100	15.377	4457	4459	4460	rBV	684	302	0.01%	0.002%




Sum of corrected areas: 14572746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034799.D
Acq On : 21 Mar 2024 19:33
Operator : SY/MD
Sample : P1757-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

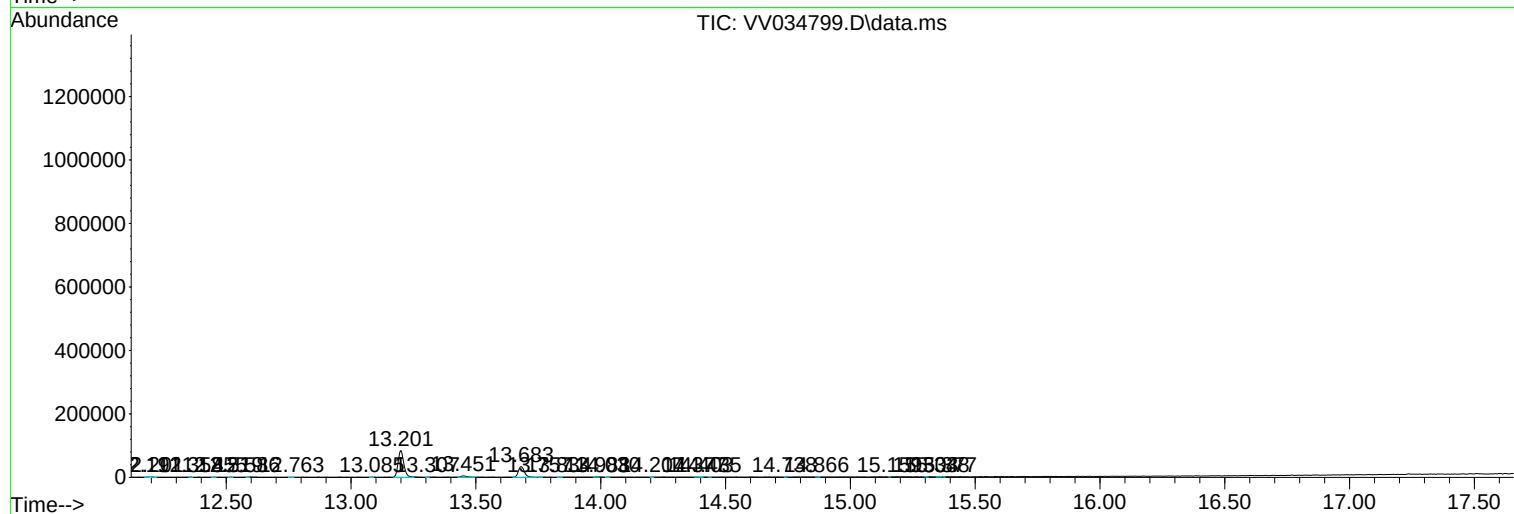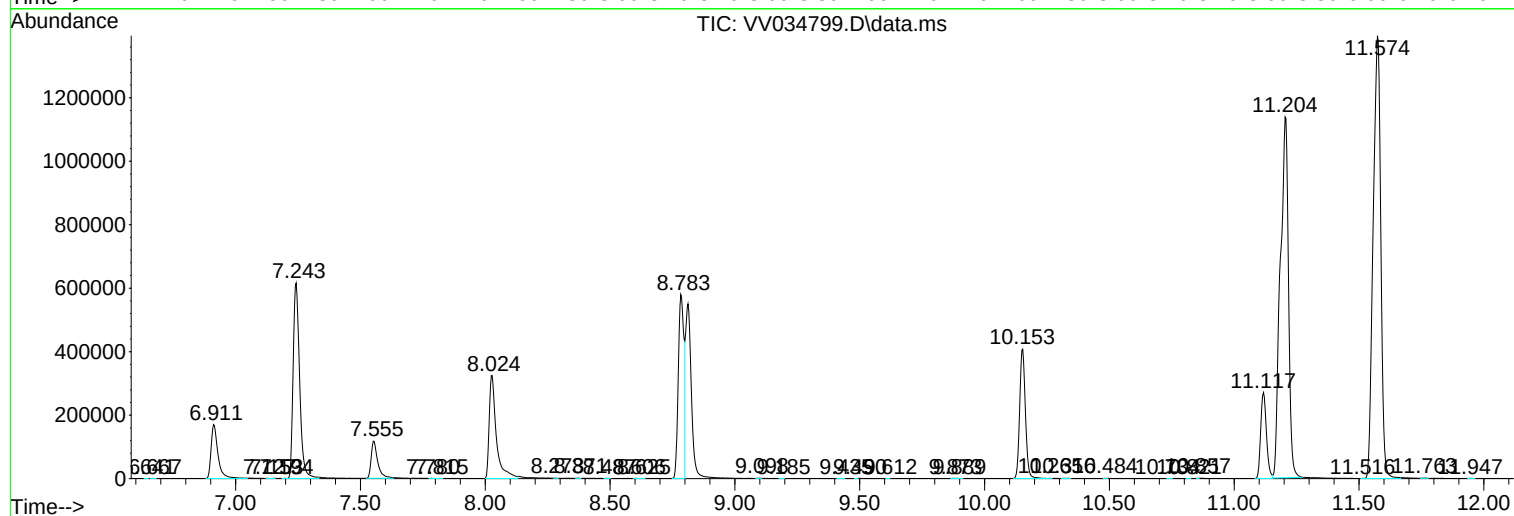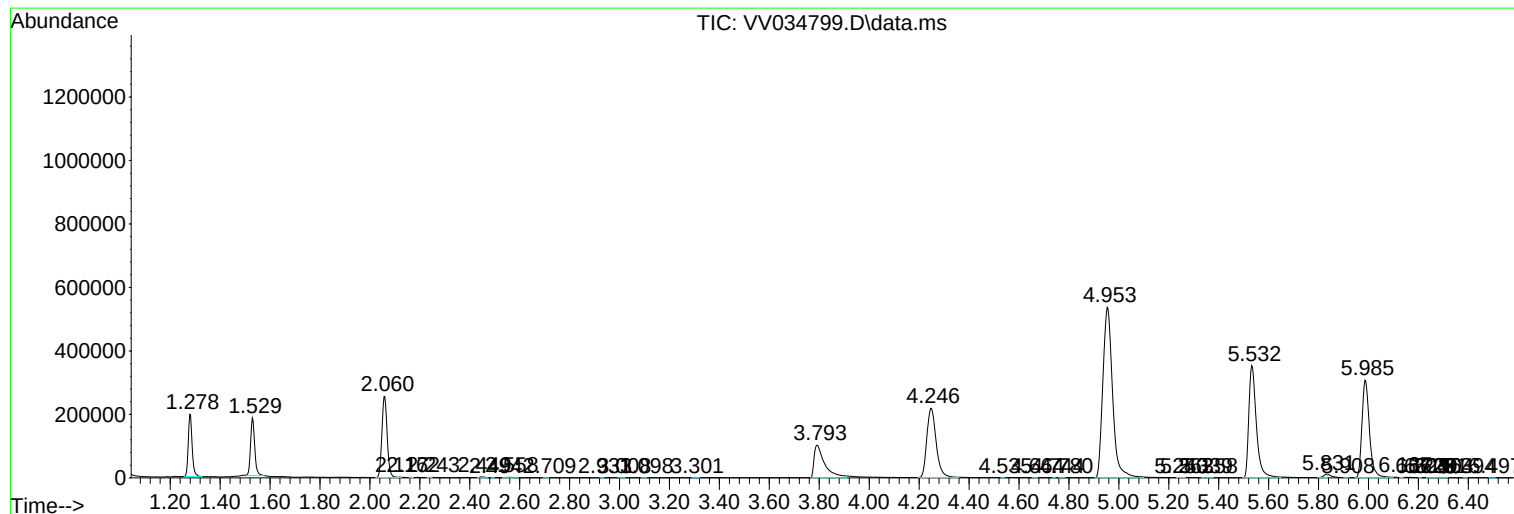

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034799.D
Acq On : 21 Mar 2024 19:33
Operator : SY/MD
Sample : P1757-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034799.D
Acq On : 21 Mar 2024 19:33
Operator : SY/MD
Sample : P1757-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc