

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034800.D
 Acq On : 21 Mar 2024 19:57
 Operator : SY/MD
 Sample : P1757-02DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	213351	229446	9.17%	1.829%
2	1.529	146	152	172	rVB	190169	227141	9.08%	1.810%
3	2.060	306	317	335	rBV	289910	429956	17.18%	3.426%
4	2.449	431	438	447	rVB4	2305	3781	0.15%	0.030%
5	2.558	464	472	482	rVB4	1405	2467	0.10%	0.020%
6	2.600	482	485	487	rBV2	263	154	0.01%	0.001%
7	2.777	537	540	541	rBV	277	168	0.01%	0.001%
8	2.934	587	589	590	rBV	160	76	0.00%	0.001%
9	3.076	630	633	634	rBV	146	85	0.00%	0.001%
10	3.111	642	644	646	rBV	197	87	0.00%	0.001%
11	3.230	679	681	683	rBV2	199	119	0.00%	0.001%
12	3.381	726	728	737	rVB2	318	316	0.01%	0.003%
13	3.436	737	745	750	rBV2	245	392	0.02%	0.003%
14	3.465	750	754	755	rVB2	250	127	0.01%	0.001%
15	3.478	755	758	760	rBV	127	95	0.00%	0.001%
16	3.564	780	785	792	rVB2	296	302	0.01%	0.002%
17	3.600	792	796	799	rBV	164	172	0.01%	0.001%
18	3.661	812	815	818	rBV2	316	190	0.01%	0.002%
19	3.693	822	825	828	rBV2	286	213	0.01%	0.002%
20	3.789	847	855	905	rBV	102365	313421	12.52%	2.498%
21	4.246	982	997	1025	rBV	225694	580791	23.21%	4.629%
22	4.616	1109	1112	1116	rVB2	405	221	0.01%	0.002%
23	4.638	1116	1119	1121	rBV2	278	220	0.01%	0.002%
24	4.686	1131	1134	1138	rBV3	294	269	0.01%	0.002%
25	4.744	1150	1152	1155	rVV2	366	234	0.01%	0.002%
26	4.844	1179	1183	1185	rBV2	264	263	0.01%	0.002%
27	4.953	1202	1217	1256	rBV2	543437	1556061	62.18%	12.401%
28	5.449	1368	1371	1375	rVB2	401	282	0.01%	0.002%
29	5.532	1386	1397	1432	rBV	380539	787768	31.48%	6.278%
30	5.834	1480	1491	1510	rBV3	10613	23771	0.95%	0.189%
31	5.985	1526	1538	1572	rBV	310179	647717	25.88%	5.162%
32	6.284	1628	1631	1632	rBV	249	150	0.01%	0.001%
33	6.333	1642	1646	1648	rBV2	190	149	0.01%	0.001%
34	6.426	1671	1675	1680	rVB2	246	225	0.01%	0.002%
35	6.455	1680	1684	1688	rBV2	365	344	0.01%	0.003%
36	6.503	1697	1699	1704	rVB	420	291	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034800.D
 Acq On : 21 Mar 2024 19:57
 Operator : SY/MD
 Sample : P1757-02DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.539	1704	1710	1713	rBV2	263	287	0.01%	0.002%
38	6.558	1713	1716	1720	rBV2	161	121	0.00%	0.001%
39	6.587	1720	1725	1729	rBV	265	271	0.01%	0.002%
40	6.866	1810	1812	1815	rBV	177	66	0.00%	0.001%
41	6.911	1815	1826	1854	rBV	169428	322147	12.87%	2.567%
42	7.243	1918	1929	1957	rBV	627964	1114108	44.52%	8.879%
43	7.551	2016	2025	2049	rBV	117525	211934	8.47%	1.689%
44	7.831	2110	2112	2116	rVB2	396	173	0.01%	0.001%
45	7.850	2116	2118	2119	rBV2	290	127	0.01%	0.001%
46	7.924	2139	2141	2142	rBV2	211	66	0.00%	0.001%
47	7.940	2142	2146	2148	rVB2	324	191	0.01%	0.002%
48	8.024	2161	2172	2220	rBV	322257	655671	26.20%	5.225%
49	8.551	2332	2336	2338	rBV2	382	308	0.01%	0.002%
50	8.612	2352	2355	2359	rVB2	211	175	0.01%	0.001%
51	8.632	2359	2361	2366	rBV3	354	287	0.01%	0.002%
52	8.661	2366	2370	2372	rBV2	190	166	0.01%	0.001%
53	8.690	2376	2379	2381	rBV	355	163	0.01%	0.001%
54	8.712	2381	2386	2389	rVB3	257	272	0.01%	0.002%
55	8.735	2389	2393	2396	rBV2	385	309	0.01%	0.002%
56	8.783	2397	2408	2415	rBV	597172	1023611	40.91%	8.158%
57	9.075	2496	2499	2501	rBV2	527	302	0.01%	0.002%
58	9.130	2513	2516	2520	rBV3	250	197	0.01%	0.002%
59	9.201	2535	2538	2540	rBV2	235	112	0.00%	0.001%
60	9.249	2551	2553	2555	rBV	145	88	0.00%	0.001%
61	9.336	2578	2580	2581	rBV	195	98	0.00%	0.001%
62	9.497	2624	2630	2635	rVB3	628	762	0.03%	0.006%
63	9.529	2635	2640	2641	rBV2	358	229	0.01%	0.002%
64	9.558	2647	2649	2653	rVB2	264	135	0.01%	0.001%
65	9.574	2653	2654	2658	rBV	163	108	0.00%	0.001%
66	9.802	2722	2725	2727	rBV2	279	156	0.01%	0.001%
67	9.886	2744	2751	2760	rVB4	692	1154	0.05%	0.009%
68	9.927	2760	2764	2770	rVB2	222	256	0.01%	0.002%
69	10.030	2793	2796	2801	rBV2	209	208	0.01%	0.002%
70	10.072	2806	2809	2813	rBV2	198	146	0.01%	0.001%
71	10.153	2822	2834	2855	rBV	414161	657438	26.27%	5.239%
72	10.300	2877	2880	2882	rBV2	315	205	0.01%	0.002%
73	10.432	2915	2921	2922	rBV	333	268	0.01%	0.002%
74	10.477	2931	2935	2939	rBV3	324	275	0.01%	0.002%
75	10.641	2984	2986	2992	rBV2	200	192	0.01%	0.002%
76	10.760	3022	3023	3026	rBV	151	79	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
 Data File : VV034800.D
 Acq On : 21 Mar 2024 19:57
 Operator : SY/MD
 Sample : P1757-02DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.786	3029	3031	3032	rBV	204	70	0.00%	0.001%
78	10.863	3052	3055	3059	rVB2	628	428	0.02%	0.003%
79	10.976	3088	3090	3091	rBV	185	65	0.00%	0.001%
80	11.117	3124	3134	3145	rBV	179467	276295	11.04%	2.202%
81	11.188	3146	3156	3157	rBV	652413	775603	30.99%	6.181%
82	11.574	3259	3276	3301	rBV2	1116263	2502364	100.00%	19.942%
83	11.799	3343	3346	3348	rBV2	358	174	0.01%	0.001%
84	11.815	3348	3351	3355	rBV3	840	643	0.03%	0.005%
85	11.931	3385	3387	3390	rBV2	220	102	0.00%	0.001%
86	12.059	3424	3427	3430	rBV	390	279	0.01%	0.002%
87	12.159	3455	3458	3460	rVB2	387	196	0.01%	0.002%
88	12.191	3463	3468	3478	rVB4	1031	1526	0.06%	0.012%
89	12.239	3478	3483	3485	rBV2	418	386	0.02%	0.003%
90	12.320	3507	3508	3511	rVB	173	65	0.00%	0.001%
91	12.358	3513	3520	3523	rBV2	558	670	0.03%	0.005%
92	12.439	3542	3545	3546	rBV	236	153	0.01%	0.001%
93	12.586	3589	3591	3598	rVB4	740	797	0.03%	0.006%
94	12.683	3618	3621	3623	rBV	235	130	0.01%	0.001%
95	12.696	3623	3625	3628	rBV2	356	233	0.01%	0.002%
96	13.201	3771	3782	3800	rBV	78735	126362	5.05%	1.007%
97	13.451	3856	3860	3872	rVB3	2799	3759	0.15%	0.030%
98	13.512	3877	3879	3883	rVB3	457	253	0.01%	0.002%
99	13.683	3922	3932	3944	rBV2	35503	56754	2.27%	0.452%
100	14.066	4048	4051	4054	rBV3	550	423	0.02%	0.003%




Sum of corrected areas: 12548055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034800.D
Acq On : 21 Mar 2024 19:57
Operator : SY/MD
Sample : P1757-02DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

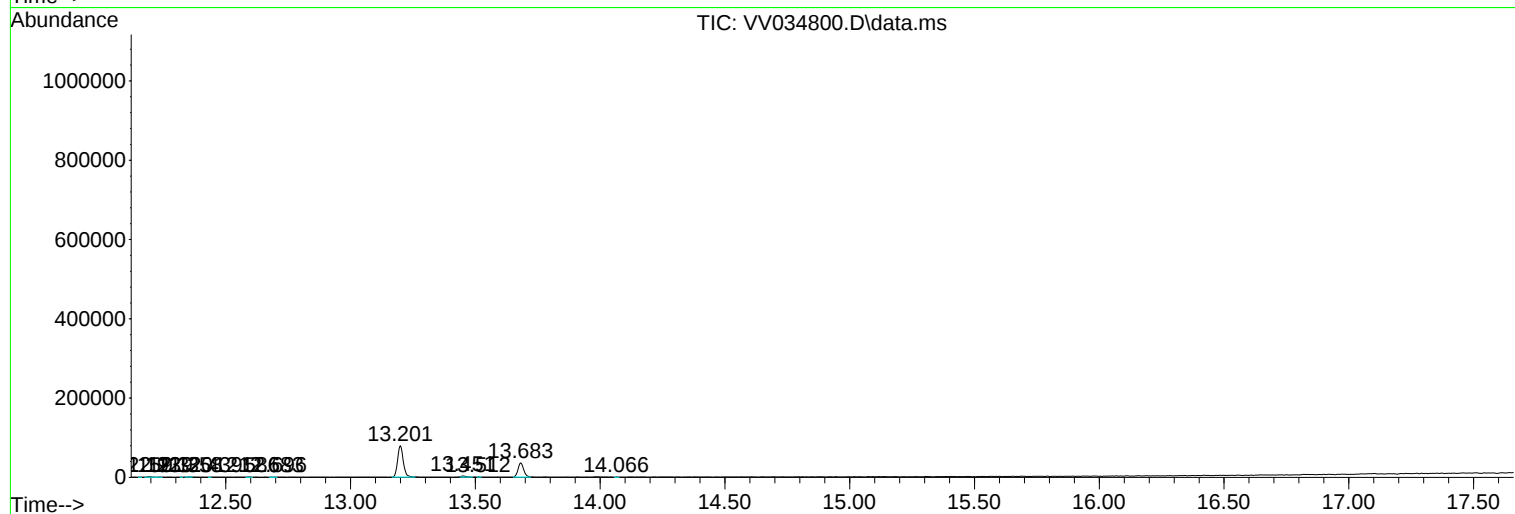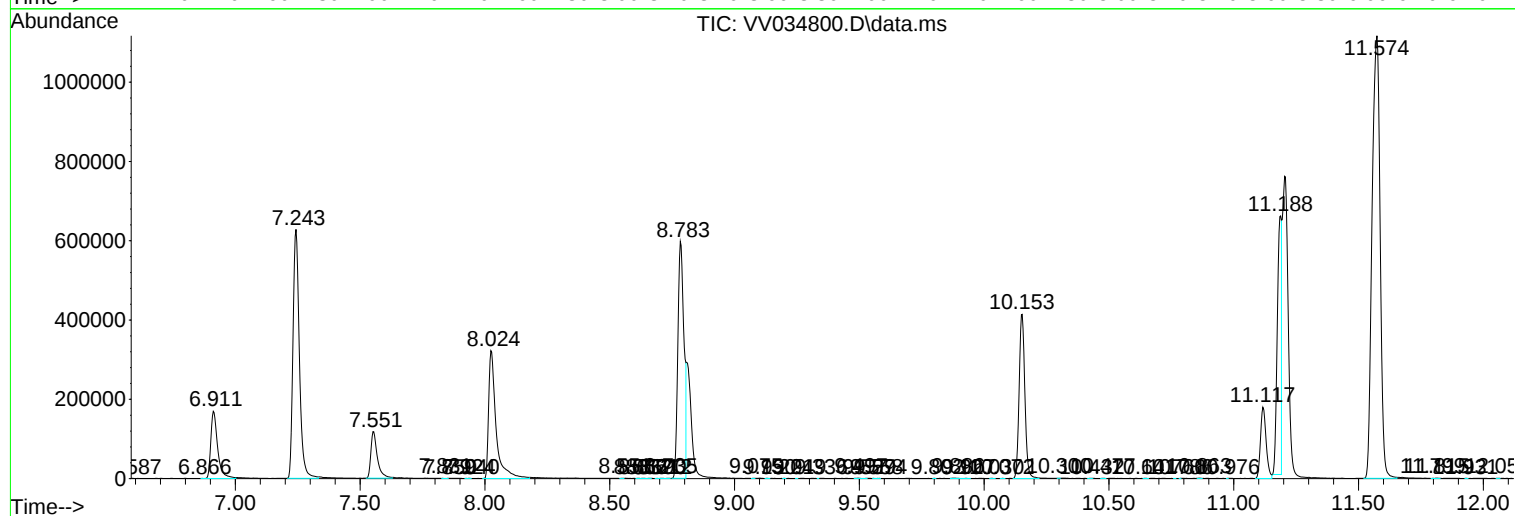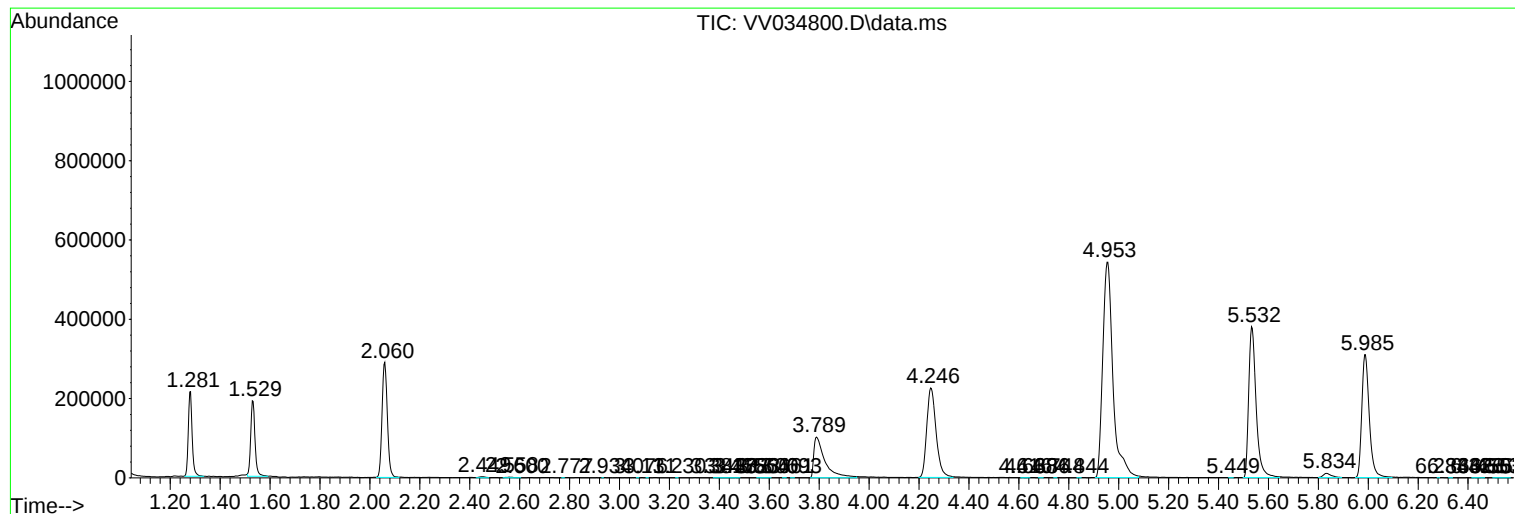

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034800.D
Acq On : 21 Mar 2024 19:57
Operator : SY/MD
Sample : P1757-02DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032124\
Data File : VV034800.D
Acq On : 21 Mar 2024 19:57
Operator : SY/MD
Sample : P1757-02DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc