

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032219\
 Data File : VV009837.D
 Acq On : 22 Mar 2019 19:25
 Operator : SY/MD
 Sample : K2052-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P019-TW001-01

Quant Time: Mar 23 05:04:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 23 03:53:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	87599	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88533	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	38976	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48940	4.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.40%
7) Chloroethane-d5	1.59	69	50289	5.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.20%
11) 1,1-Dichloroethene-d2	2.13	63	97155	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	3.96	46	65772	53.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.36%
24) Chloroform-d	4.41	84	53979	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.09	65	29538	5.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.00%
32) Benzene-d6	5.10	84	115561	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	35337	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.36	98	100139	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.67	79	10937	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.14	63	52557	48.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	25375	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	37817	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	7331	0.555 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032219\
Data File : VV009837.D
Acq On : 22 Mar 2019 19:25
Operator : SY/MD
Sample : K2052-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P019-TW001-01

Quant Time: Mar 23 05:04:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 23 03:53:22 2019
Response via : Initial Calibration

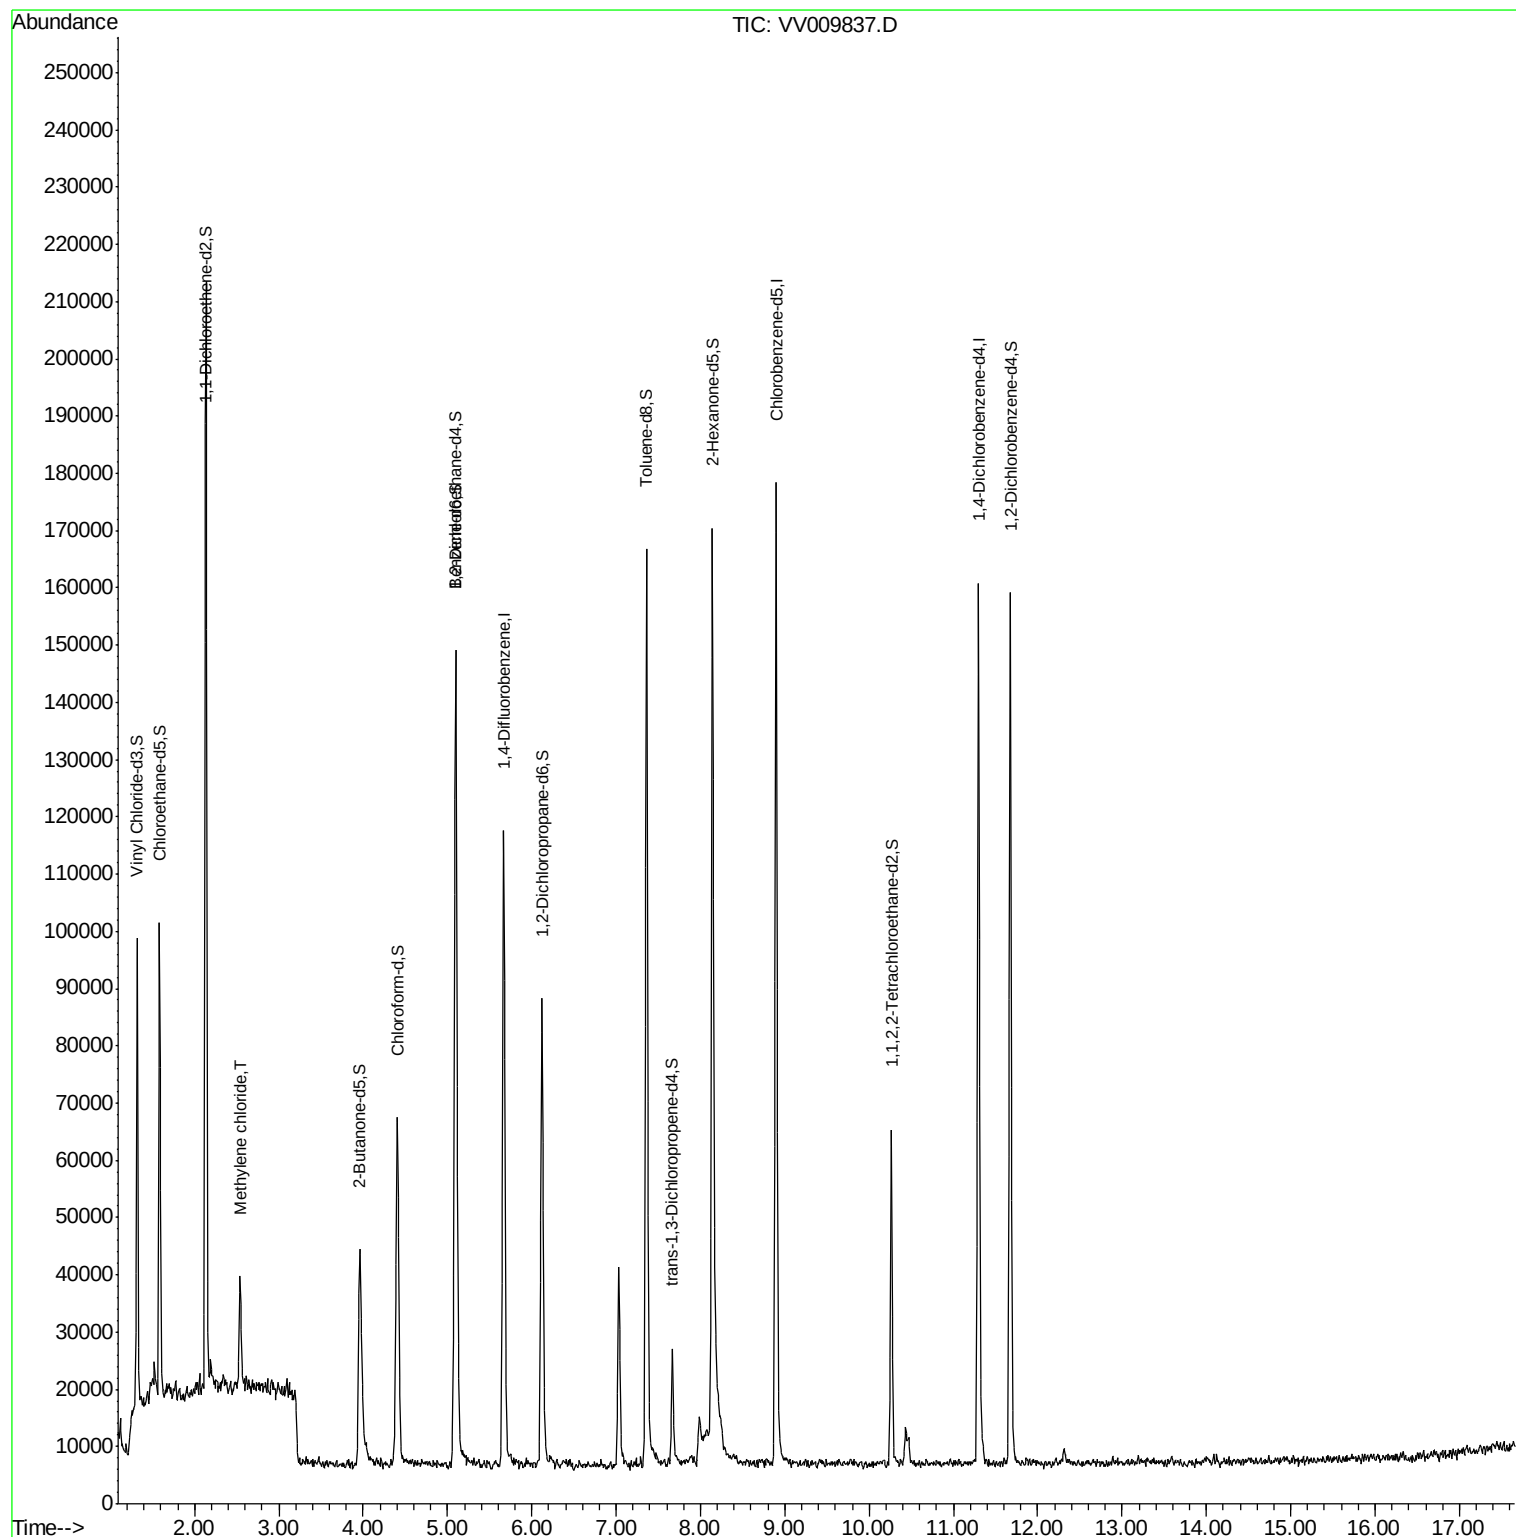

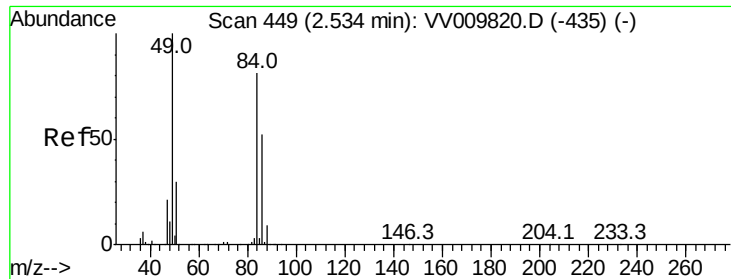

#16
 Methylene chloride
 Concen: 0.555 ug/L
 RT: 2.54 min Scan# 451
 Delta R.T. 0.01 min
 Lab File: VV009837.D
 Acq: 22 Mar 2019 19:25

Instrument :
 MSVOA_V
 ClientSampleId :
 P019-TW001-01

Tot Ion: 84 Resp: 7331
 Ion Ratio Lower Upper
 84 100
 86 64.7 46.1 85.5
 49 135.0 89.7 166.5

