


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032219\
 Data File : VV009819.D
 Acq On : 22 Mar 2019 10:49
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 23 21:59:27 2019

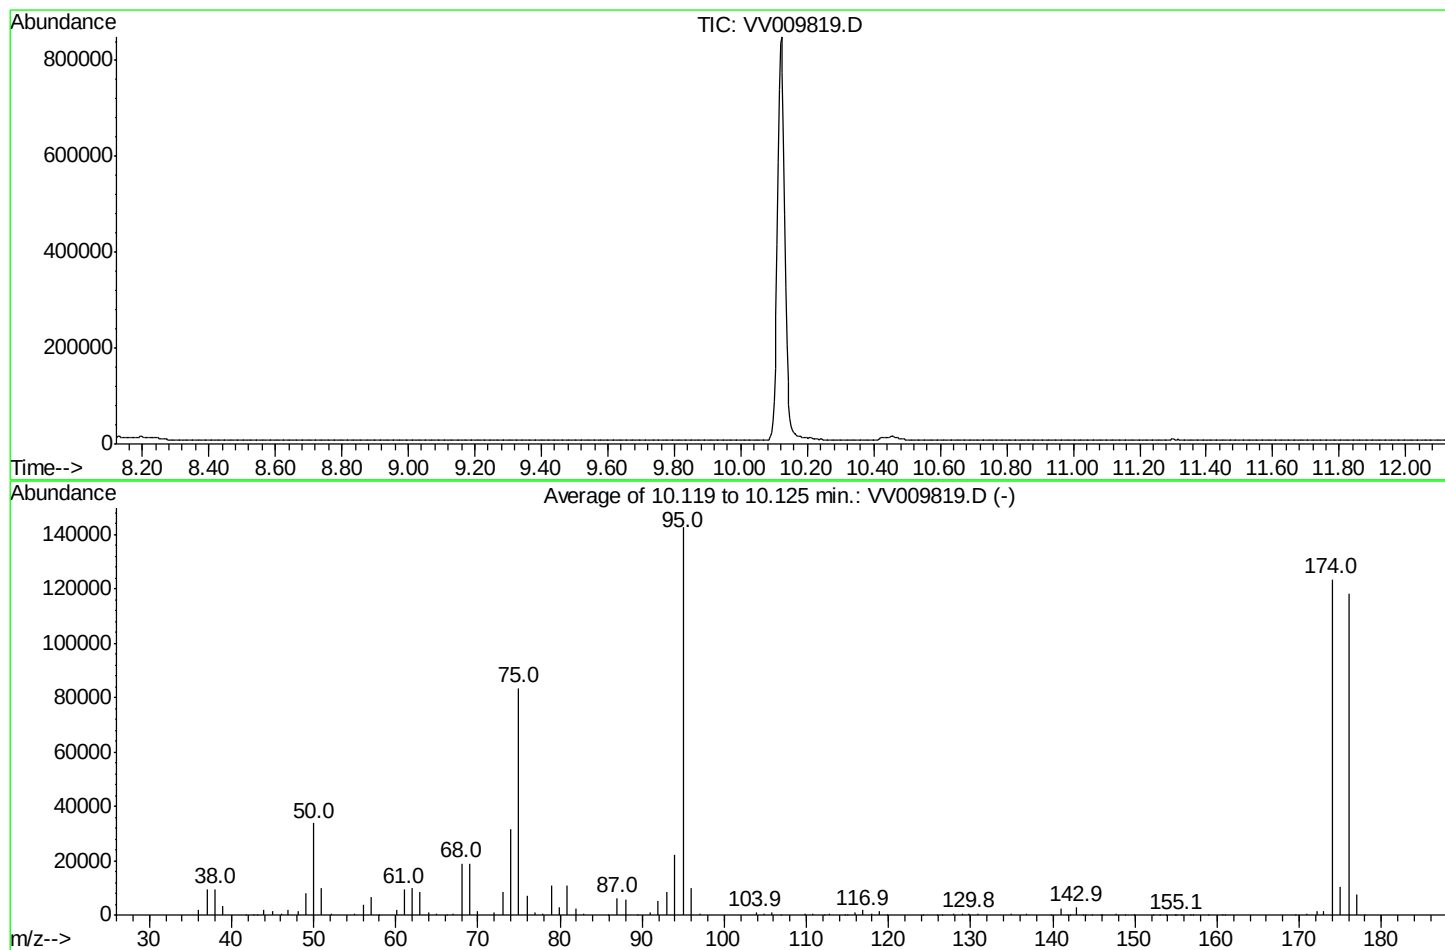

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	33720	PASS
75	95	30	80	58.6	83576	PASS
95	95	100	100	100.0	142677	PASS
96	95	5	9	6.9	9911	PASS
173	174	0.00	2	1.3	1624	PASS
174	95	50	120	86.6	123554	PASS
175	174	5	9	8.3	10283	PASS
176	174	95	101	95.7	118216	PASS
177	176	5	9	6.3	7496	PASS

Scan 2795 (10.077 min): VV009819.D
BFB32

m/z	Abundance
36.50	112.0
38.80	105.0
40.00	7611.0
40.90	101.0
43.90	343.0
94.40	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1924.0
37.00	9690.0
38.00	9630.0
39.00	3889.0
40.00	7317.0
41.00	109.0
42.70	125.0
43.10	101.0
44.00	2245.0
45.00	1774.0
46.10	335.0
47.00	2080.0
48.10	1245.0
49.00	8366.0
50.00	35928.0
51.00	10482.0
52.10	444.0
54.90	701.0
56.00	4141.0
57.00	6819.0
57.90	234.0
60.00	1786.0
61.00	9644.0
62.00	10218.0
63.00	9348.0
64.00	799.0
64.90	421.0
66.20	233.0
67.00	382.0
68.00	19888.0
69.00	18928.0
70.00	1503.0
72.00	1225.0
73.00	8801.0
74.00	33232.0
75.00	86424.0
76.00	7604.0
76.90	1040.0
77.90	437.0
78.90	11399.0
79.90	3186.0
80.90	11598.0
81.90	2331.0
82.90	480.0
85.90	192.0
86.90	6766.0
87.90	6181.0
89.40	111.0
91.00	867.0
92.00	5147.0
93.00	8881.0
94.00	22960.0
95.00	144896.0
96.00	10426.0
97.00	378.0
103.90	1230.0
104.80	278.0
105.80	1022.0
106.90	148.0
109.80	275.0
110.70	396.0
112.10	251.0
112.80	295.0
115.00	227.0
115.90	959.0
116.90	1821.0
117.90	809.0
118.90	1289.0
124.20	128.0
125.80	123.0
128.00	541.0
128.90	403.0
129.90	576.0
130.80	325.0
134.90	250.0
136.80	438.0
139.70	212.0
141.00	2566.0
142.00	356.0
142.90	2735.0
144.00	201.0
144.80	219.0
146.10	272.0
147.70	463.0
148.80	140.0
149.90	185.0
152.20	109.0
152.90	177.0
153.80	118.0
154.80	381.0
155.60	113.0
156.80	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

158.90	187.0
160.70	261.0
169.50	155.0
170.90	343.0
172.10	1315.0
174.00	122328.0
175.00	10017.0
176.00	118120.0
176.90	7705.0
177.90	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1979.0
37.00	9570.0
38.00	9854.0
39.00	3774.0
40.00	7220.0
42.70	101.0
44.00	2136.0
45.00	1729.0
46.10	384.0
46.90	1924.0
48.00	1283.0
49.00	8467.0
50.00	34672.0
51.00	10482.0
52.10	479.0
54.90	710.0
56.00	3834.0
57.00	6899.0
57.90	165.0
60.10	1842.0
61.00	9709.0
62.00	10162.0
63.00	8664.0
64.10	751.0
64.90	524.0
66.20	223.0
66.90	424.0
68.00	19736.0
69.00	19352.0
70.00	1434.0
72.00	1200.0
73.00	8881.0
74.00	32960.0
75.00	86520.0
76.10	7567.0
76.90	1126.0
77.90	446.0
78.90	11328.0
79.90	3042.0
80.90	11363.0
81.90	2289.0
82.90	535.0
85.80	235.0
87.00	6533.0
88.00	5789.0
91.00	929.0
92.00	5308.0
93.00	8942.0
94.00	23120.0
95.00	147712.0
96.00	10243.0
97.00	329.0
103.90	1121.0
104.80	275.0
105.80	999.0
106.80	165.0
109.70	278.0
110.70	371.0
112.10	226.0
112.80	315.0
115.00	234.0
115.90	996.0
116.90	1855.0
117.90	727.0
118.90	1338.0
119.90	104.0
124.10	124.0
128.00	514.0
128.90	418.0
129.90	645.0
130.80	400.0
135.00	357.0
136.80	478.0
139.70	249.0
141.00	2523.0
142.10	385.0
142.90	3063.0
144.00	162.0
144.80	275.0
146.00	232.0
147.80	353.0
148.80	120.0
149.80	211.0
152.90	119.0
153.80	146.0
155.00	332.0
156.80	195.0
159.00	195.0
160.90	301.0
169.50	186.0
170.90	455.0
172.10	1289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

173.00	2456.0
174.00	128088.0
175.00	10657.0
176.00	122512.0
177.00	7759.0
177.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1765.0
37.00	8740.0
38.00	8788.0
39.00	3291.0
39.90	7170.0
41.70	115.0
44.00	1926.0
45.00	1482.0
46.10	384.0
46.90	1822.0
48.00	1164.0
49.00	7517.0
50.00	30560.0
51.00	9408.0
52.10	473.0
55.00	650.0
56.00	3194.0
57.00	5949.0
57.90	138.0
60.00	1777.0
61.00	8949.0
62.00	8898.0
63.00	6961.0
64.10	738.0
64.90	578.0
66.10	158.0
66.80	516.0
68.00	17512.0
69.00	17880.0
70.00	1195.0
72.00	1086.0
73.00	8014.0
74.00	29008.0
75.00	77784.0
76.10	6743.0
77.00	1127.0
77.90	580.0
78.90	10038.0
79.90	2625.0
80.90	10190.0
81.90	2042.0
82.90	518.0
85.70	276.0
87.00	5787.0
88.00	5166.0
91.00	880.0
91.90	5168.0
93.00	7982.0
94.00	20736.0
95.00	135424.0
96.00	9064.0
97.00	248.0
103.90	981.0
104.90	259.0
105.80	885.0
106.80	214.0
109.70	245.0
110.80	319.0
112.10	147.0
112.80	289.0
114.60	108.0
115.00	177.0
115.80	960.0
116.90	1552.0
117.90	644.0
118.90	1121.0
119.80	131.0
126.50	101.0
127.80	514.0
129.00	350.0
129.80	616.0
130.80	414.0
135.00	466.0
136.80	463.0
139.70	242.0
141.00	2221.0
141.80	289.0
142.90	2866.0
143.70	169.0
144.80	235.0
145.80	250.0
147.80	312.0
149.80	243.0
153.00	106.0
153.80	141.0
155.10	355.0
157.00	245.0
159.00	216.0
160.90	303.0
169.50	186.0
170.90	457.0
172.10	1184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

173.00	2416.0
174.00	120248.0
175.00	10176.0
176.00	114016.0
177.00	7024.0
177.90	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32