

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032221\
 Data File : VW020707.D
 Acq On : 22 Mar 2021 17:39
 Operator : SY/MD
 Sample : M1698-15ME
 Misc : 5.34g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4L3ME

Quant Time: Mar 23 02:16:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 23 02:12:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	465056	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	464509	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.259	152	217286	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	156677	41.77	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.54%		
7) Chloroethane-d5	1.568	69	82703	27.56	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	55.12%#		
11) 1,1-Dichloroethene-d2	2.082	63	227578	31.92	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.84%		
21) 2-Butanone-d5	3.908	46	149577	62.13	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	62.13%		
24) Chloroform-d	4.349	84	284928	43.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.40%		
26) 1,2-Dichloroethane-d4	5.034	65	198128	46.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.10%		
32) Benzene-d6	5.047	84	555929	43.32	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.64%		
36) 1,2-Dichloropropane-d6	6.072	67	175949	42.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.70%		
41) Toluene-d8	7.317	98	493812	43.29	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.58%		
43) trans-1,3-Dichloroprop...	7.625	79	81272	42.35	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.70%		
47) 2-Hexanone-d5	7.940	63	152	0.10	ug/L	-0.15
Spiked Amount 100.000	Range 45 - 130		Recovery =	0.10%#		
57) 1,1,2,2-Tetrachloroeth...	10.230	84	235492	45.89	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.78%		
64) 1,2-Dichlorobenzene-d4	11.635	152	196677	46.71	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.42%		
Target Compounds						
46) Tetrachloroethene	7.976	164	239005	94.20	ug/L	97
48) 2-Hexanone	8.107	43	7811	1.82	ug/L #	45
59) 1,2,3-Trichloropropane	11.259	75	29104	6.28	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020707.D
Acq On : 22 Mar 2021 17:39
Operator : SY/MD
Sample : M1698-15ME
Misc : 5.34g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4L3ME

Quant Time: Mar 23 02:16:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 23 02:12:43 2021
Response via : Initial Calibration

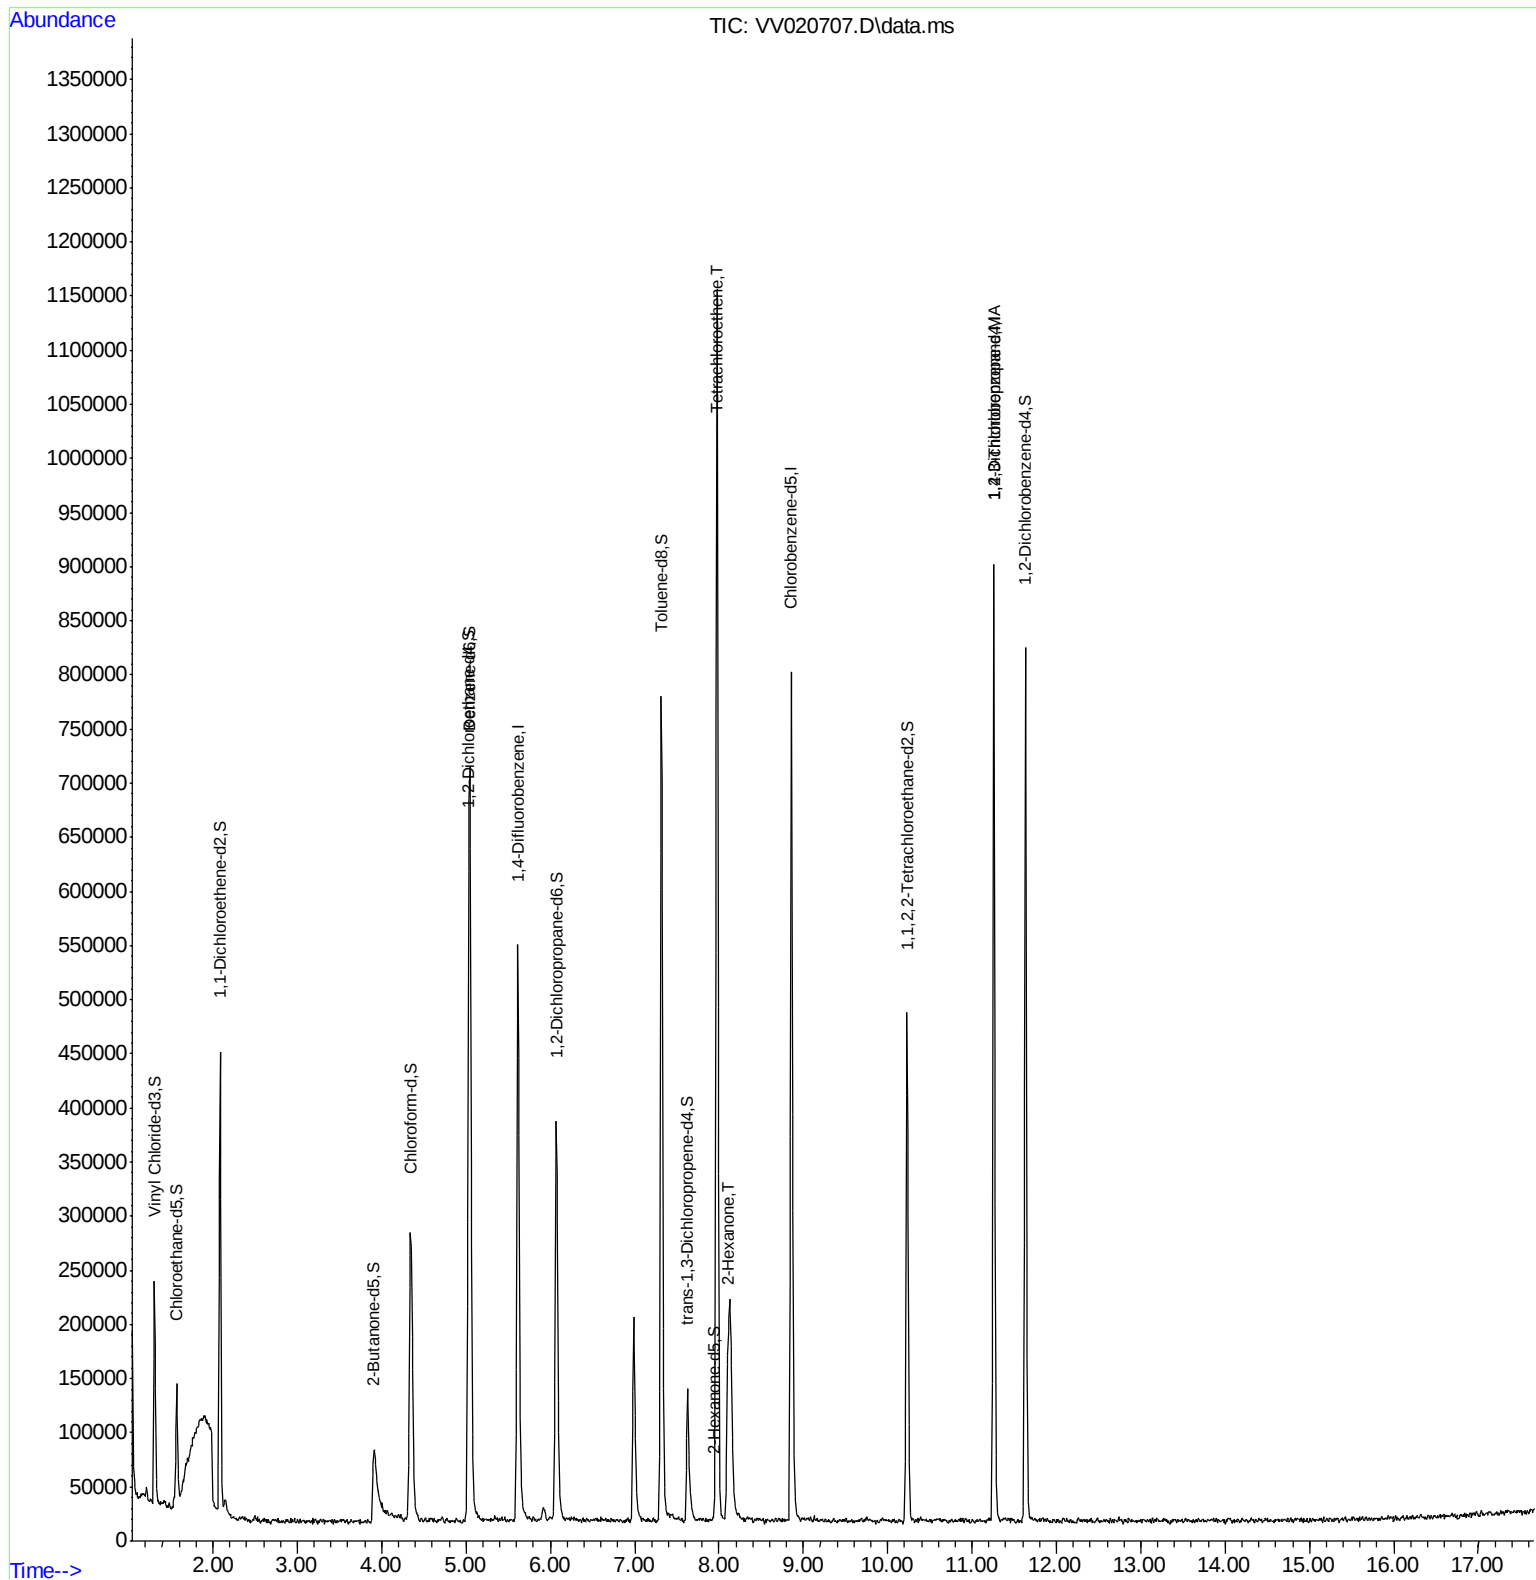




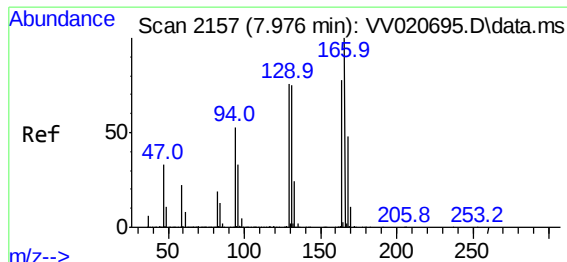


#46
Tetrachloroethene
Concen: 94.20 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. -0.000 min
Lab File: VV020707.D
Acq: 22 Mar 2021 17:39

Instrument :
MSVOA_V
ClientSampleId :
BG4L3ME

Tgt Ion:164 Resp: 239005




Ion	Ratio	Lower	Upper
164	100		
129	95.6	70.6	131.0
131	91.7	66.8	124.0
166	124.5	88.2	163.8

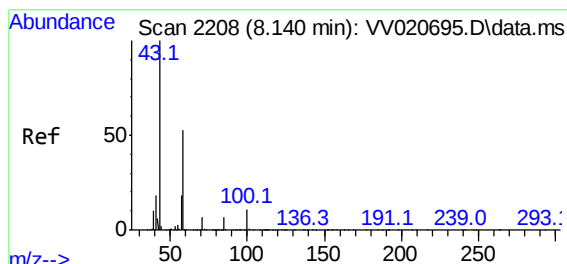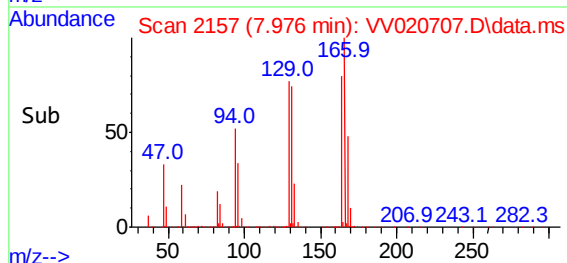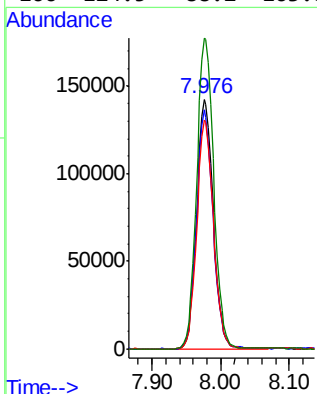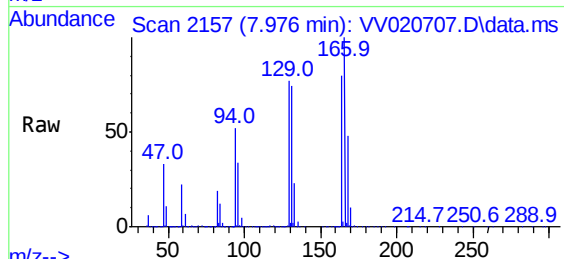


#48
2-Hexanone
Concen: 1.82 ug/L
RT: 8.107 min Scan# 2198
Delta R.T. -0.032 min
Lab File: VV020707.D
Acq: 22 Mar 2021 17:39

Tgt Ion: 43 Resp: 7811


Ion	Ratio	Lower	Upper
43	100		
58	5.8	41.8	62.6#
57	0.0	15.0	22.4#
100	0.0	8.9	13.3#

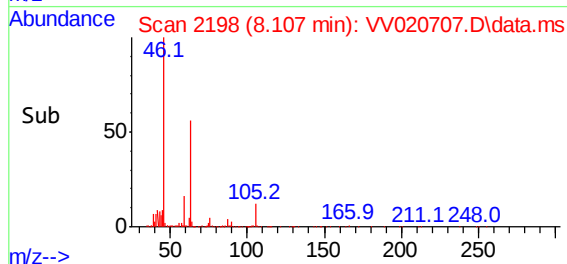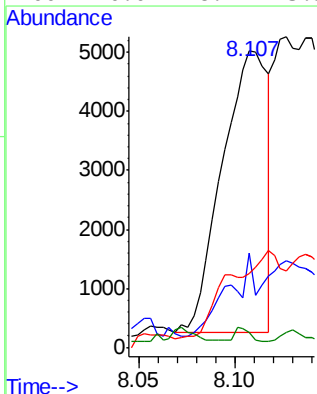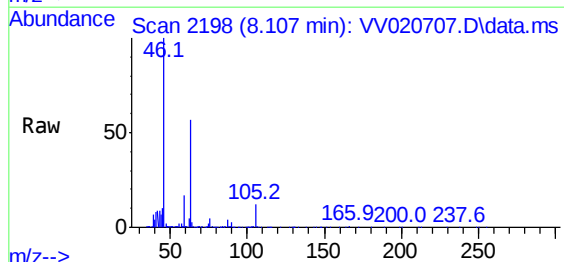

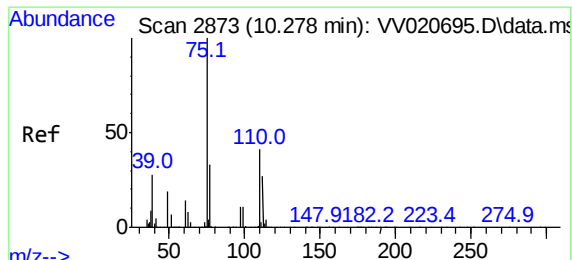

#59
 1,2,3-Trichloropropane
 Concen: 6.28 ug/L
 RT: 11.259 min Scan# 3178
 Delta R.T. 0.981 min
 Lab File: VV020707.D
 Acq: 22 Mar 2021 17:39

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4L3ME

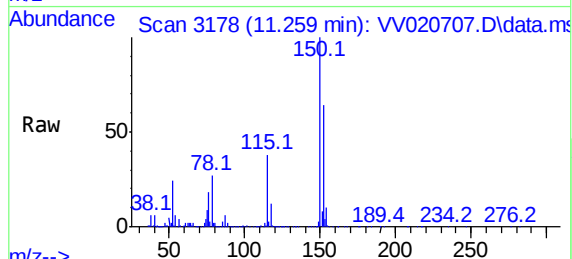

Tgt Ion: 75 Resp: 29104
 Ion Ratio Lower Upper
 75 100
 77 35.6 25.4 38.0

